

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030420\
 Data File : BP002057.D
 Acq On : 04 Mar 2020 19:08
 Operator : CG/JU
 Sample : L1677-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC1

Quant Time: Mar 05 06:23:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	294867	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1226909	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	764063	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1666020	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1659340	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1844867	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	32416	4.73	ng/uL	0.00
5) Phenol-d5	6.82	99	590132	26.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	338222	28.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	530255	27.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	500116	27.06	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	253562	26.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	275596	25.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	541367	26.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	729291	32.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1606580	27.78	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1978971	28.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	193706	17.52	ng/ul	0.00
58) Fluorene-d10	15.27	176	1449560	28.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	149311	16.26	ng/ul	0.00
71) Anthracene-d10	17.13	188	2154452	28.77	ng/ul	0.00
79) Pyrene-d10	19.37	212	2510825	28.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2753748	29.17	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.73	163	433341	7.260	ng/ul 100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030420\
Data File : BP002057.D
Acq On : 04 Mar 2020 19:08
Operator : CG/JU
Sample : L1677-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC1

Quant Time: Mar 05 06:23:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

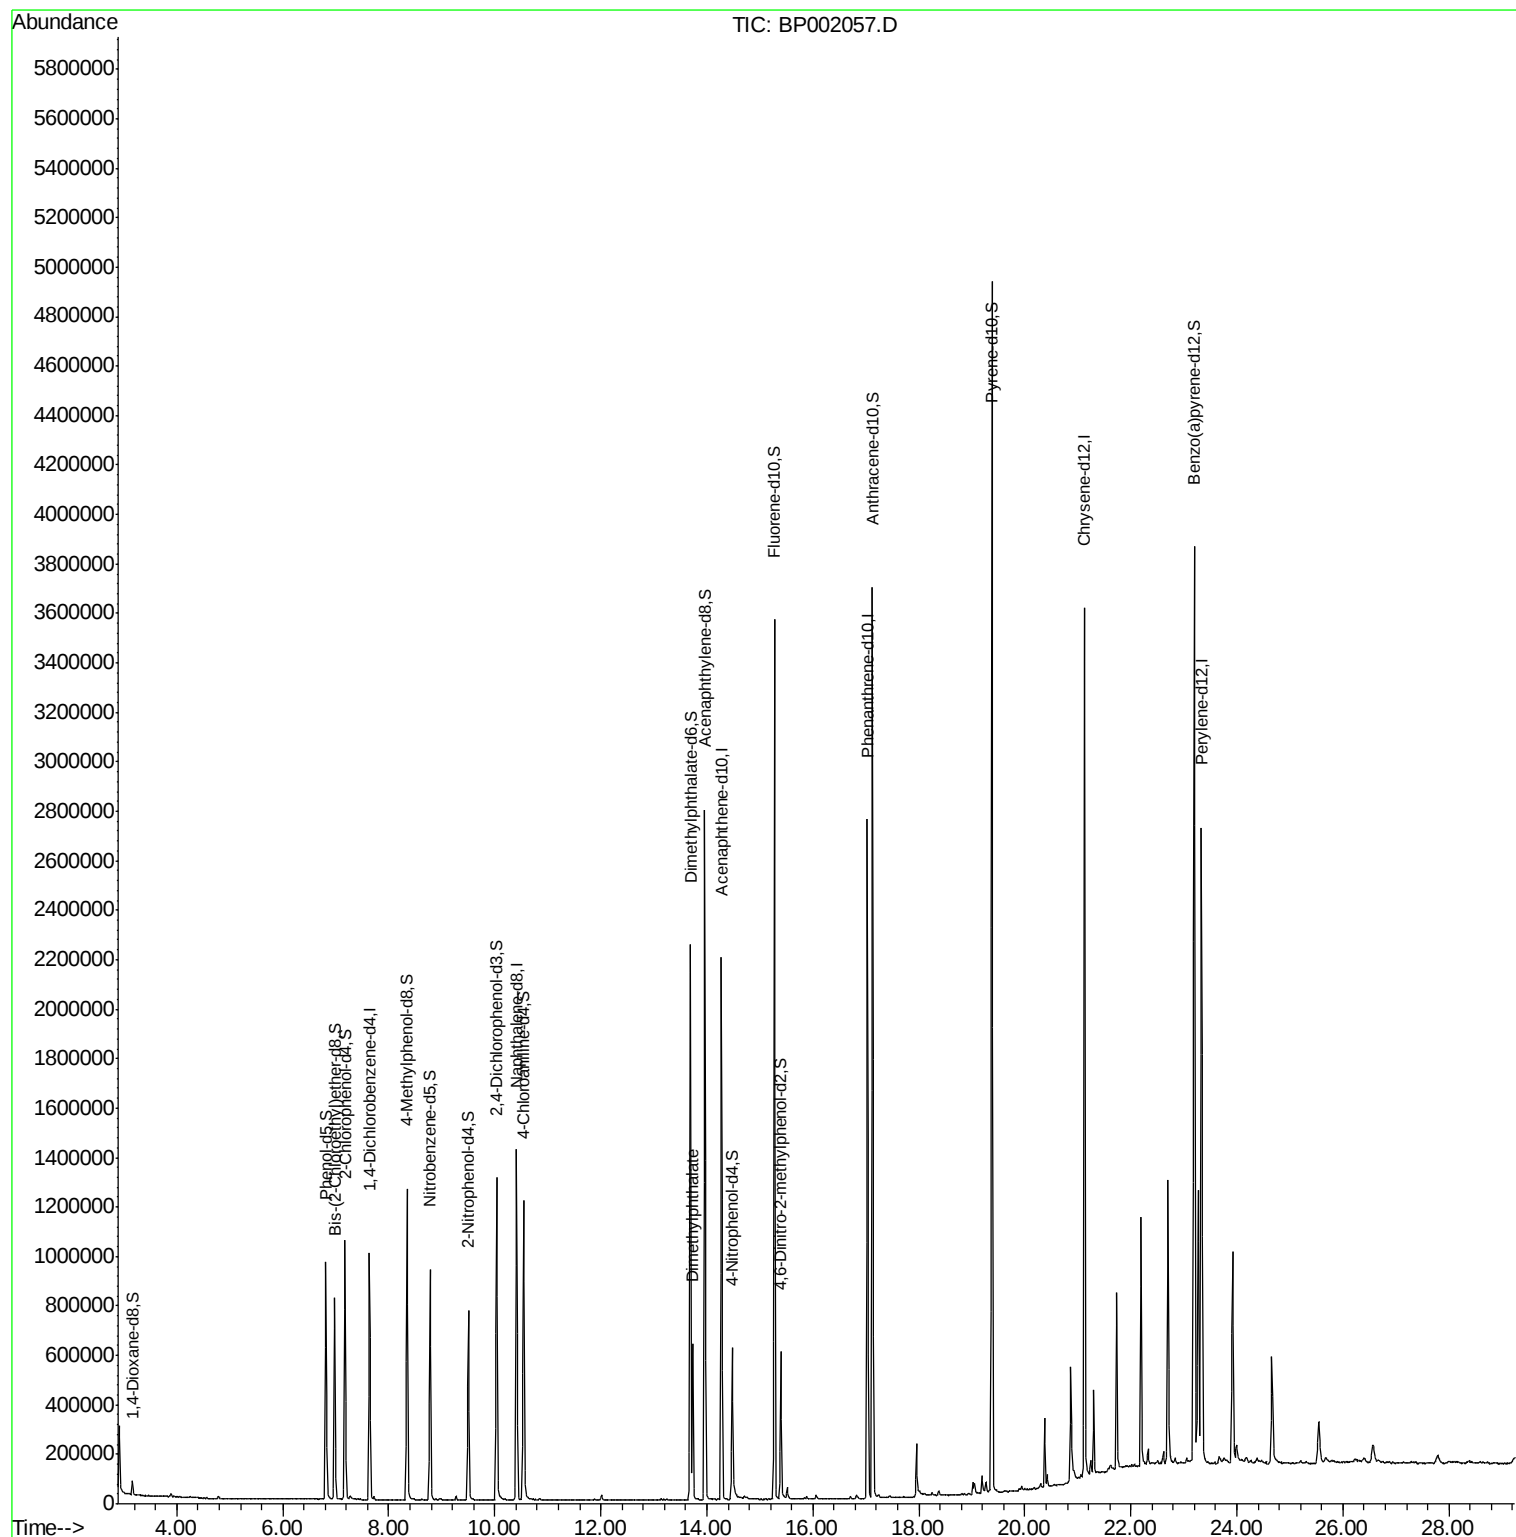

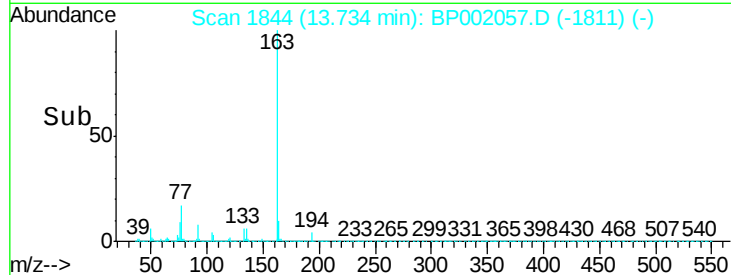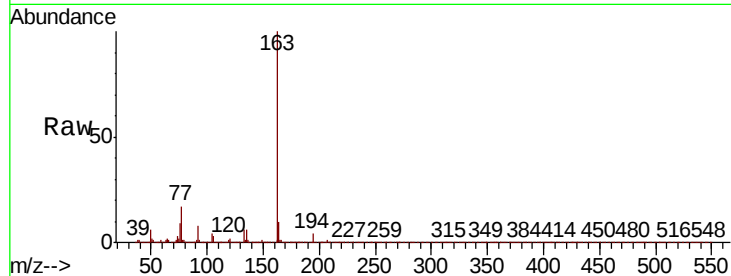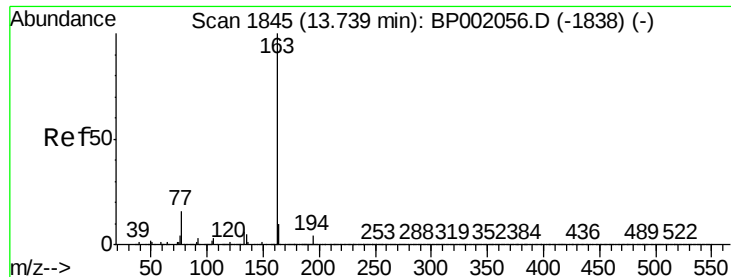

#45

Dimethylphthalate

Concen: 7.260 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002057.D

Acq: 04 Mar 2020 19:08

Instrument :

BNA_P

ClientSampleId :

C0CC1

Tot Ion:163 Resp: 433341

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.4 8.2 12.4

