

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030420\
 Data File : BP002061.D
 Acq On : 04 Mar 2020 21:24
 Operator : CG/JU
 Sample : L1677-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CD3

Quant Time: Mar 05 06:24:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	286906	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1174719	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	747893	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1617751	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1577685	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1831109	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	8671	1.30	ng/uL	0.00
5) Phenol-d5	6.82	99	130020	5.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	82611	7.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	120328	6.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	107349	5.97	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	49407	5.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	49007	4.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	111402	5.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	148351	6.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	367141	6.49	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	430947	6.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	19778	1.83	ng/ul	0.00
58) Fluorene-d10	15.27	176	339363	6.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	17649	1.98	ng/ul	0.00
71) Anthracene-d10	17.12	188	500911	6.89	ng/ul	0.00
79) Pyrene-d10	19.37	212	637002	7.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	671050	7.16	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	79296	1.357	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030420\
Data File : BP002061.D
Acq On : 04 Mar 2020 21:24
Operator : CG/JU
Sample : L1677-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD3

Quant Time: Mar 05 06:24:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

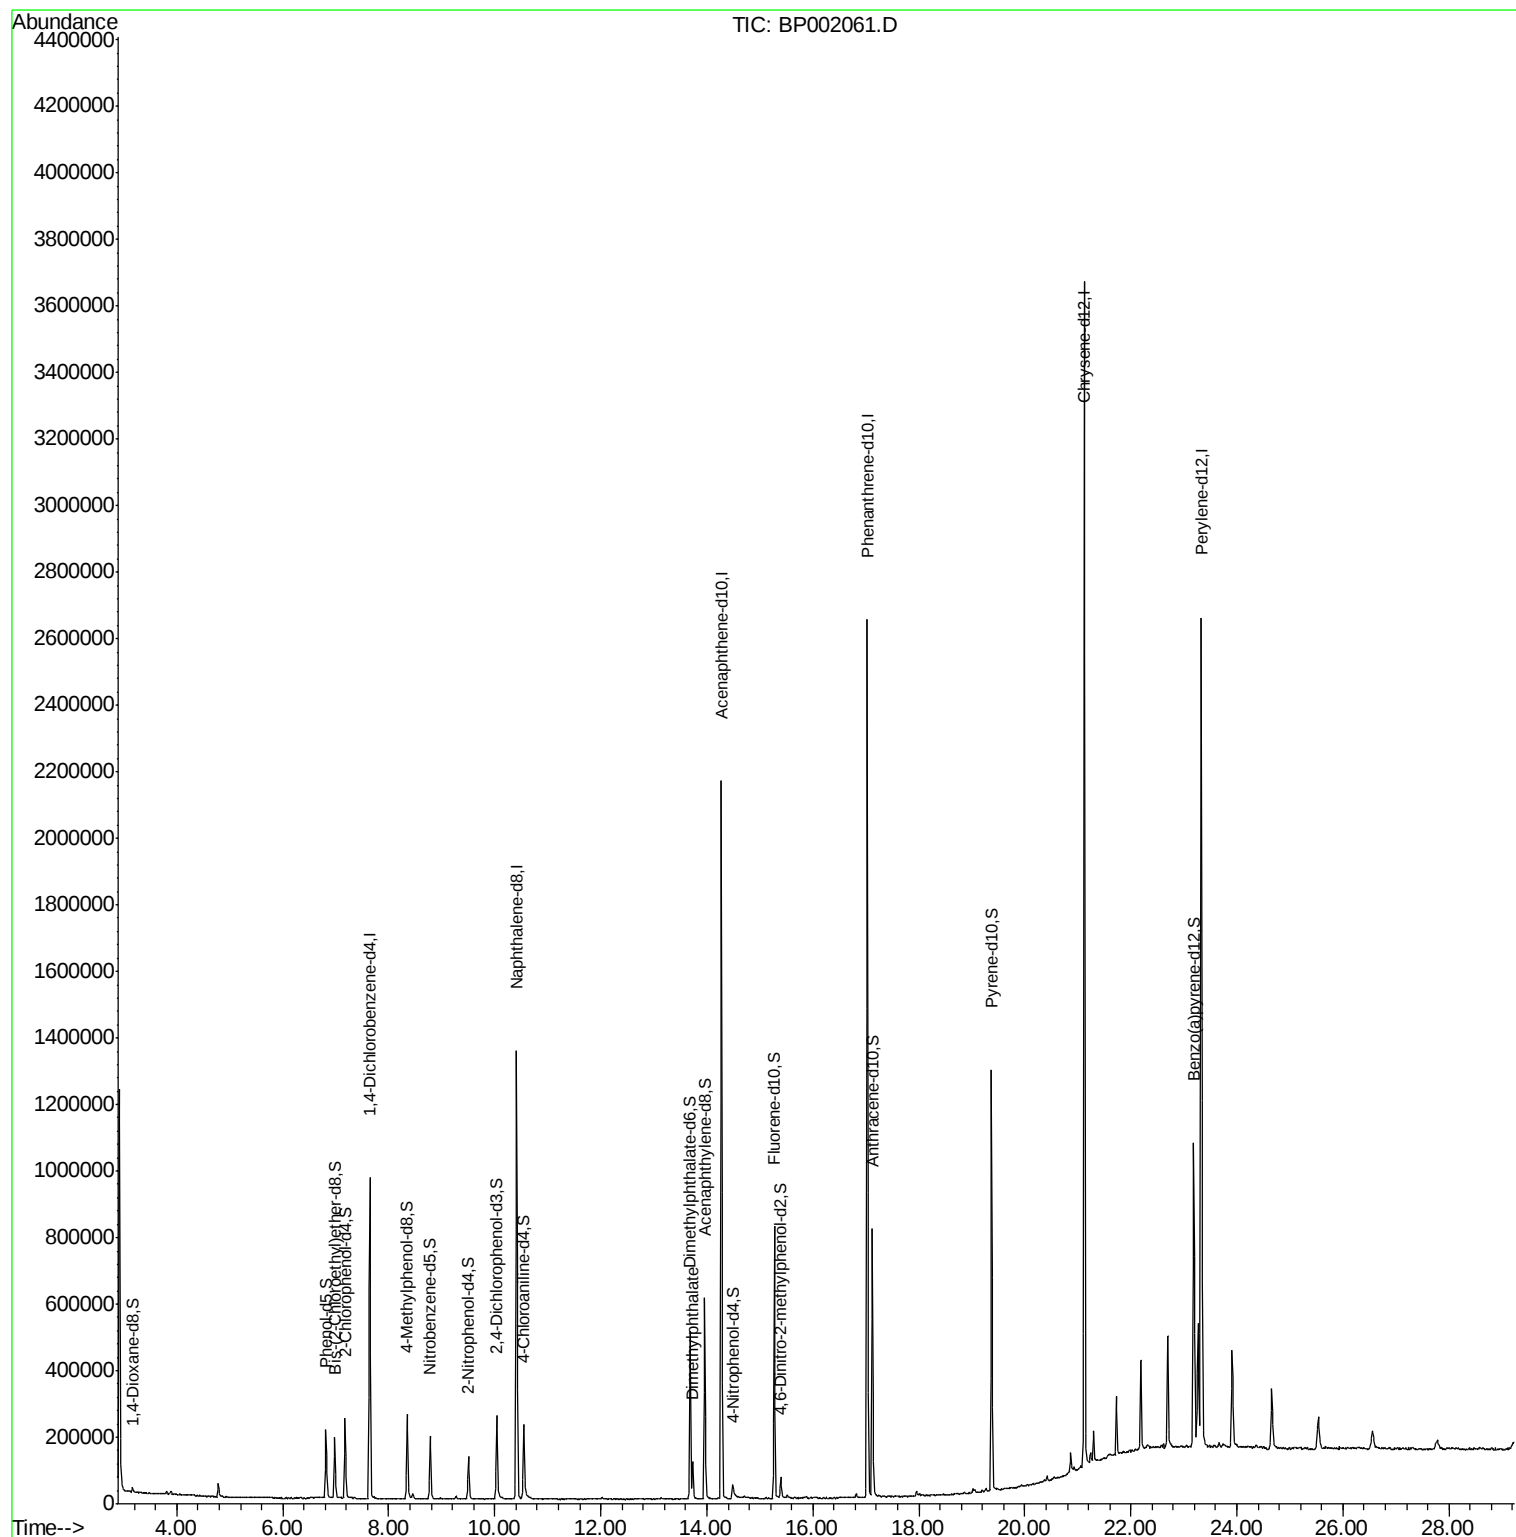

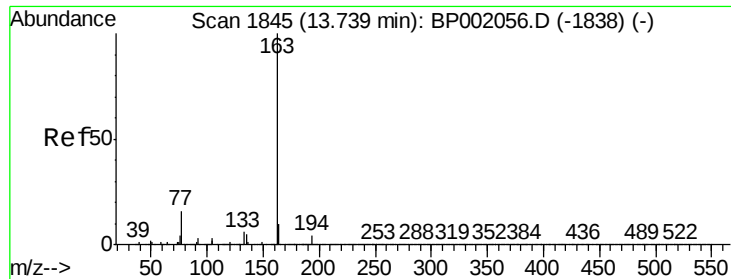

#45

Dimethylphthalate

Concen: 1.357 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002061.D

Acq: 04 Mar 2020 21:24

Instrument :

BNA_P

ClientSampleId :

C0CD3


Tot Ion:163 Resp: 79296

Ion Ratio Lower Upper

163 100

194 4.8 3.6 5.4

164 9.5 8.2 12.4

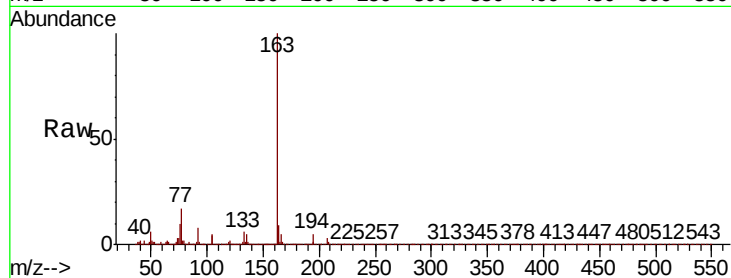

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

