

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030420\
 Data File : BP002063.D
 Acq On : 04 Mar 2020 23:06
 Operator : CG/JU
 Sample : L1677-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CD2

Quant Time: Mar 05 07:09:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	290613	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1190725	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	748461	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1598104	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1563402	20.00	ng/ul	-0.01
86) Perylene-d12	23.32	264	1772381	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	31417	4.65	ng/uL	0.00
5) Phenol-d5	6.82	99	572794	25.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	329847	28.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	508484	26.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	477655	26.22	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	235163	25.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	254741	24.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	513414	25.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	690120	31.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1595641	28.17	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1938710	28.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	178923	16.52	ng/ul	0.00
58) Fluorene-d10	15.27	176	1422424	29.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	130522	14.81	ng/ul	0.00
71) Anthracene-d10	17.12	188	2122407	29.55	ng/ul	0.00
79) Pyrene-d10	19.37	212	2441869	29.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2676622	29.52	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	471989	8.072	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030420\
Data File : BP002063.D
Acq On : 04 Mar 2020 23:06
Operator : CG/JU
Sample : L1677-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD2

Quant Time: Mar 05 07:09:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

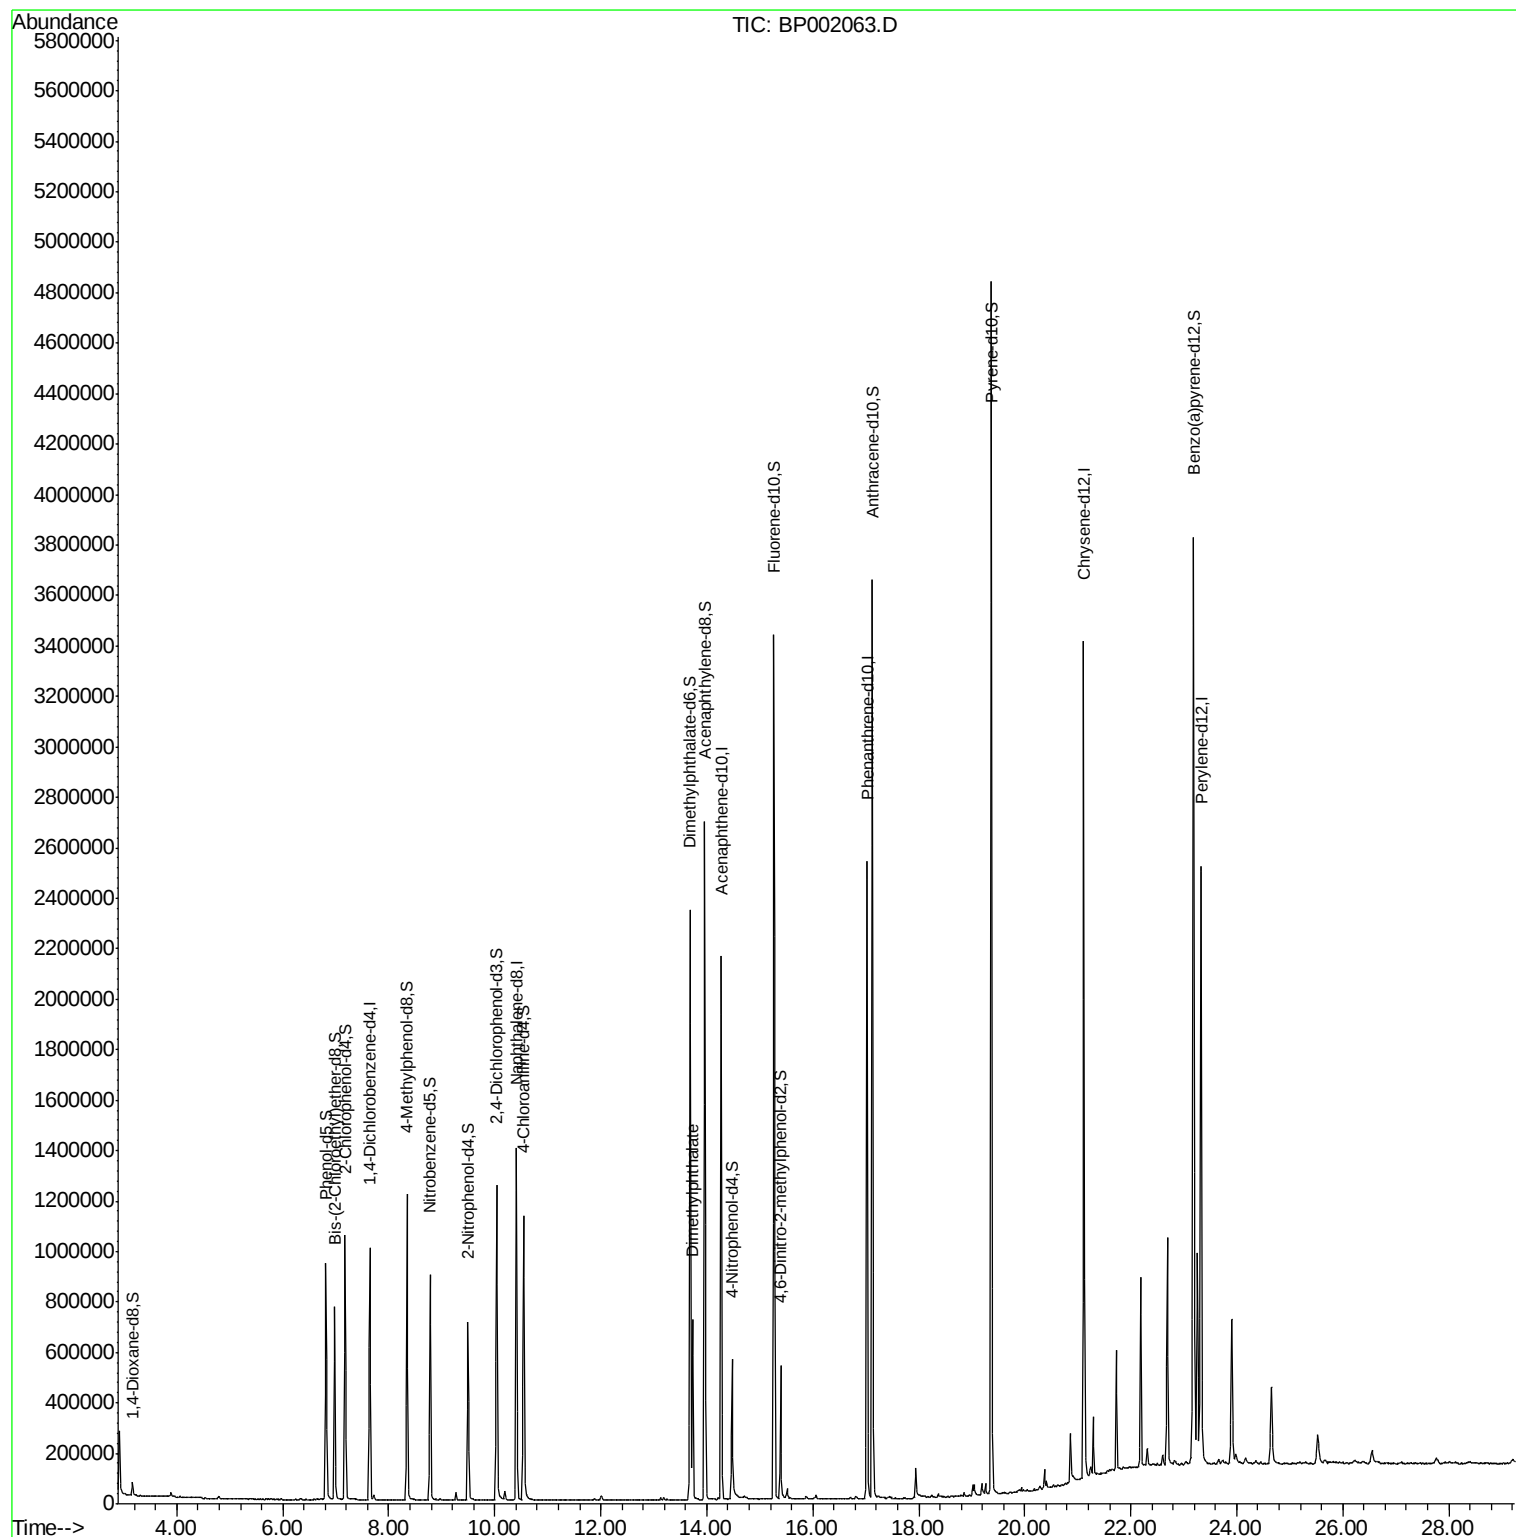

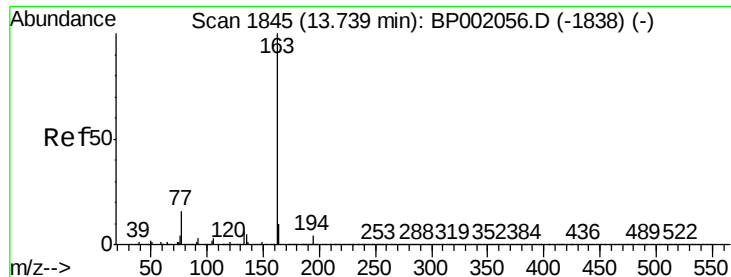

#45

Dimethylphthalate

Concen: 8.072 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002063.D

Acq: 04 Mar 2020 23:06

Instrument :

BNA_P

ClientSampleId :

C0CD2


Tot Ion:163 Resp: 471989

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.4 8.2 12.4

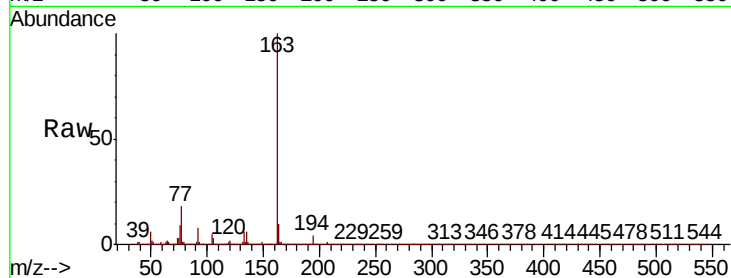

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

