

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030520\
 Data File : BP002083.D
 Acq On : 05 Mar 2020 22:45
 Operator : CG/JU
 Sample : L1780-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 06 06:33:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	278493	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1148119	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	734207	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1584576	20.00	ng/ul	-0.01
78) Chrysene-d12	21.12	240	1576488	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1811637	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	26663	4.12	ng/uL	0.00
5) Phenol-d5	6.82	99	47520	2.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	107930	9.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	141311	7.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	82890	4.75	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	69918	7.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	69979	7.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	152398	7.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1668	0.08	ng/ul	0.03
44) Dimethylphthalate-d6	13.69	166	519028	9.34	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	561223	8.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	8118	0.76	ng/ul	0.01
58) Fluorene-d10	15.27	176	479423	9.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	32109	3.68	ng/ul	0.00
71) Anthracene-d10	17.12	188	713527	10.02	ng/ul	0.00
79) Pyrene-d10	19.37	212	860349	10.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	790669	8.53	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	115943	2.021	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030520\
Data File : BP002083.D
Acq On : 05 Mar 2020 22:45
Operator : CG/JU
Sample : L1780-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Mar 06 06:33:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

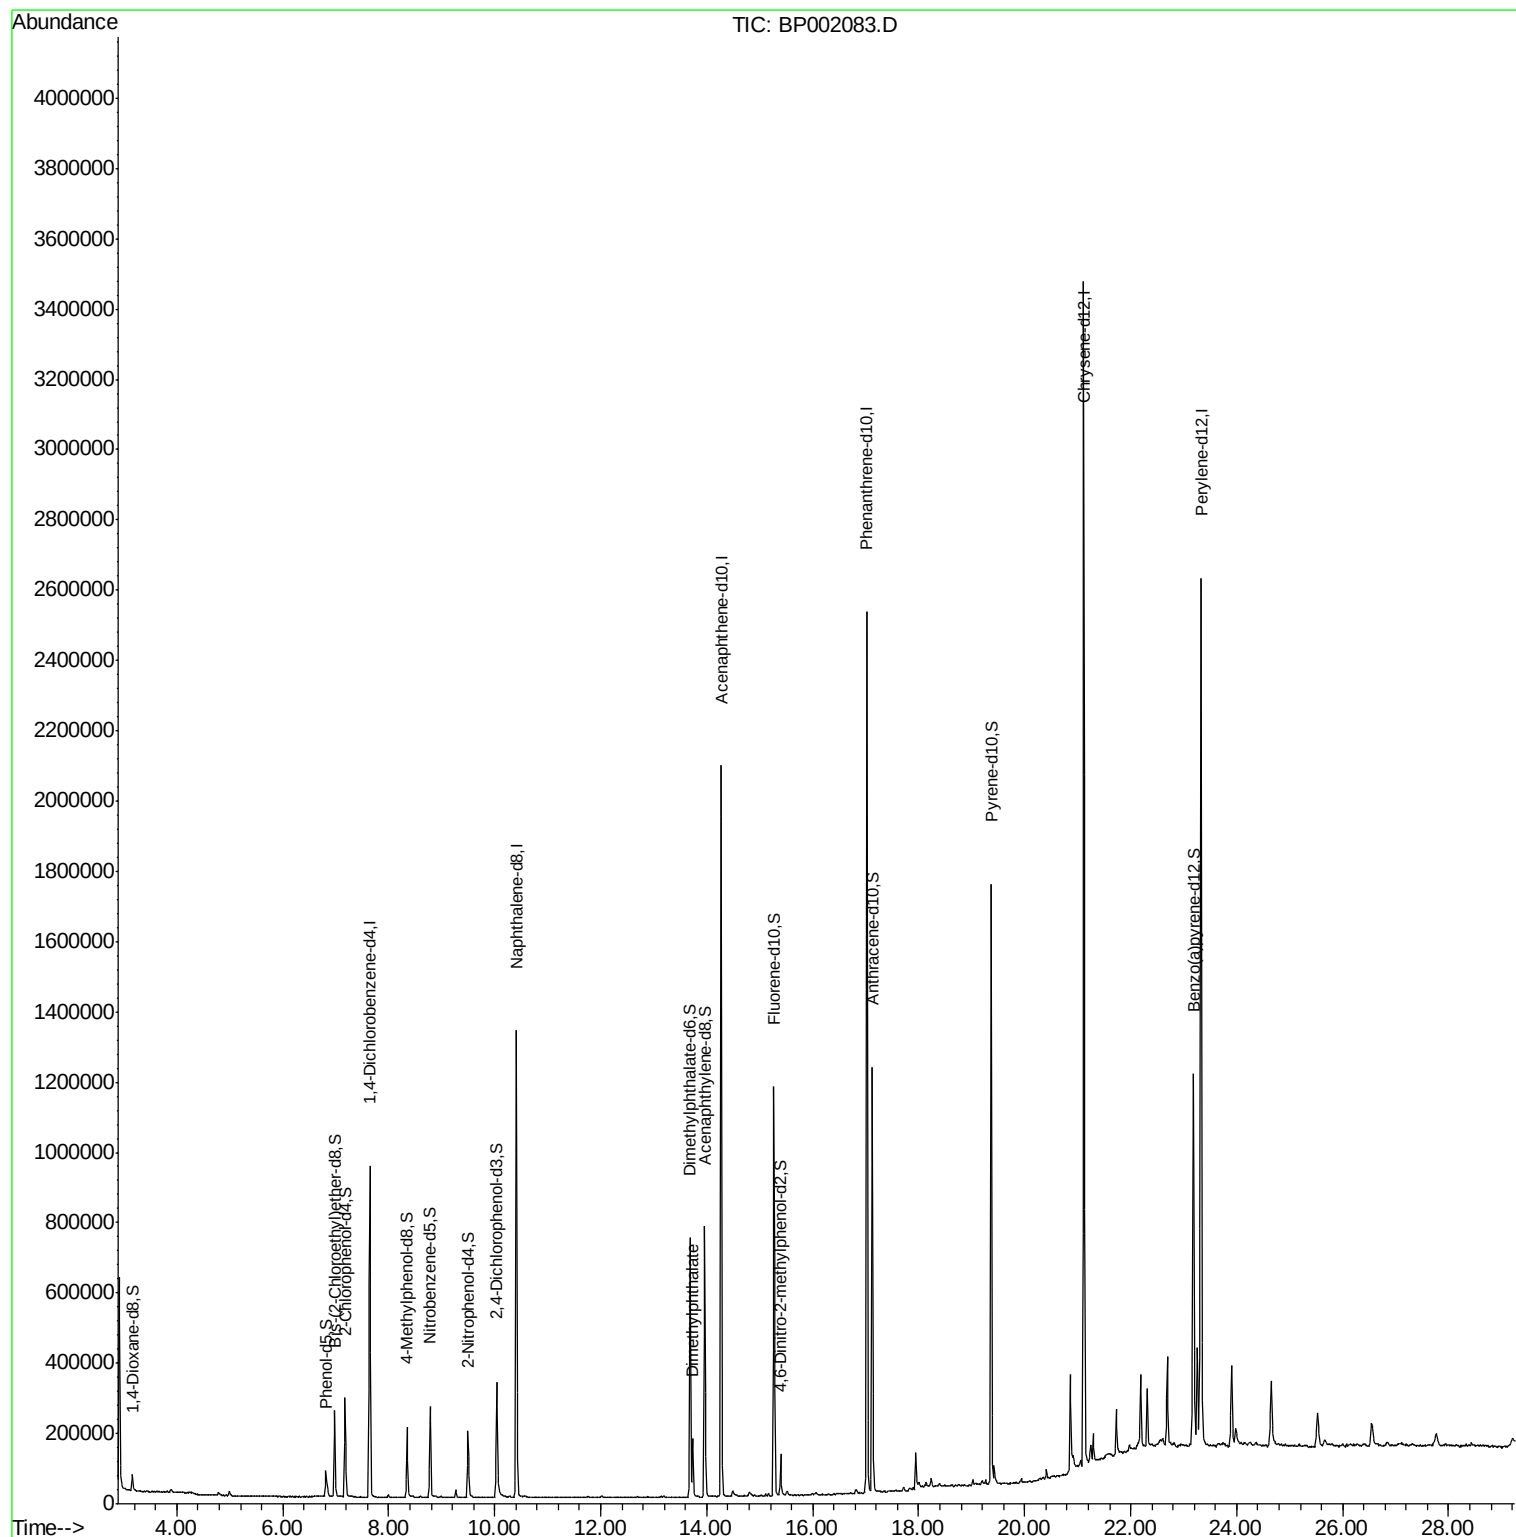

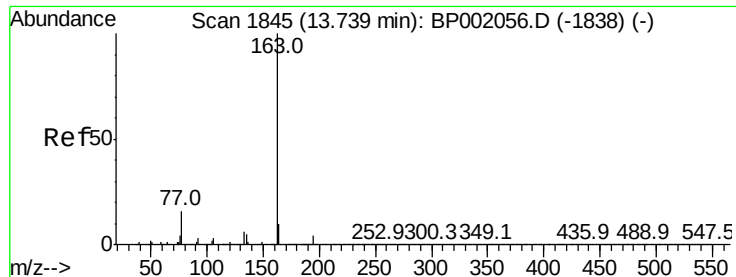

#45

Dimethylphthalate

Concen: 2.021 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002083.D

Acq: 05 Mar 2020 22:45

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 115943

Ion Ratio Lower Upper

163 100

194 4.7 3.6 5.4

164 10.3 8.2 12.4

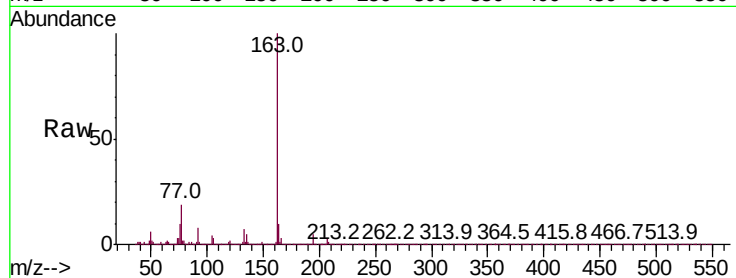

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

