

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030520\
 Data File : BP002068.D
 Acq On : 05 Mar 2020 14:00
 Operator : CG/JU
 Sample : L1677-20
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CB7

Quant Time: Mar 05 15:39:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	282038	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1151317	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	727185	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1579339	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	1566424	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1805267	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	30872	4.71	ng/uL	0.00
5) Phenol-d5	6.82	99	595471	27.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	336123	29.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	521938	28.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	497079	28.11	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	246921	27.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	272602	27.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	529129	27.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	736895	35.07	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1606137	29.18	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1976762	30.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	187894	17.86	ng/ul	0.00
58) Fluorene-d10	15.27	176	1417939	29.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	155040	17.81	ng/ul	0.00
71) Anthracene-d10	17.13	188	2181321	30.73	ng/ul	0.00
79) Pyrene-d10	19.37	212	2501944	30.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	2672713	28.94	ng/ul	0.00


Target Compounds					Ovalue	
2) 1,4-Dioxane	3.20	88	10462	1.496	ng/uL#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030520\
Data File : BP002068.D
Acq On : 05 Mar 2020 14:00
Operator : CG/JU
Sample : L1677-20
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB7

Quant Time: Mar 05 15:39:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

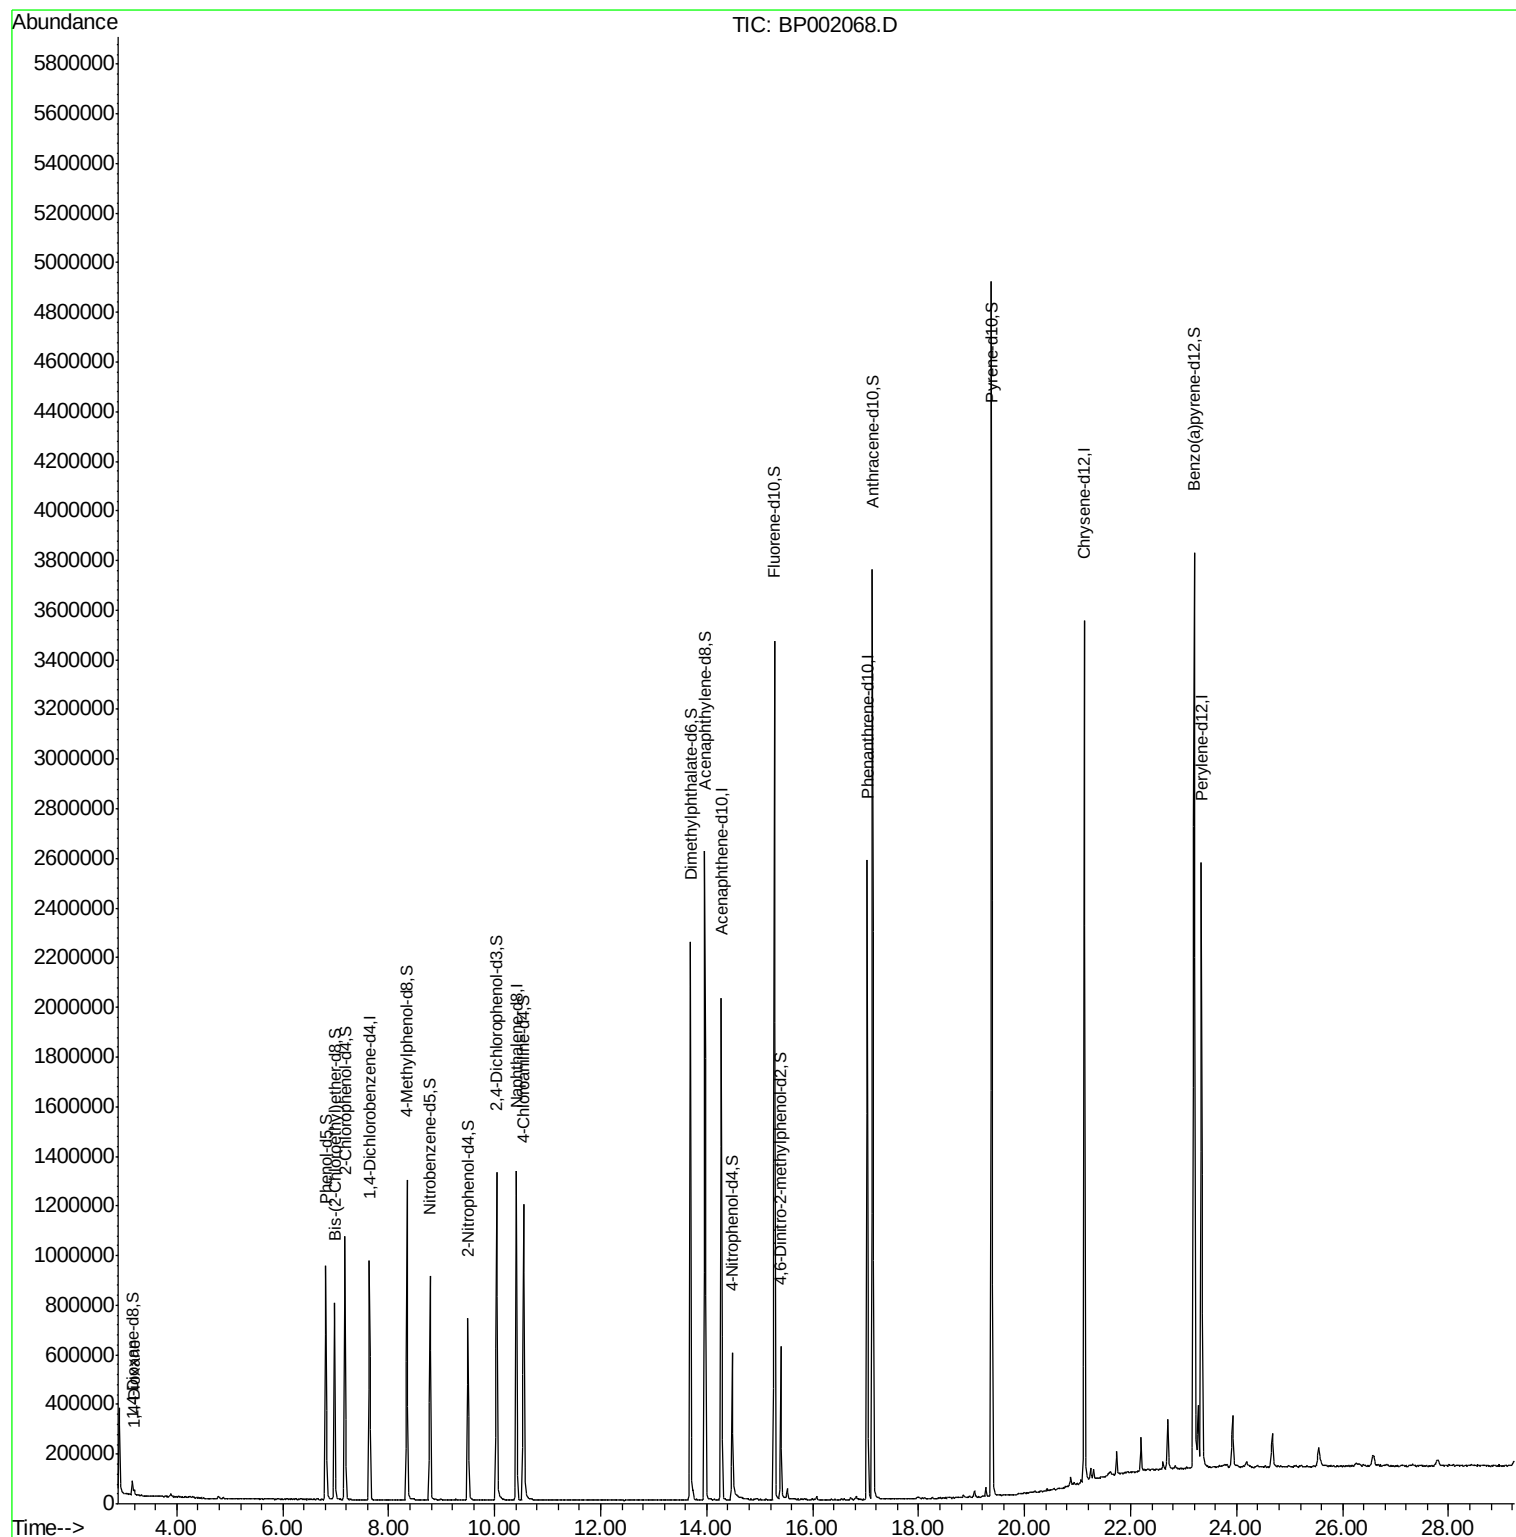

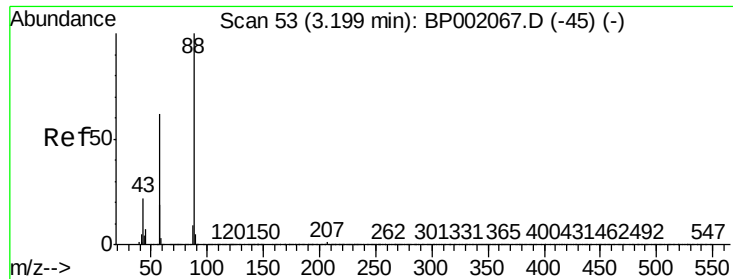

#2

1,4-Dioxane

Concen: 1.496 ng/uL

RT: 3.20 min Scan# 53

Delta R.T. 0.00 min

Lab File: BP002068.D

Acq: 05 Mar 2020 14:00

Instrument :

BNA_P

ClientSampleId :

C0CB7

Tot Ion: 88 Resp: 10462

Ion Ratio Lower Upper

88 100

43 19.6 22.6 34.0#

58 57.7 49.6 74.4

