

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030520\
 Data File : BP002074.D
 Acq On : 05 Mar 2020 17:40
 Operator : CG/JU
 Sample : L1780-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DG2

Quant Time: Mar 06 06:31:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	265753	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1087854	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	696314	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1508257	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1487651	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1687748	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	33114	5.36	ng/uL	0.00
5) Phenol-d5	6.82	99	142888	7.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	385633	35.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	489919	27.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	283993	17.05	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	284262	34.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	303896	32.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	554743	30.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	39964	2.01	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1868742	35.46	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2284364	36.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	31063	3.08	ng/ul	0.00
58) Fluorene-d10	15.27	176	1713517	37.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	196670	23.65	ng/ul	0.00
71) Anthracene-d10	17.12	188	2704532	39.90	ng/ul	0.00
79) Pyrene-d10	19.37	212	3107440	39.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3427434	39.69	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.73	163	144512	2.657	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030520\
Data File : BP002074.D
Acq On : 05 Mar 2020 17:40
Operator : CG/JU
Sample : L1780-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0DG2

Quant Time: Mar 06 06:31:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

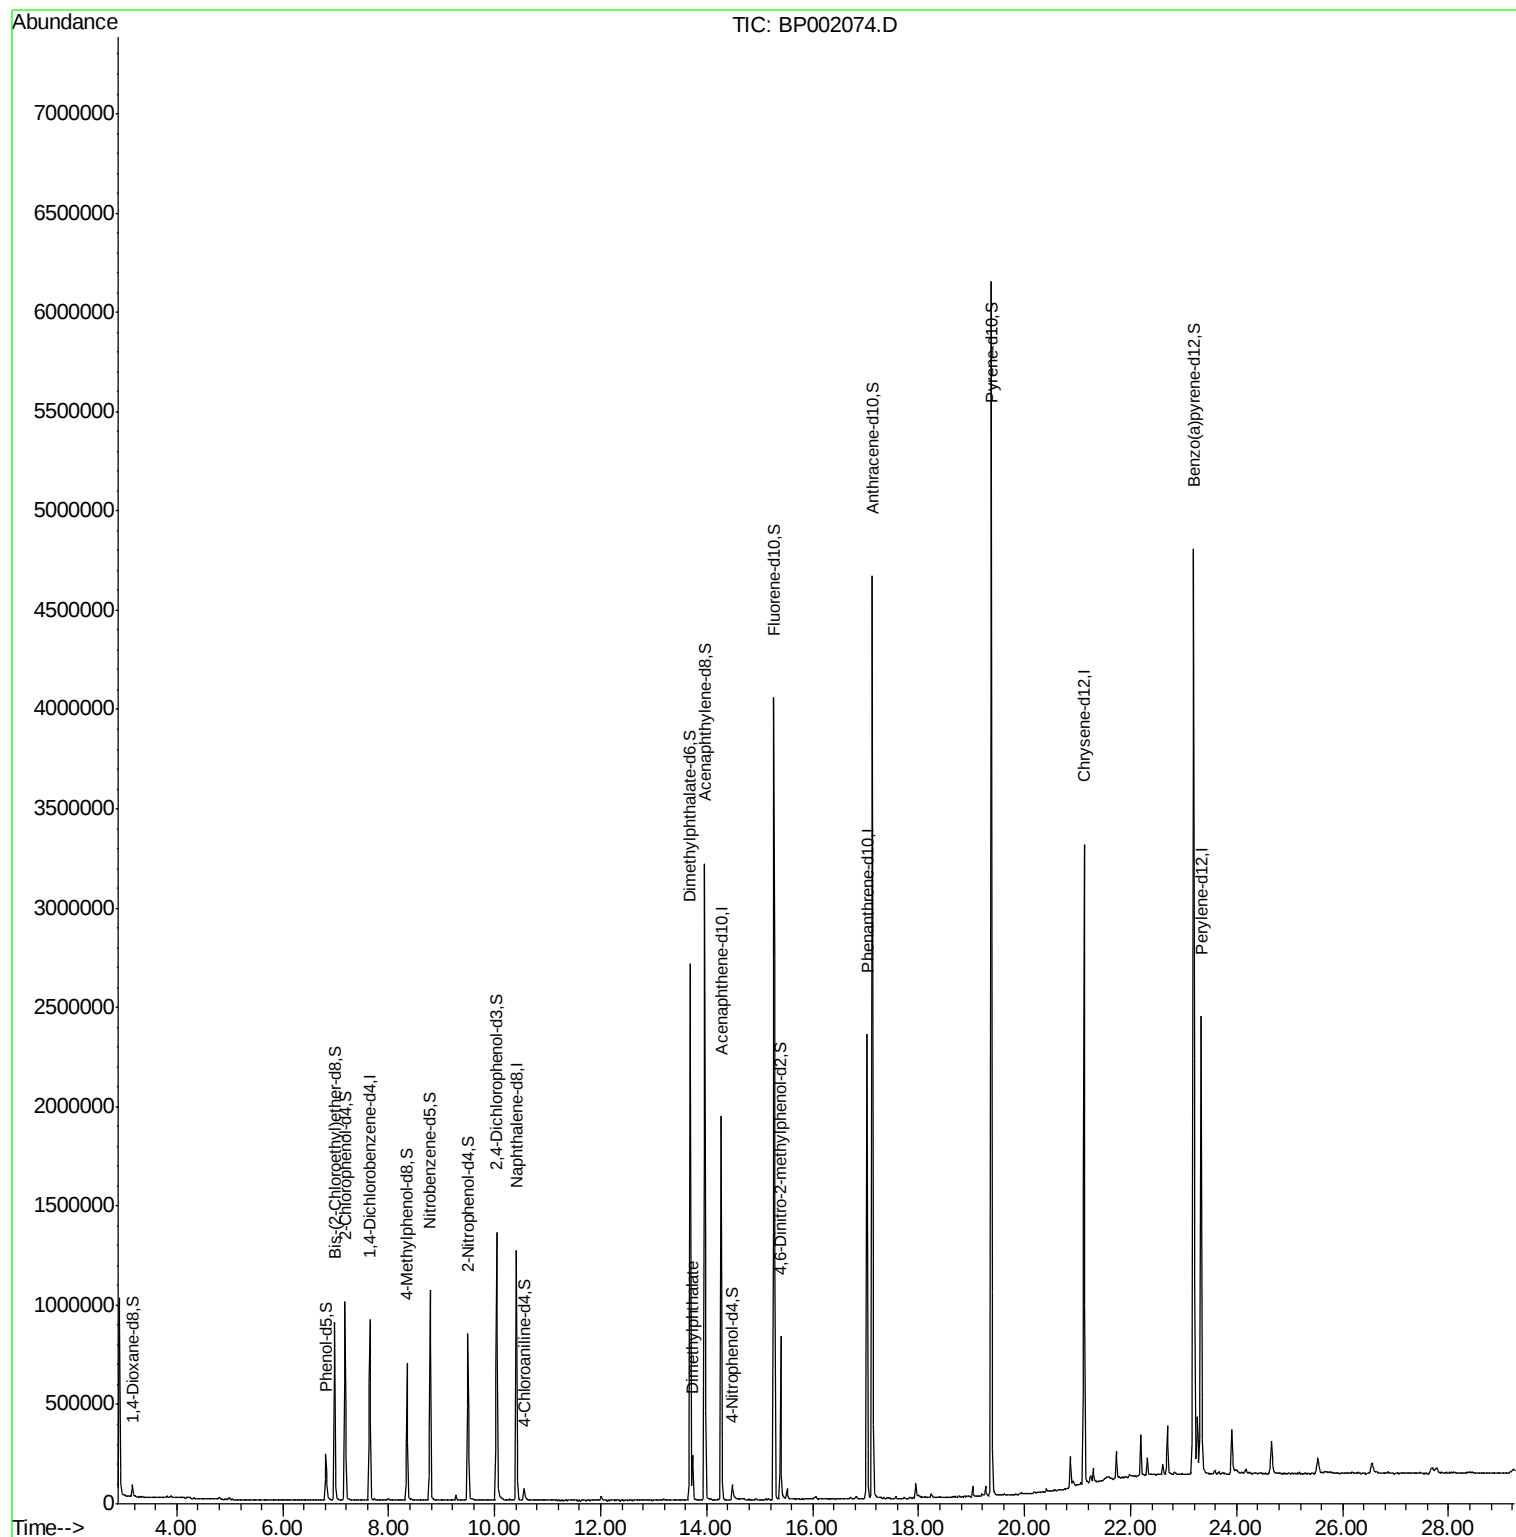

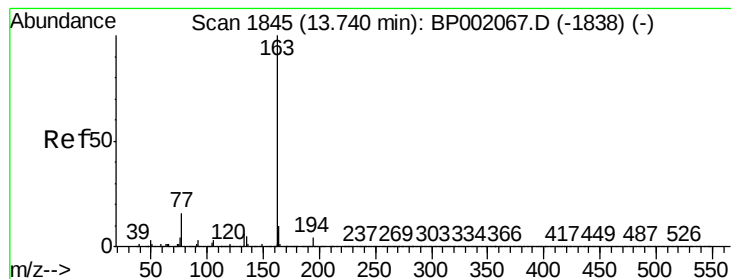

#45

Dimethylphthalate

Concen: 2.657 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002074.D

Acq: 05 Mar 2020 17:40

Instrument :

BNA_P

ClientSampleId :

C0DG2

Tot Ion:163 Resp: 144512

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.7 8.2 12.4

