

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030520\
 Data File : BP002081.D
 Acq On : 05 Mar 2020 21:38
 Operator : CG/JU
 Sample : L1780-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DH1

Manual Integrations
 APPROVED

mohammad
 3/6/2020 1:24:10 PM

Quant Time: Mar 06 07:44:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	252174	20.00	ng/ul	0.02
18) Naphthalene-d8	10.41	136	1125953	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	717940	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1570777	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1614935	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1824306	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	28358	4.83	ng/uL	0.00
5) Phenol-d5	6.82	99	38913	2.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	78889	7.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	103191	6.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	61071	3.86	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	49731	5.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	53486	5.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	108385	5.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	14728	0.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	363173	6.68	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	406982	6.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	6907m	0.66	ng/ul	0.01
58) Fluorene-d10	15.27	176	326455	6.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	22366	2.58	ng/ul	0.00
71) Anthracene-d10	17.12	188	518852	7.35	ng/ul	0.00
79) Pyrene-d10	19.37	212	637304	7.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	682143	7.31	ng/ul	-0.01

Target Compounds

					Ovalue
6) Phenol	6.85	94	41235	2.065	ng/ul 96
10) 2-Chlorophenol	7.21	128	38234	2.241	ng/ul 97
20) Nitrobenzene	8.84	77	6089565	315.982	ng/ul 99
37) 1,2,4,5-Tetrachlorobenzene	12.46	216	110384	4.612	ng/ul 97
45) Dimethylphthalate	13.73	163	121411	2.165	ng/ul 100
73) 1,2,3,4-Tetrachlorobenzene	13.07	216	123879	4.909	ng/uL 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030520\
Data File : BP002081.D
Acq On : 05 Mar 2020 21:38
Operator : CG/JU
Sample : L1780-12
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0DH1

Manual Integrations
APPROVED

mohammad
3/6/2020 1:24:10 PM

Quant Time: Mar 06 07:44:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

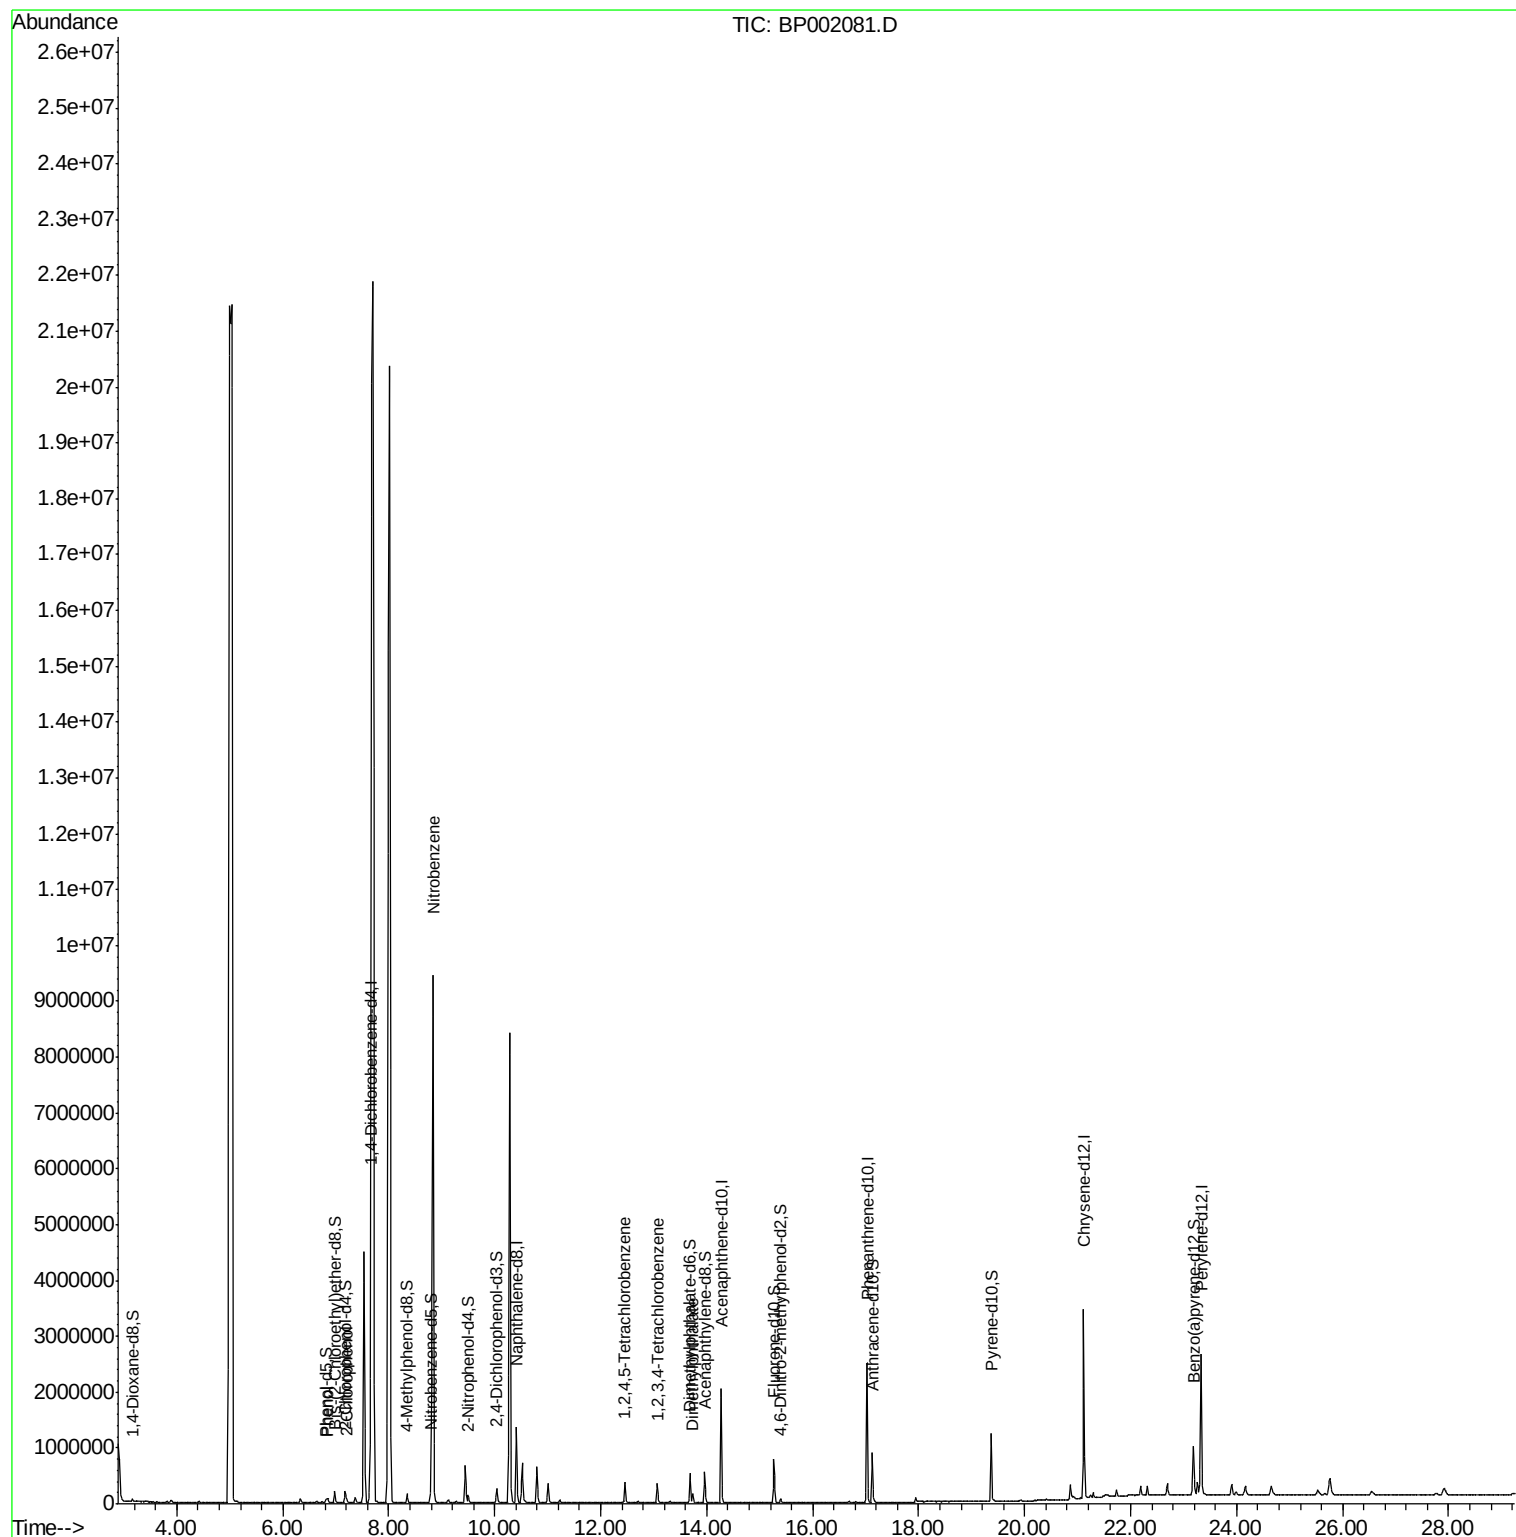

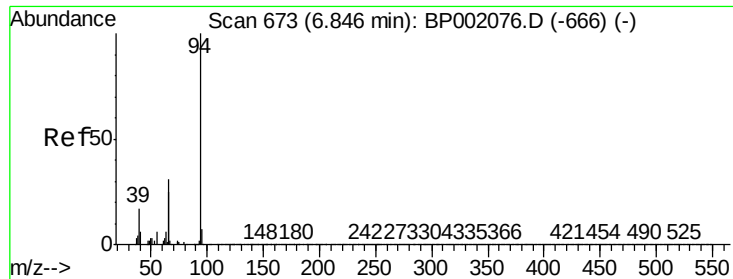

#6

Phenol

Concen: 2.065 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. 0.01 min

Lab File: BP002081.D

Acq: 05 Mar 2020 21:38

Instrument :

BNA_P





ClientSampleId :

C0DH1

Tot Ion:	94	Resp:	41235
Ion	Ratio	Lower	Upper
94	100		
65	24.9	20.6	30.8
66	32.2	28.2	42.2

Manual Integrations
APPROVED

mohammad
3/6/2020 1:24:10 PM

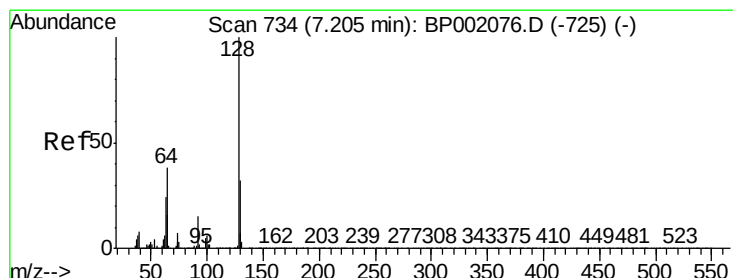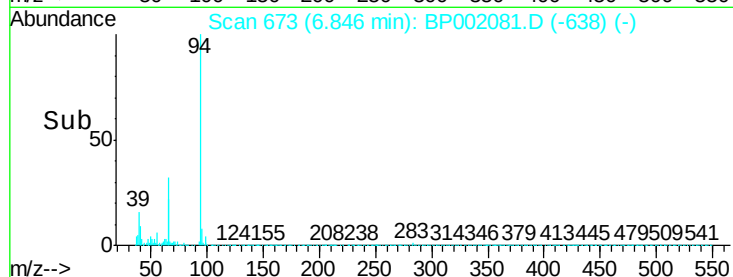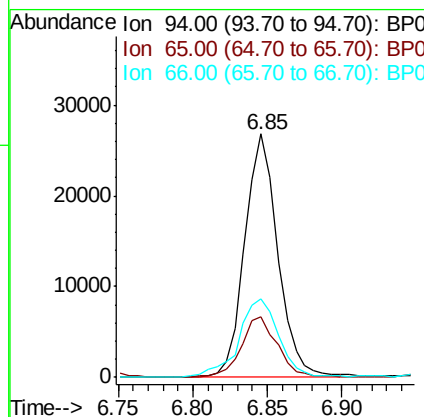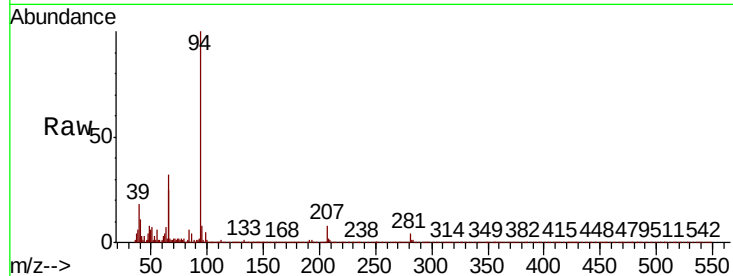

#10

2-Chlorophenol

Concen: 2.241 ng/ul




RT: 7.21 min Scan# 735


Delta R.T. 0.01 min

Lab File: BP002081.D

Acq: 05 Mar 2020 21:38

Tgt Ion:	128	Resp:	38234
Ion	Ratio	Lower	Upper
128	100		
64	37.0	31.5	47.3
130	31.5	26.3	39.5

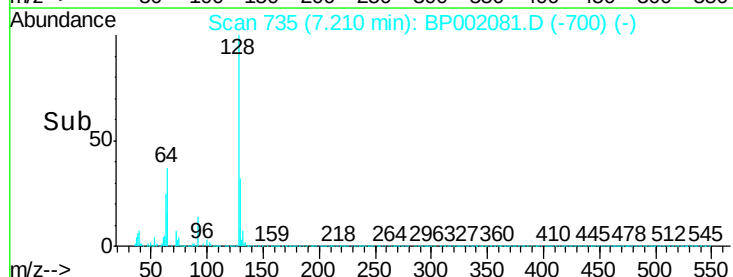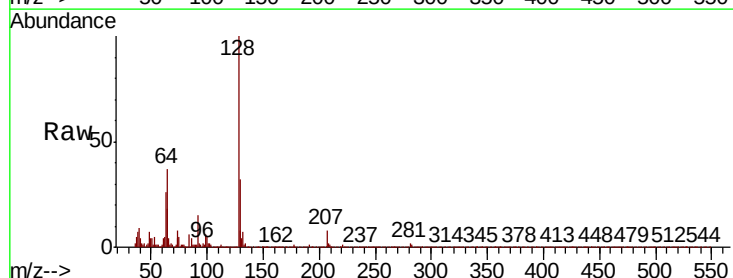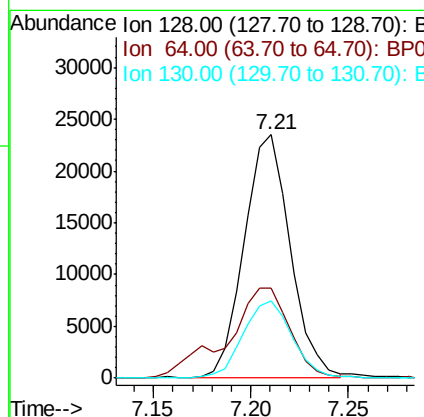

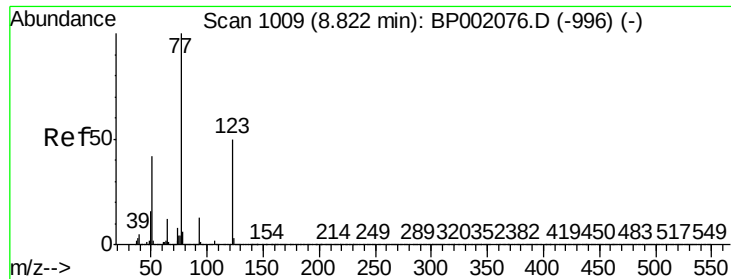





#20
Nitrobenzene
Concen: 315.982 ng/ul
RT: 8.84 min Scan# 1012
Delta R.T. 0.02 min
Lab File: BP002081.D
Acq: 05 Mar 2020 21:38

Instrument :
BNA_P
ClientSampleId :
C0DH1

Tot Ion	Ratio	Lower	Upper
77	100		
123	52.5	41.4	62.0
65	13.6	9.9	14.9




Manual Integrations
APPROVED


mohammad
3/6/2020 1:24:10 PM

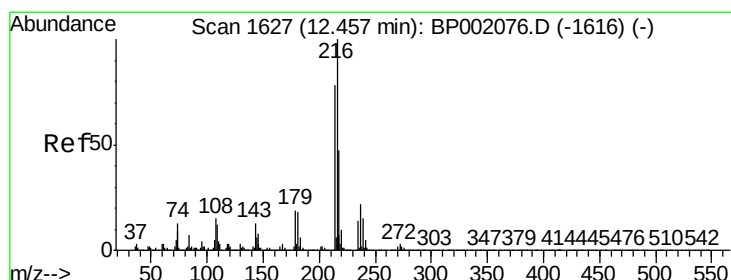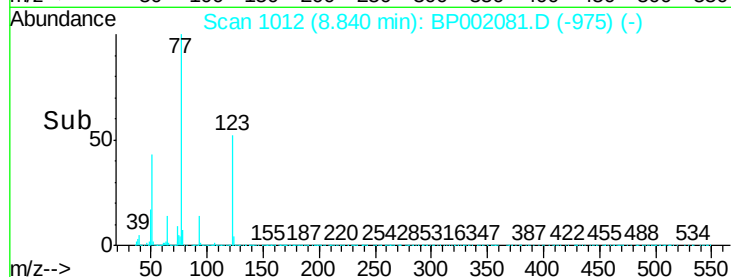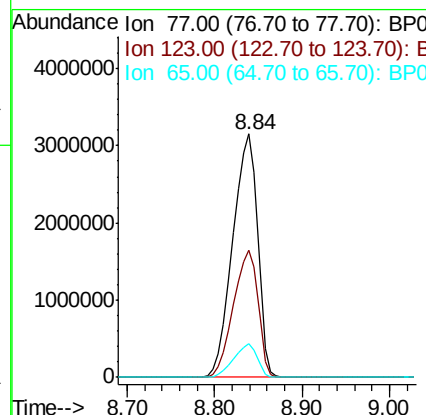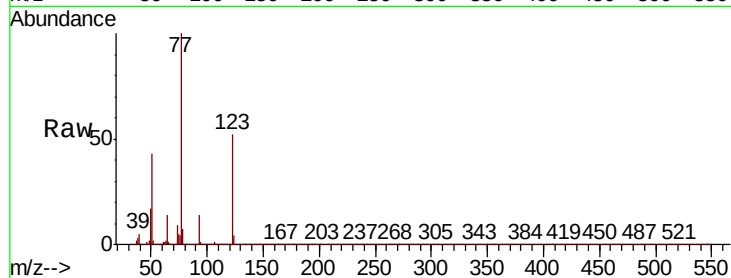

#37
1,2,4,5-Tetrachlorobenzene
Concen: 4.612 ng/ul
RT: 12.46 min Scan# 1627
Delta R.T. 0.00 min
Lab File: BP002081.D
Acq: 05 Mar 2020 21:38

Tgt Ion	Ratio	Lower	Upper
216	100		
214	81.2	61.8	92.8
179	20.0	16.0	24.0
108	14.8	11.9	17.9

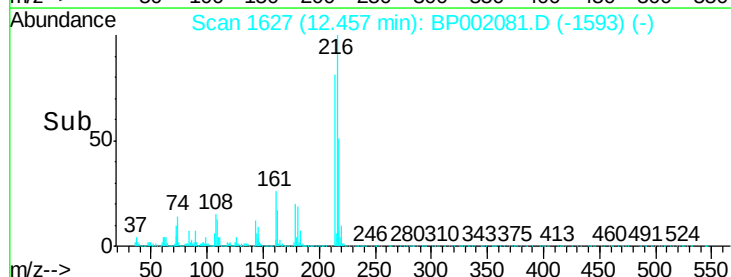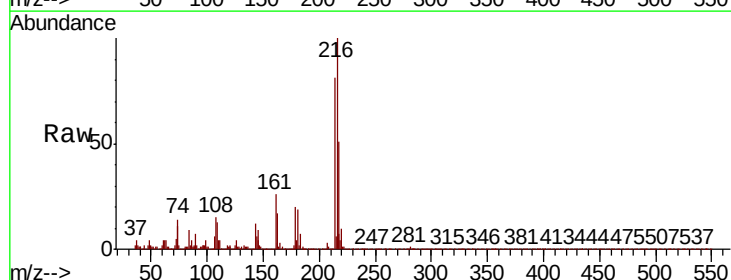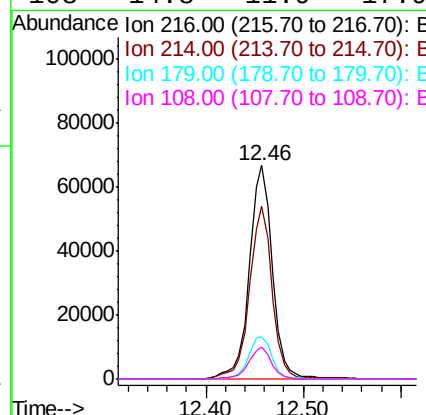

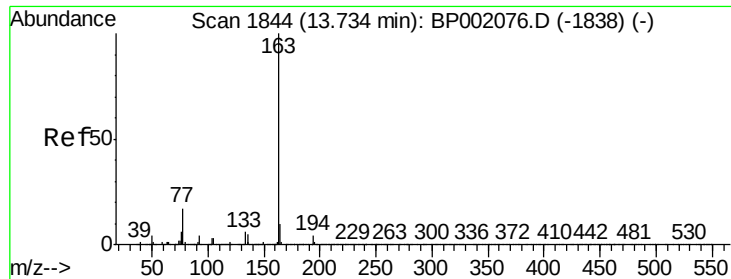





#45
Dimethylphthalate
Concen: 2.165 ng/ul
RT: 13.73 min Scan# 1844
Delta R.T. -0.01 min
Lab File: BP002081.D
Acq: 05 Mar 2020 21:38

Instrument :
BNA_P
ClientSampled :
C0DH1

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.6	5.4
164	10.1	8.2	12.4

Manual Integrations
APPROVED

mohammad
3/6/2020 1:24:10 PM

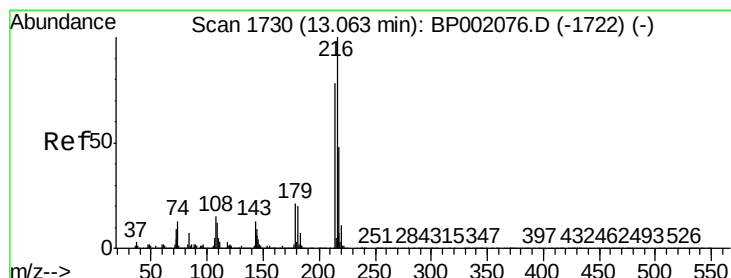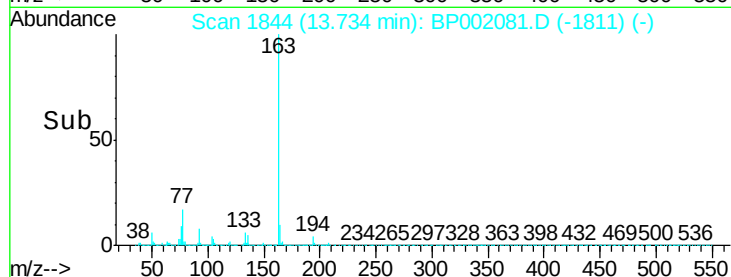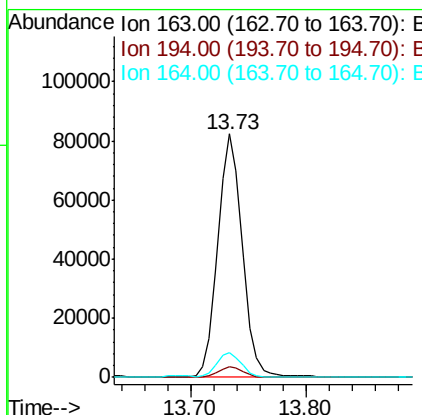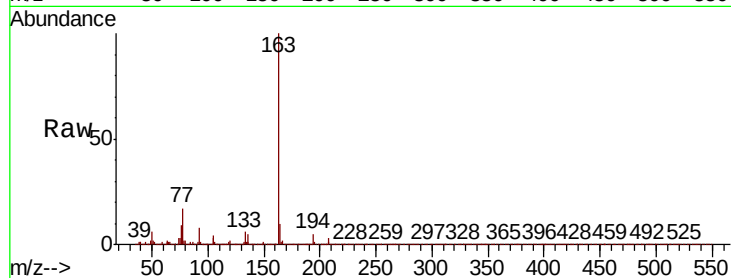

#73
1,2,3,4-Tetrachlorobenzene
Concen: 4.909 ng/uL
RT: 13.07 min Scan# 1731
Delta R.T. 0.00 min
Lab File: BP002081.D
Acq: 05 Mar 2020 21:38

Tgt Ion	Ratio	Lower	Upper
216	100		
214	74.0	63.1	94.7
218	48.5	38.2	57.2

