
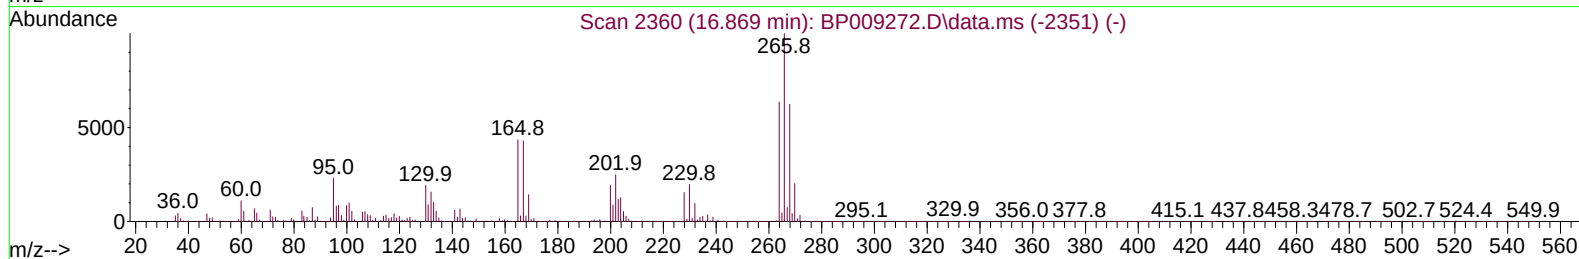
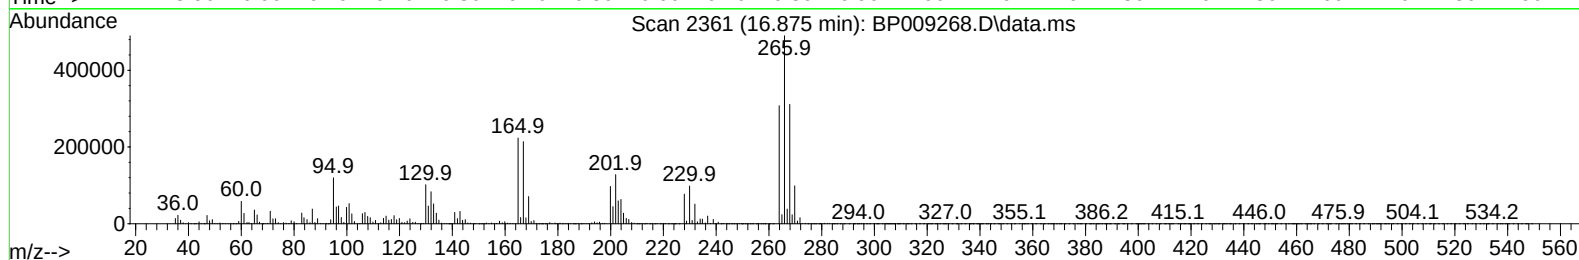


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030522\
 Data File : BP009268.D
 Acq On : 04 Mar 2022 15:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 05:02:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

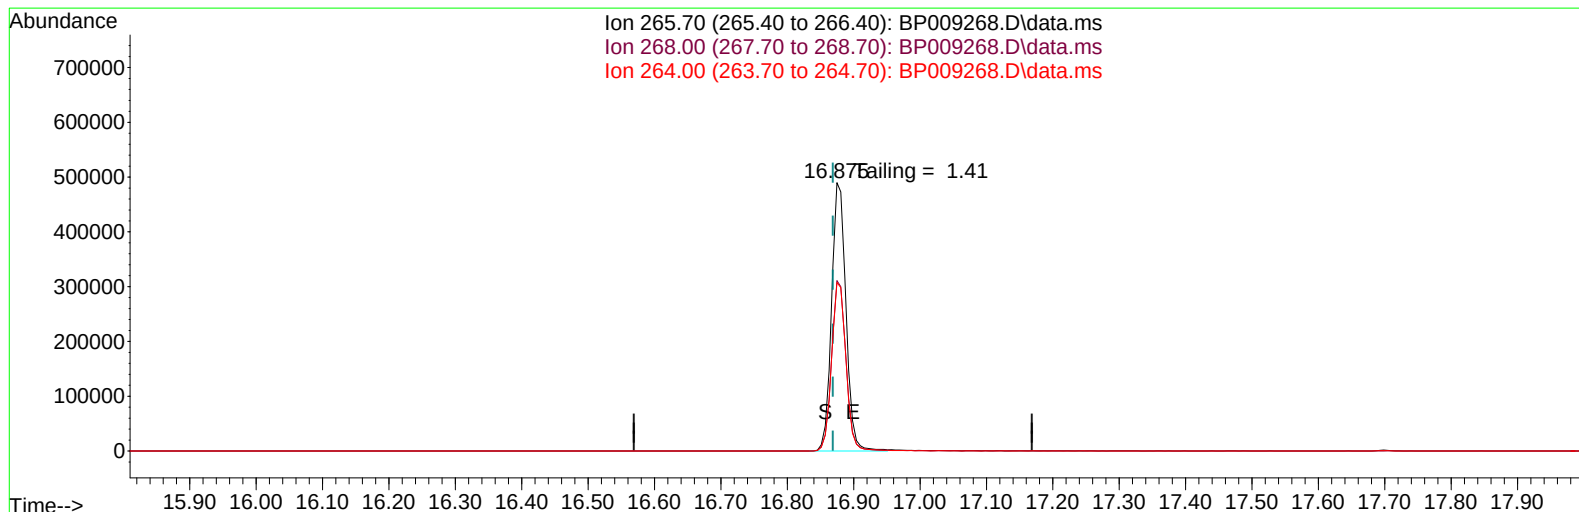

TIC: BP009268.D\data.ms

(70) Pentachlorophenol (C)




16.875min (+ 0.006) 59220.11 ng

response 739715

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.52
264.00	63.60	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030522\
 Data File : BP009268.D
 Acq On : 04 Mar 2022 15:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 05:02:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

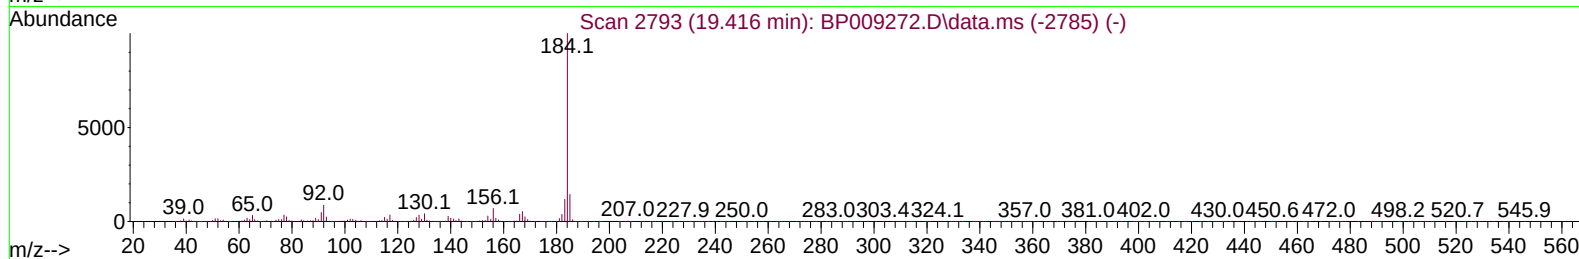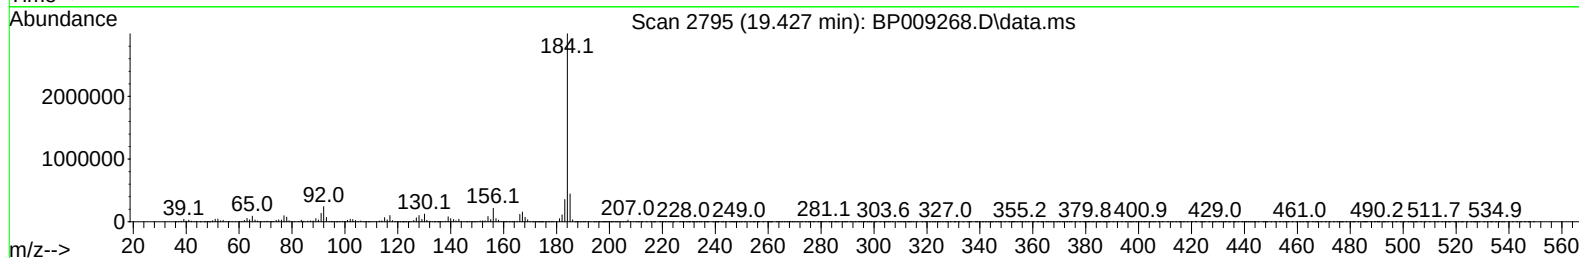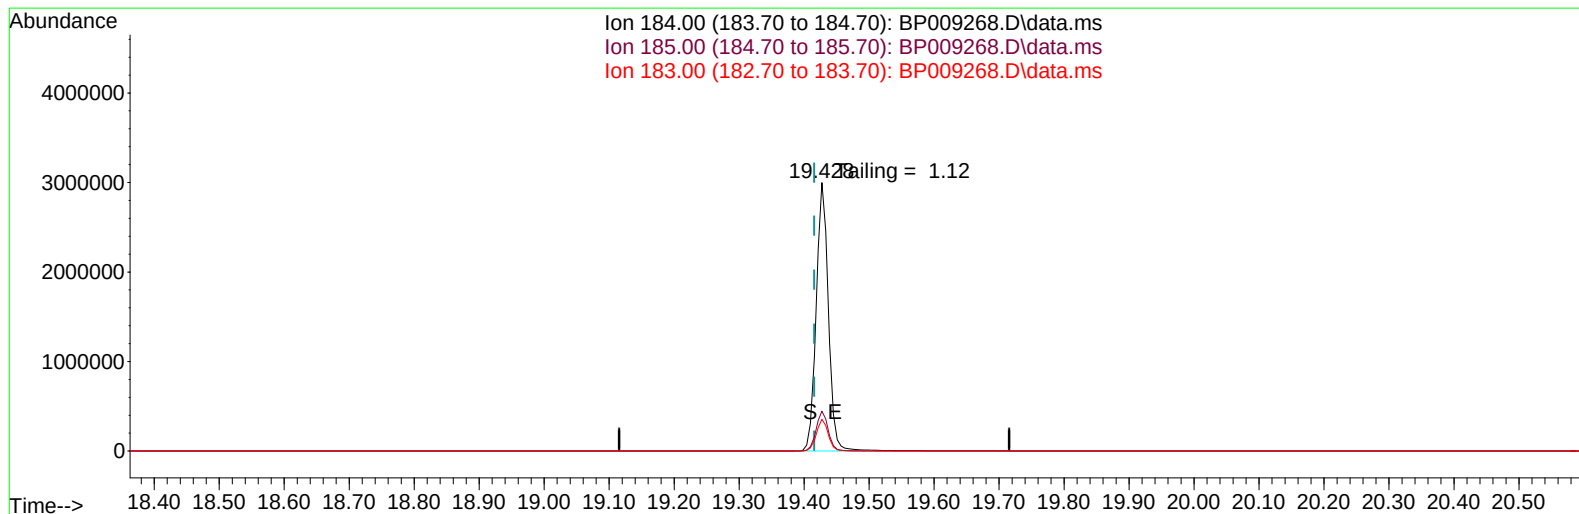

TIC: BP009268.D\data.ms

(77) Benzidine**19.427min (+ 0.012) 51823.59 ng****response 3937855**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.85
183.00	11.70	11.80
0.00	0.00	0.00