
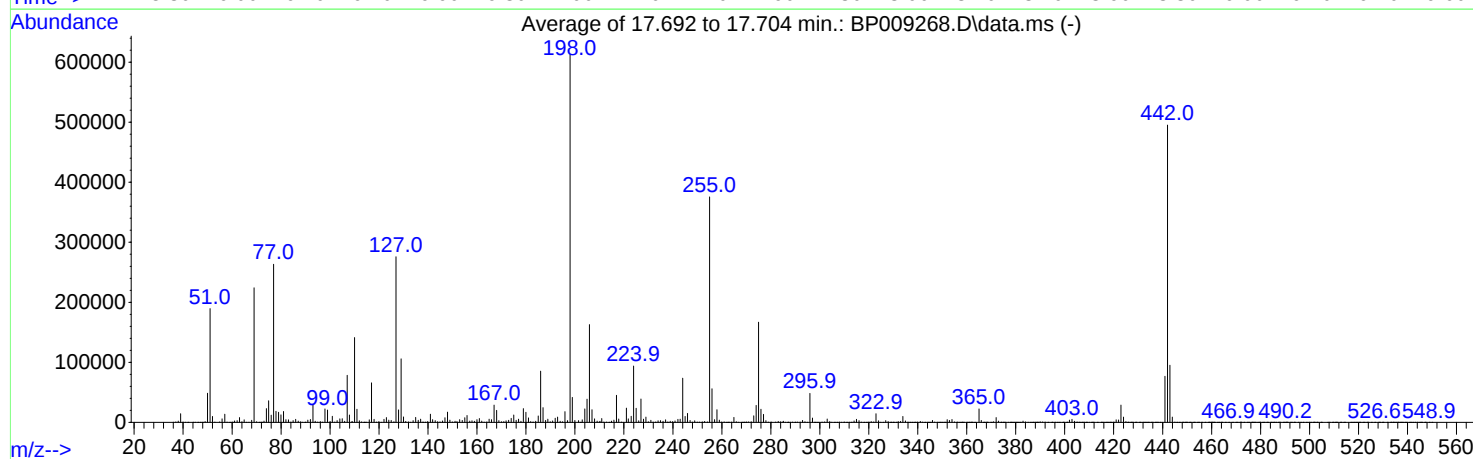


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP030522\  
 Data File : BP009268.D  
 Acq On : 04 Mar 2022 15:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP030522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Mar 05 01:55:59 2022

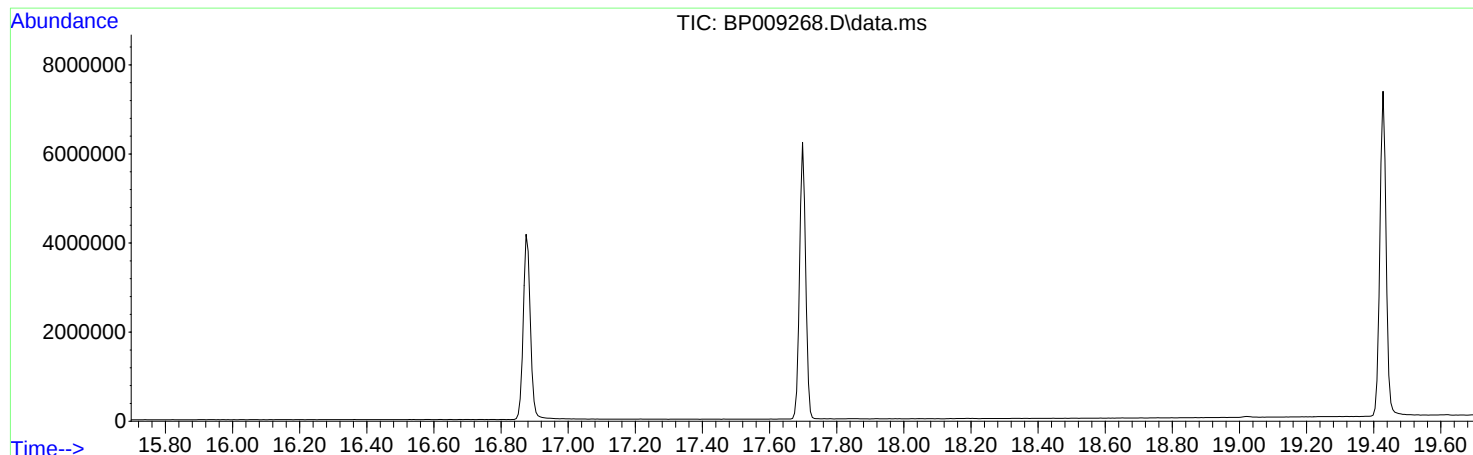




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2490

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 30.9         | 189609     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 3553       | PASS                |
| 69             | 198             | 0.00            | 100             | 36.6         | 224290     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1208       | PASS                |
| 127            | 198             | 10              | 80              | 45.0         | 275772     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 2884       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 612757     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 41661      | PASS                |
| 275            | 198             | 10              | 60              | 27.2         | 166763     | PASS                |
| 365            | 198             | 1               | 100             | 3.7          | 22368      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.5         | 76857      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 495339     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 95217      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP030522\  
 Data File : BP009268.D  
 Acq On : 04 Mar 2022 15:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 05 05:02:23 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP030522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Mar 05 01:55:59 2022  
 Response via : Initial Calibration

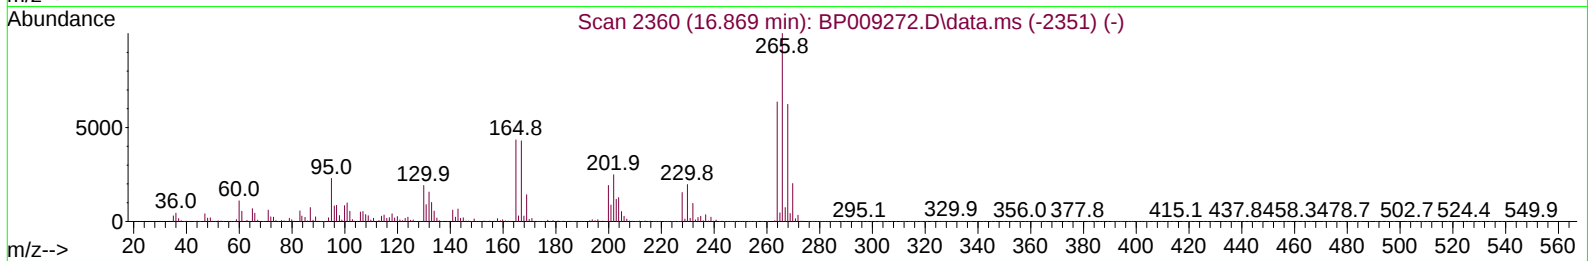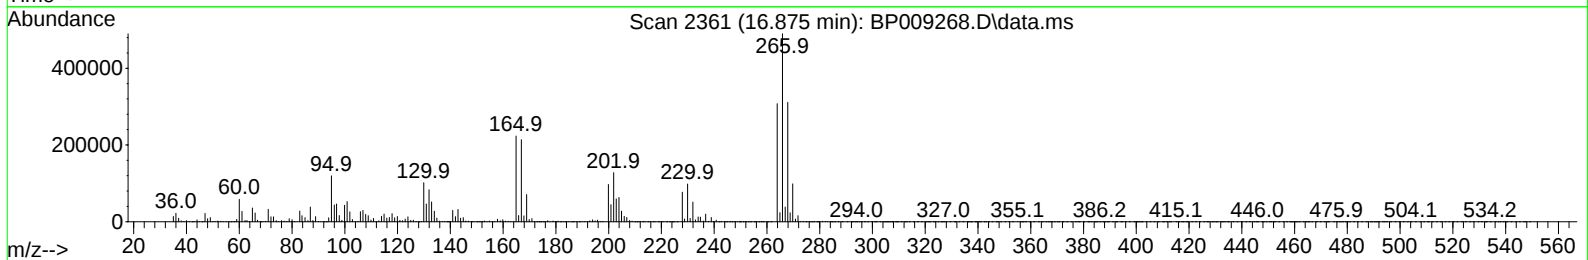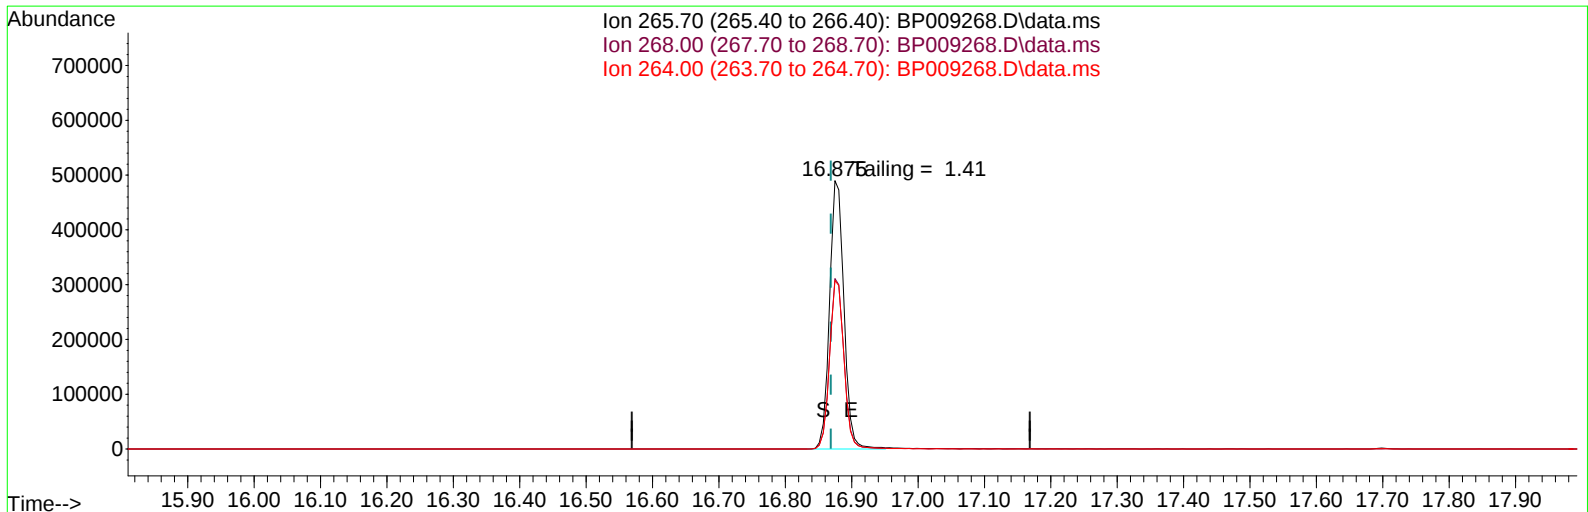

TIC: BP009268.D\data.ms

**(70) Pentachlorophenol (C)**

16.875min (+ 0.006) 59220.11 ng




response 739715

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.30  | 63.52  |
| 264.00 | 63.60  | 62.78  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP030522\  
 Data File : BP009268.D  
 Acq On : 04 Mar 2022 15:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 05 05:02:23 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP030522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Mar 05 01:55:59 2022  
 Response via : Initial Calibration

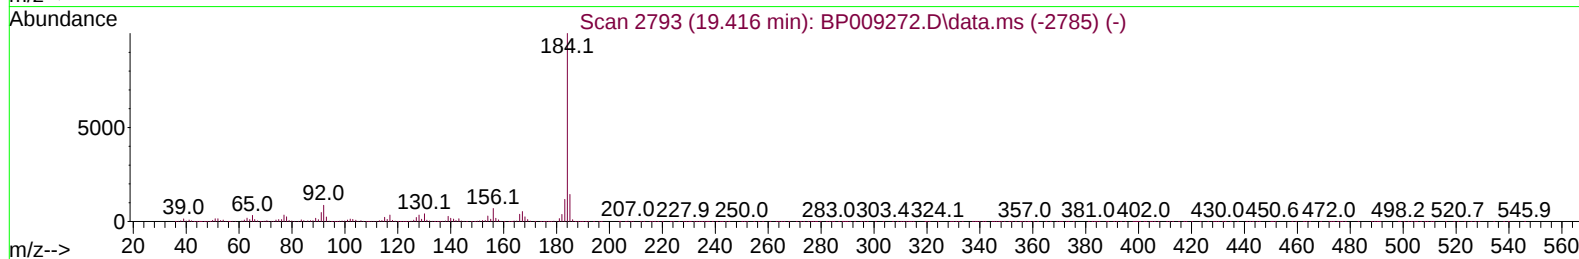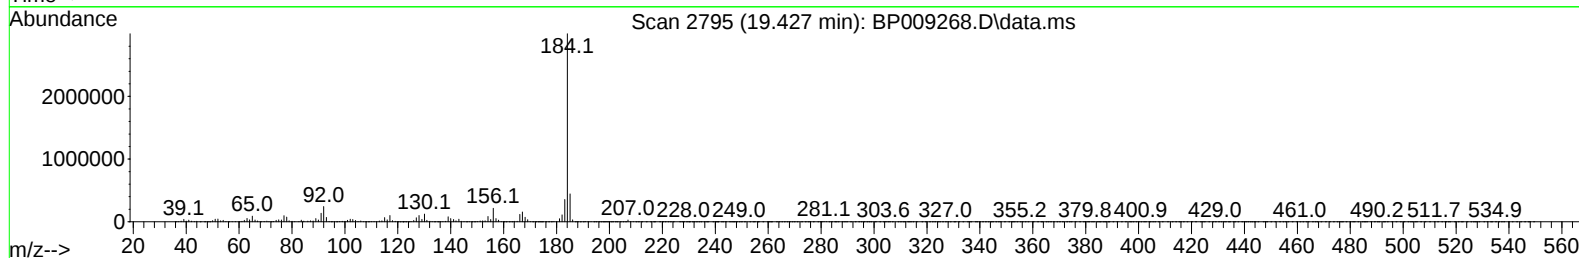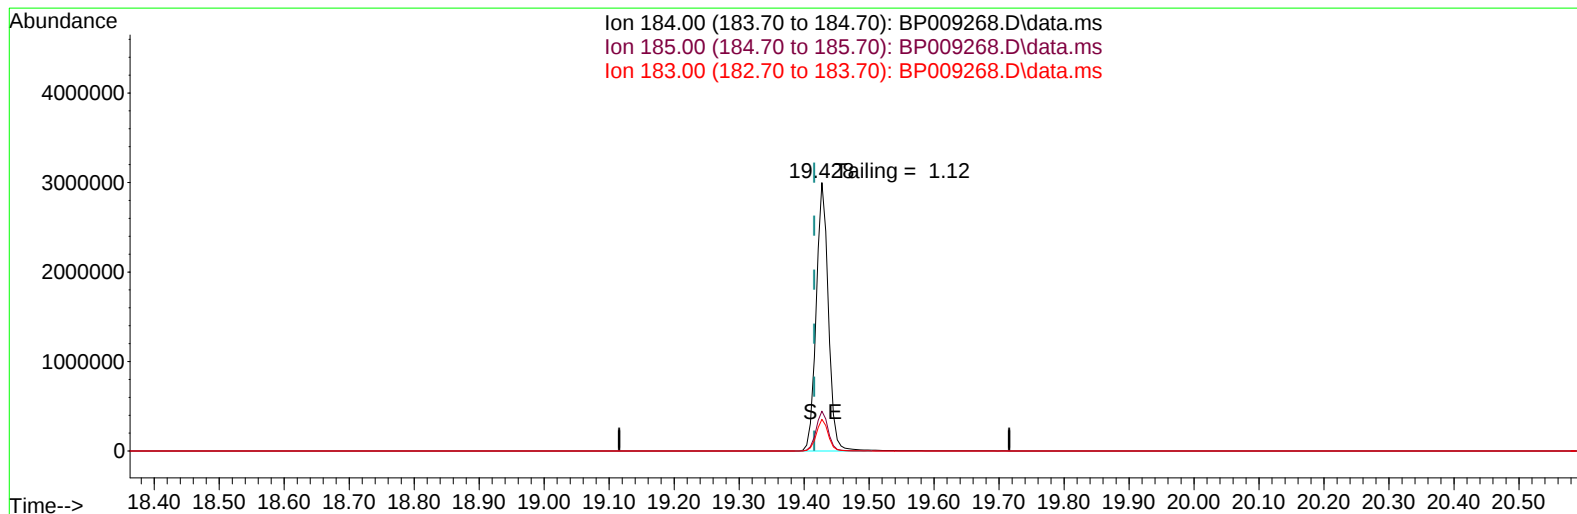

TIC: BP009268.D\data.ms

**(77) Benzidine**

**19.427min (+ 0.012) 51823.59 ng**

**response 3937855**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.85  |
| 183.00 | 11.70  | 11.80  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/5/2022      | BNA_P            | <u>BP009268.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2018015          | 20.645             |
| DDD           | 23473            | 20.21              |
| DDE           | 725              | 19.71              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 24198         | 2042213          | 1.18               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP