

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002096.D
 Acq On : 06 Mar 2020 14:42
 Operator : CG/JU
 Sample : L1780-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DG7

Quant Time: Mar 06 16:18:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 06:21:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	225643	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	907952	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	578652	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1252924	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1266817	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1435691	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.17	96	4981	0.95	ng/uL	0.00
5) Phenol-d5	6.82	99	272108	15.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	222594	24.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	322676	21.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	268445	18.98	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	157672	22.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	166354	21.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	339126	22.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	276658	16.70	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1095895	25.02	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1303951	24.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	71603	8.55	ng/ul	0.00
58) Fluorene-d10	15.27	176	997135	26.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	91118	13.19	ng/ul	0.00
71) Anthracene-d10	17.12	188	1534744	27.25	ng/ul	0.00
79) Pyrene-d10	19.37	212	1792780	27.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1802579	24.54	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	103275	2.285	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002096.D
Acq On : 06 Mar 2020 14:42
Operator : CG/JU
Sample : L1780-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0DG7

Quant Time: Mar 06 16:18:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

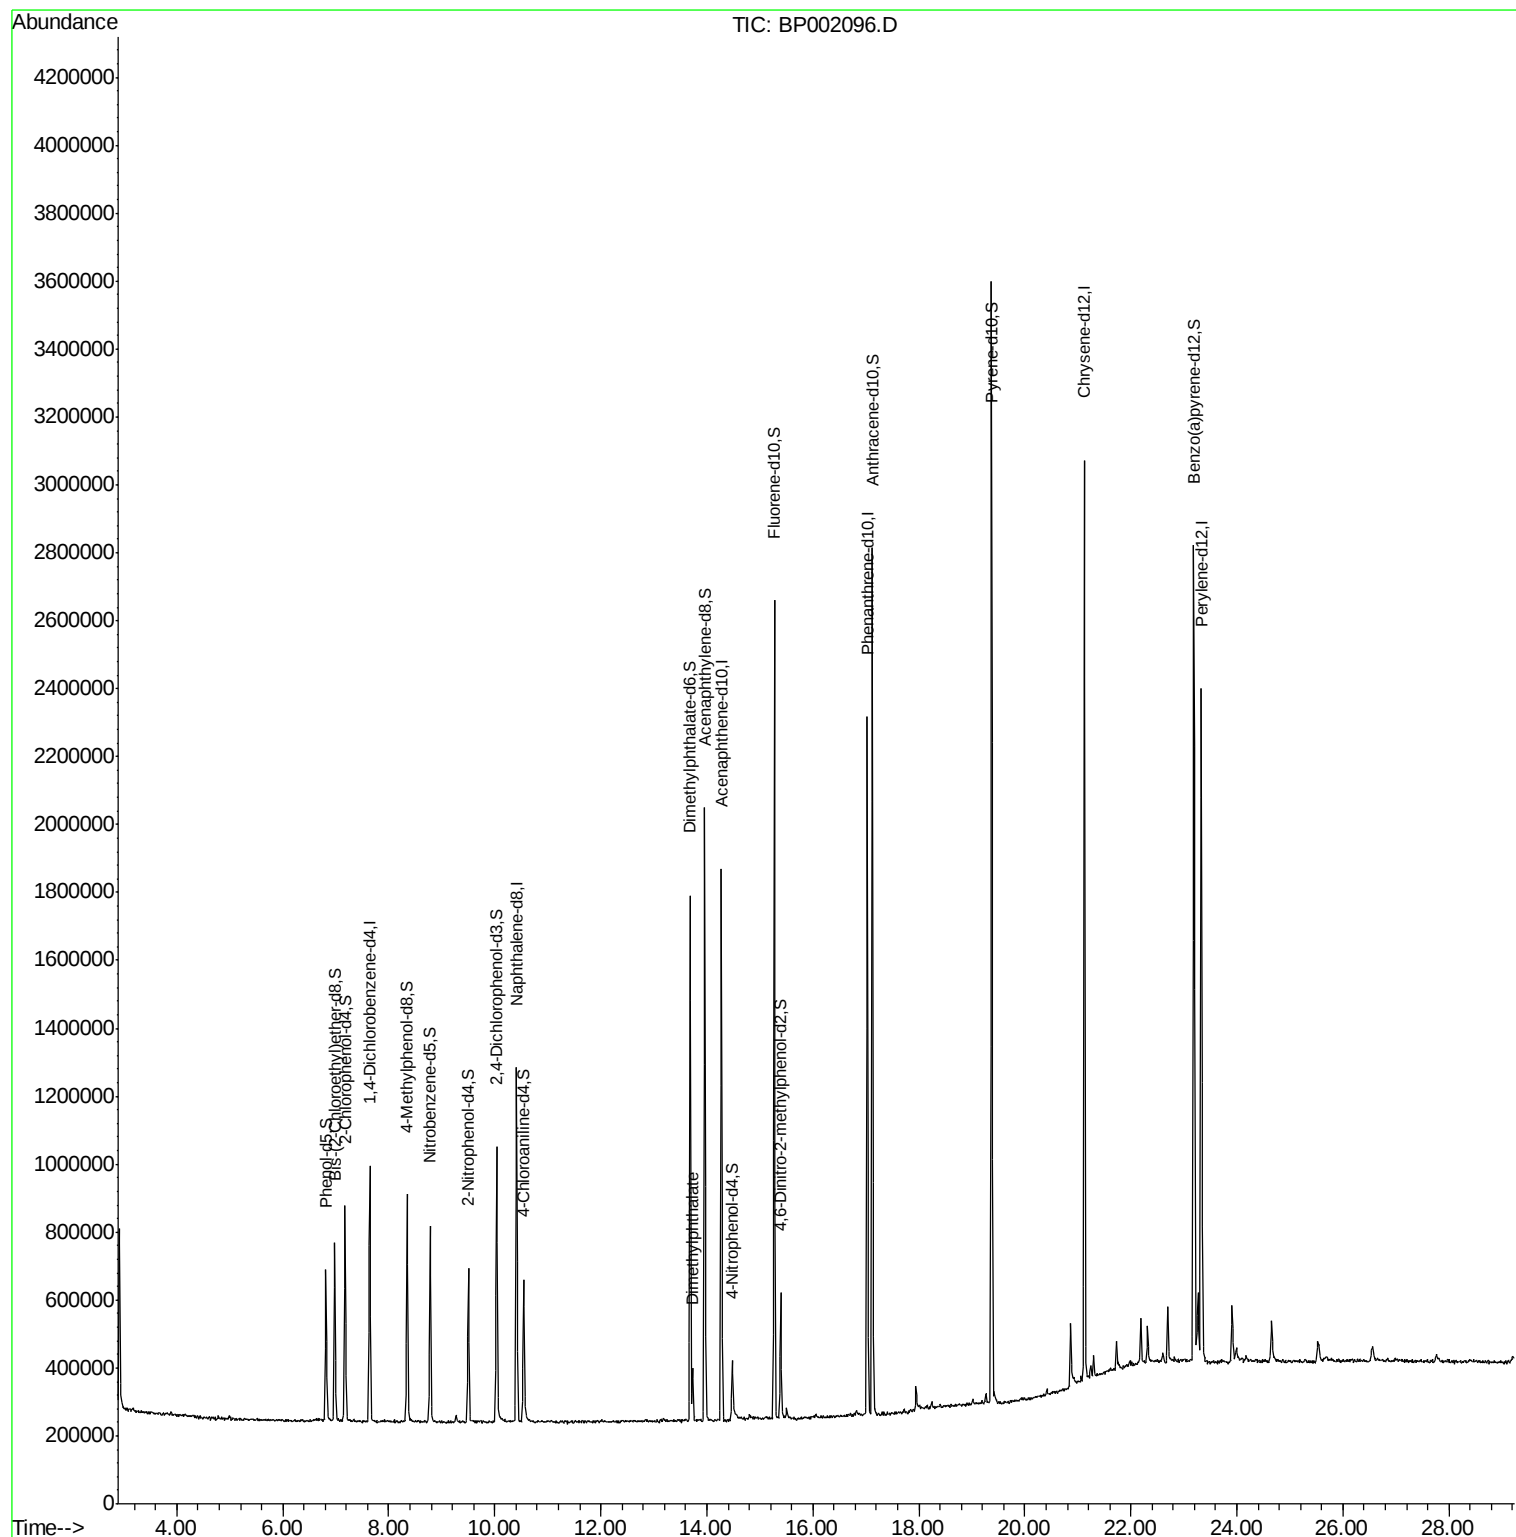

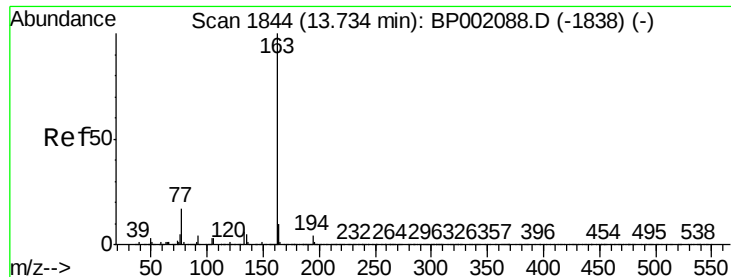

#45

Dimethylphthalate

Concen: 2.285 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002096.D

Acq: 06 Mar 2020 14:42

Instrument :

BNA_P

ClientSampleId :

C0DG7


Tot Ion:163 Resp: 103275

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4

164 10.5 8.2 12.4

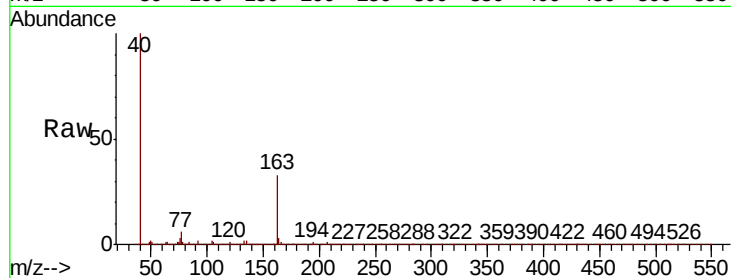

Abundance Ion 163.00 (162.70 to 163.70): E

100000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

