

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002103.D
 Acq On : 06 Mar 2020 18:46
 Operator : CG/JU
 Sample : L1782-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA9

Quant Time: Mar 07 01:53:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	258938	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1083294	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	684307	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1450986	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1399619	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1565672	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	36060	5.99	ng/uL	0.00
5) Phenol-d5	6.82	99	165673	8.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	396114	37.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	512924	30.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	315767	19.45	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	294432	35.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	314983	33.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	596916	33.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	43241	2.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1971732	38.07	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2343257	37.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	36986	3.74	ng/ul	0.00
58) Fluorene-d10	15.27	176	1757143	39.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	203394	25.43	ng/ul	0.00
71) Anthracene-d10	17.12	188	2680763	41.11	ng/ul	0.00
79) Pyrene-d10	19.37	212	3115463	42.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3402516	42.48	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	117834	2.204	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002103.D
Acq On : 06 Mar 2020 18:46
Operator : CG/JU
Sample : L1782-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA9

Quant Time: Mar 07 01:53:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

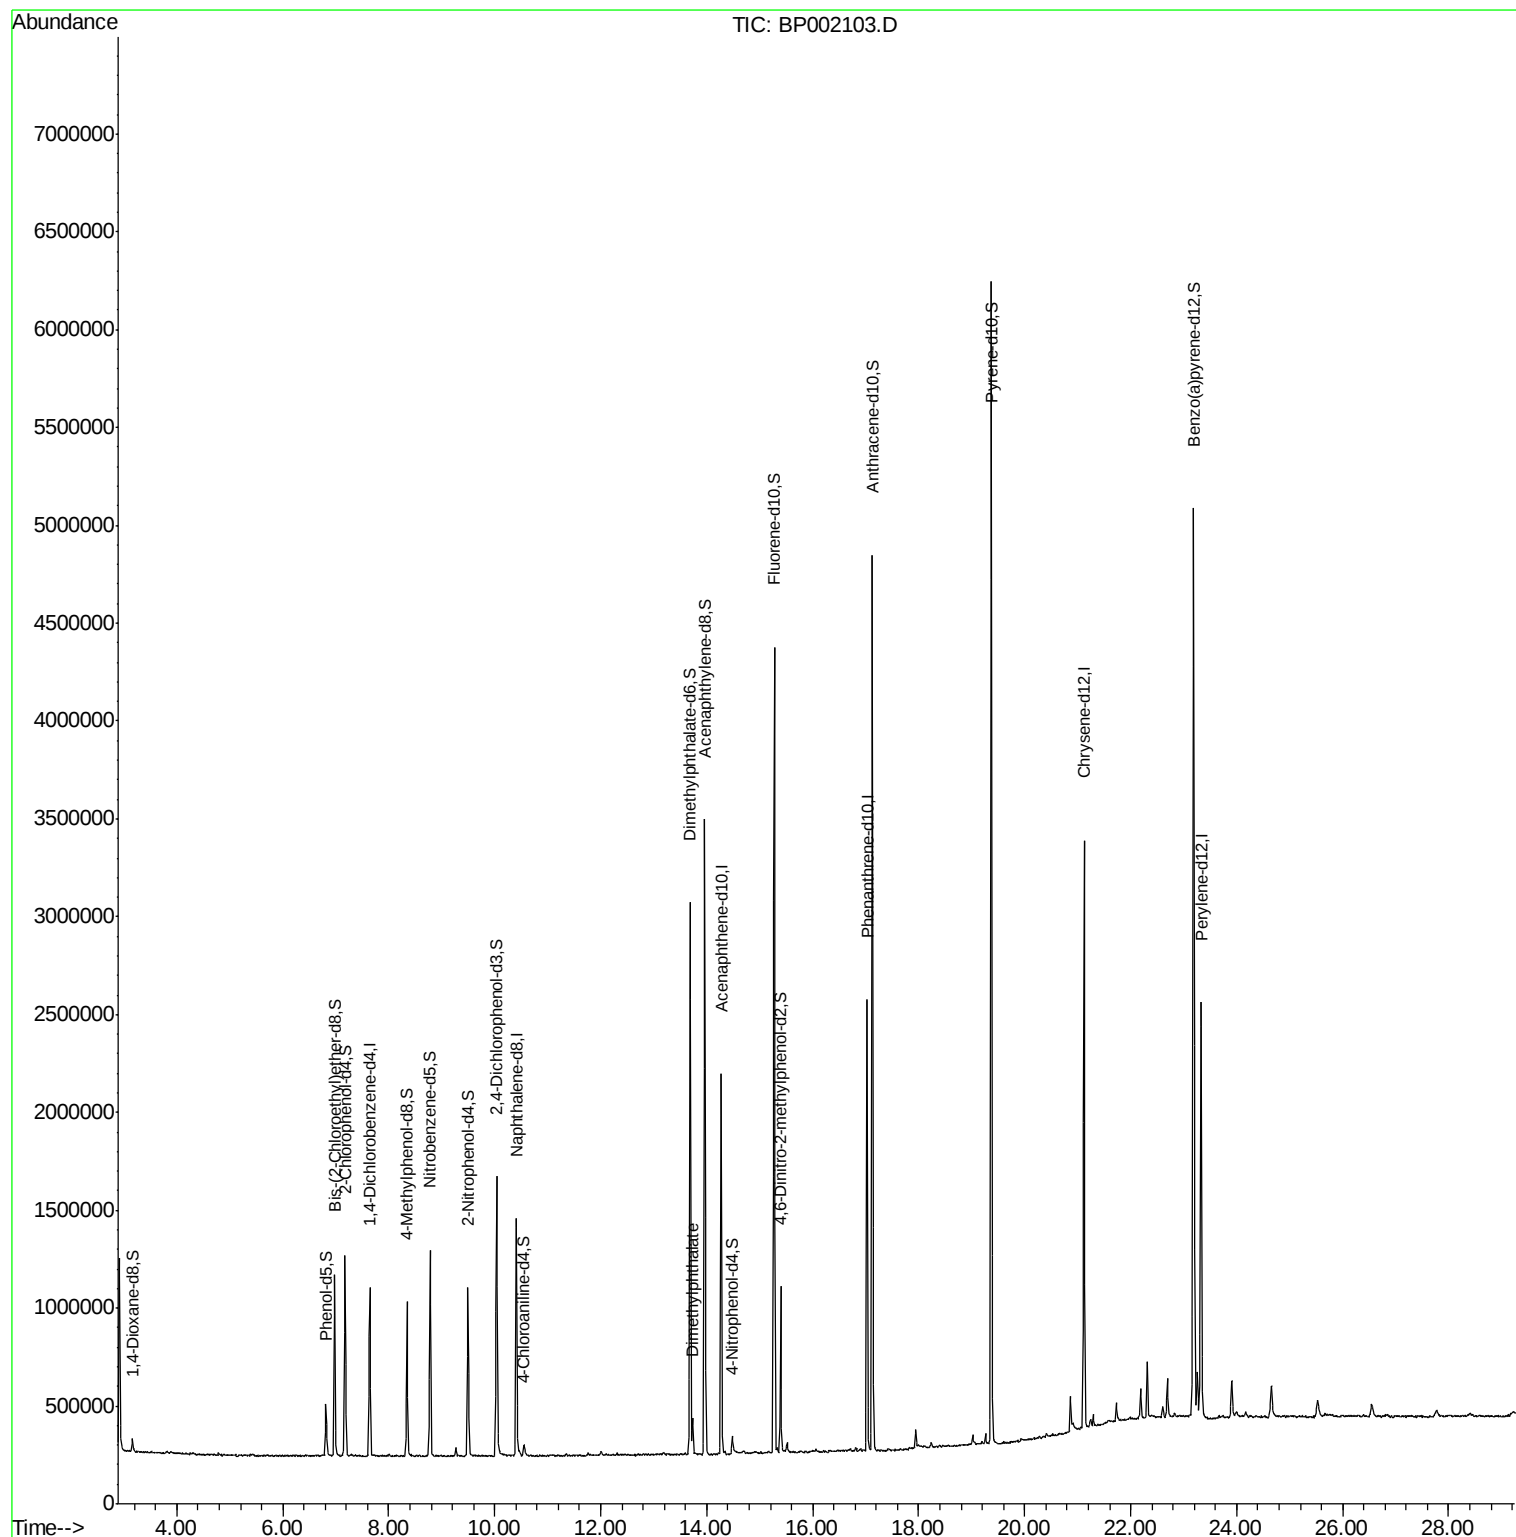

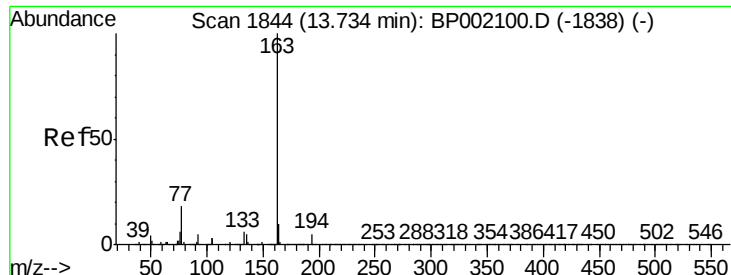

#45

Dimethylphthalate

Concen: 2.204 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002103.D

Acq: 06 Mar 2020 18:46

Instrument :

BNA_P

ClientSampleId :

C0AA9


Tot Ion:163 Resp: 117834

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4

164 10.7 8.2 12.4

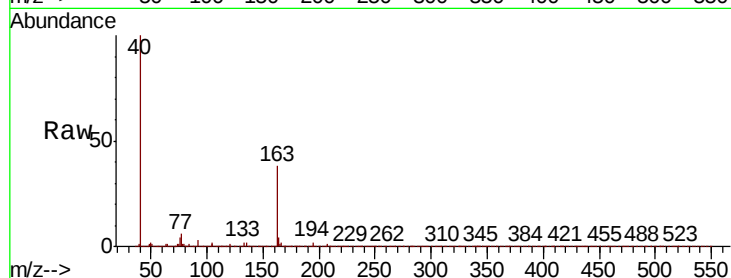

Abundance Ion 163.00 (162.70 to 163.70): E

120000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

