

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002105.D
 Acq On : 06 Mar 2020 19:54
 Operator : CG/JU
 Sample : L1782-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB1

Quant Time: Mar 07 01:57:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	267051	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1117251	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	711753	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1569252	20.00	ng/ul	-0.01
78) Chrysene-d12	21.12	240	1579603	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1809307	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	29575	4.76	ng/uL	0.00
5) Phenol-d5	6.82	99	131553	6.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	356370	33.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	450899	25.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	266936	15.95	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	266669	31.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	283963	29.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	528877	28.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	36677	1.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1807678	33.56	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2146397	33.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	30713	2.98	ng/ul	0.00
58) Fluorene-d10	15.27	176	1609720	34.54	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	193591	22.38	ng/ul	0.00
71) Anthracene-d10	17.12	188	2524550	35.79	ng/ul	0.00
79) Pyrene-d10	19.37	212	2993220	36.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3343081	36.11	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	109994	1.978	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002105.D
Acq On : 06 Mar 2020 19:54
Operator : CG/JU
Sample : L1782-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB1

Quant Time: Mar 07 01:57:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

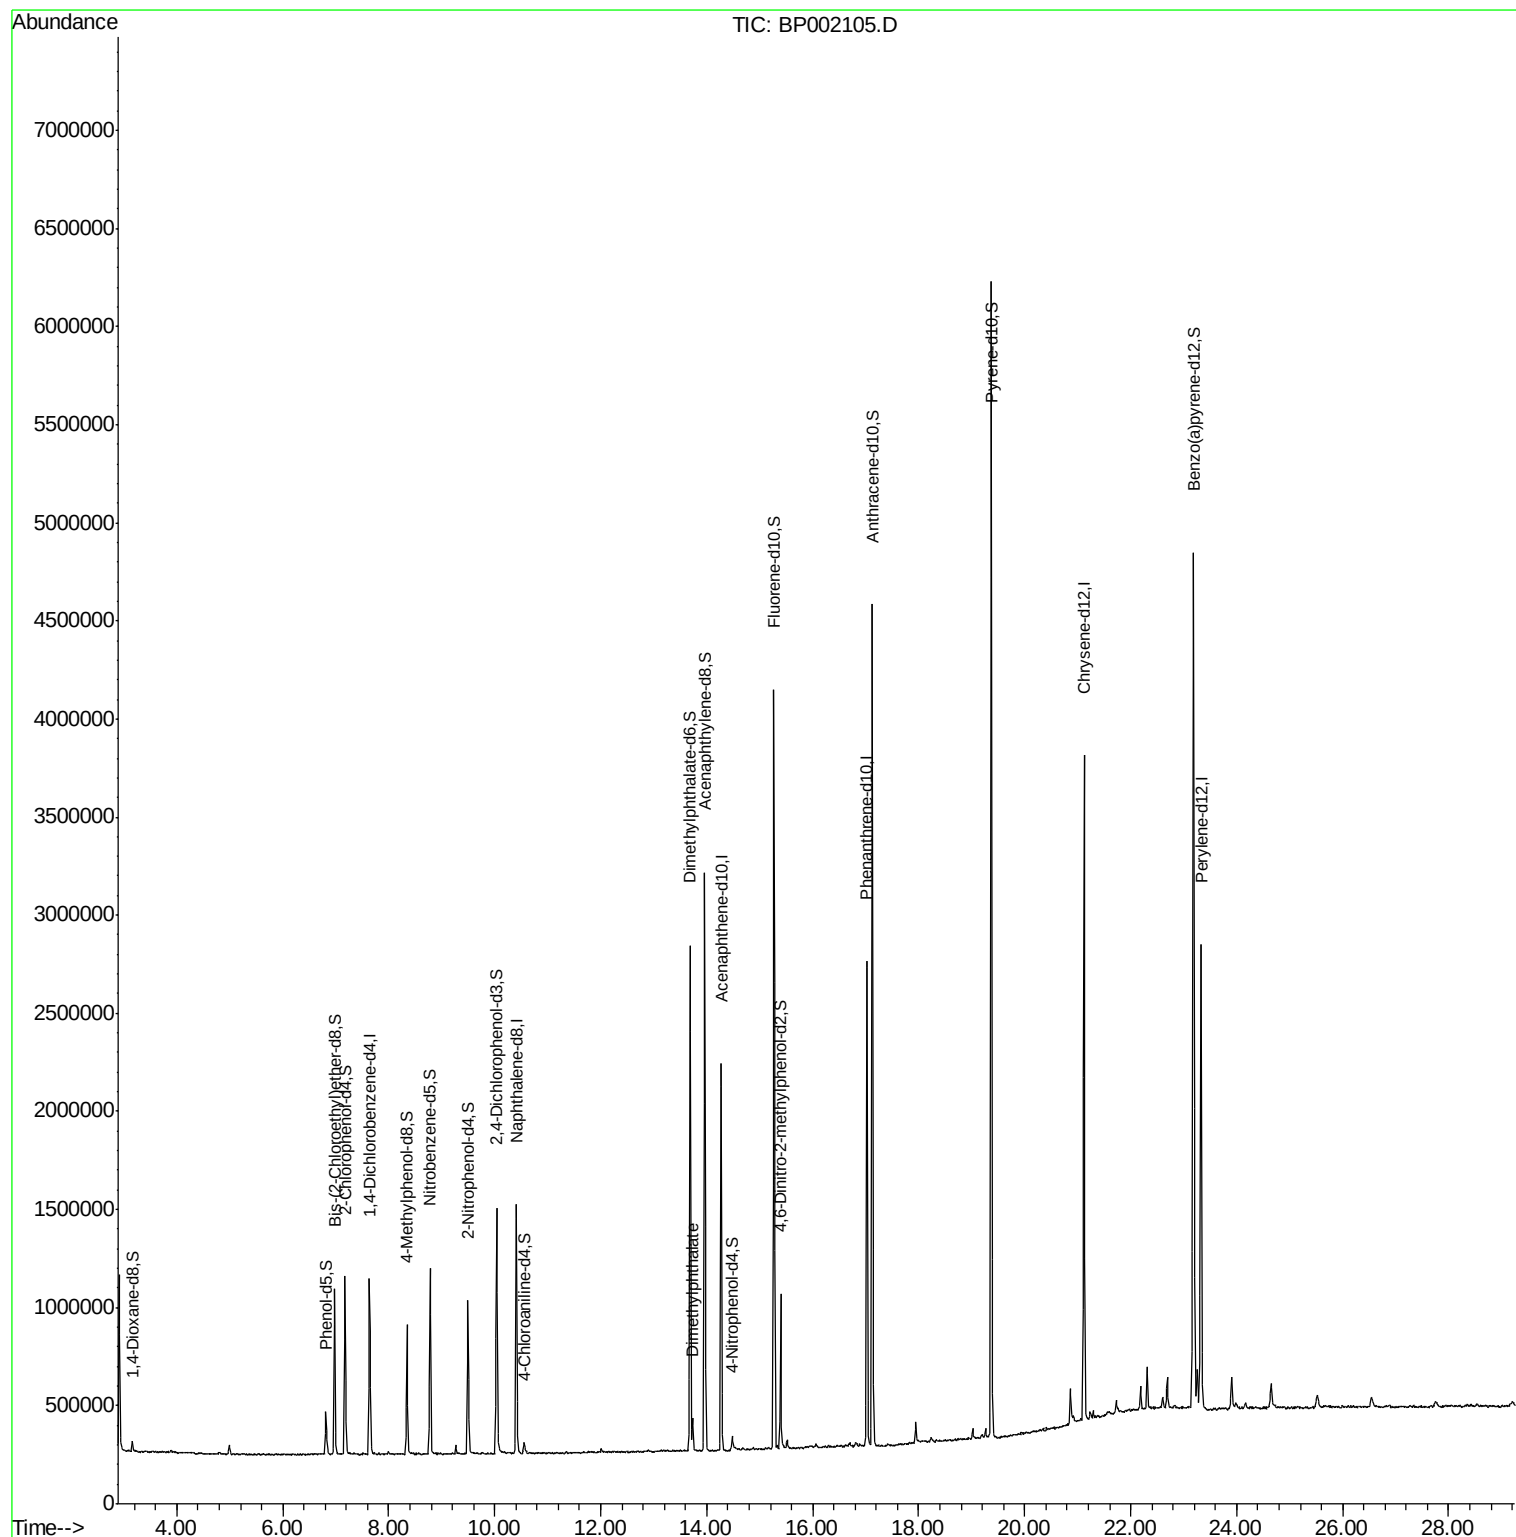

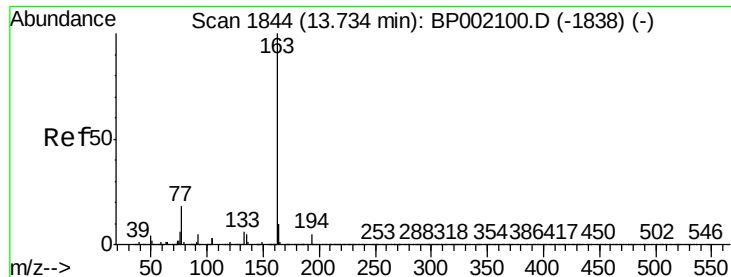

#45

Dimethylphthalate

Concen: 1.978 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002105.D

Acq: 06 Mar 2020 19:54

Instrument :

BNA_P

ClientSampleId :

C0AB1


Tot Ion:163 Resp: 109994

Ion Ratio Lower Upper

163 100

194 4.4 3.6 5.4

164 10.2 8.2 12.4

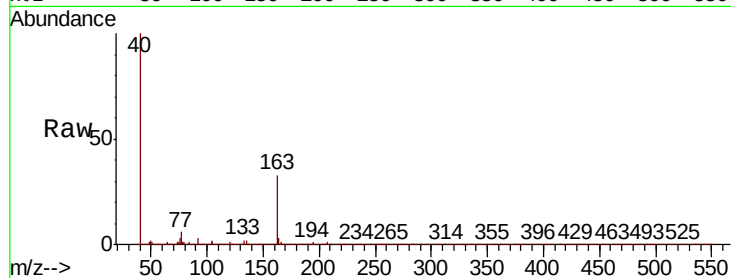

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

