

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002106.D
 Acq On : 06 Mar 2020 20:28
 Operator : CG/JU
 Sample : L1782-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Quant Time: Mar 07 02:00:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	264909	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1100615	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	693184	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1500232	20.00	ng/ul	-0.01
78) Chrysene-d12	21.12	240	1480932	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1681022	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	32556	5.28	ng/uL	0.00
5) Phenol-d5	6.82	99	147935	7.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	349213	32.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	455520	26.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	281421	16.95	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	256655	30.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	277907	29.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	522261	28.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	44400	2.21	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1726295	32.91	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2074180	33.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	31831	3.17	ng/ul	0.00
58) Fluorene-d10	15.27	176	1545344	34.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	176037	21.28	ng/ul	0.00
71) Anthracene-d10	17.12	188	2395305	35.52	ng/ul	0.00
79) Pyrene-d10	19.37	212	2782243	35.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3089830	35.93	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	86295	1.594	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002106.D
Acq On : 06 Mar 2020 20:28
Operator : CG/JU
Sample : L1782-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5

Quant Time: Mar 07 02:00:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

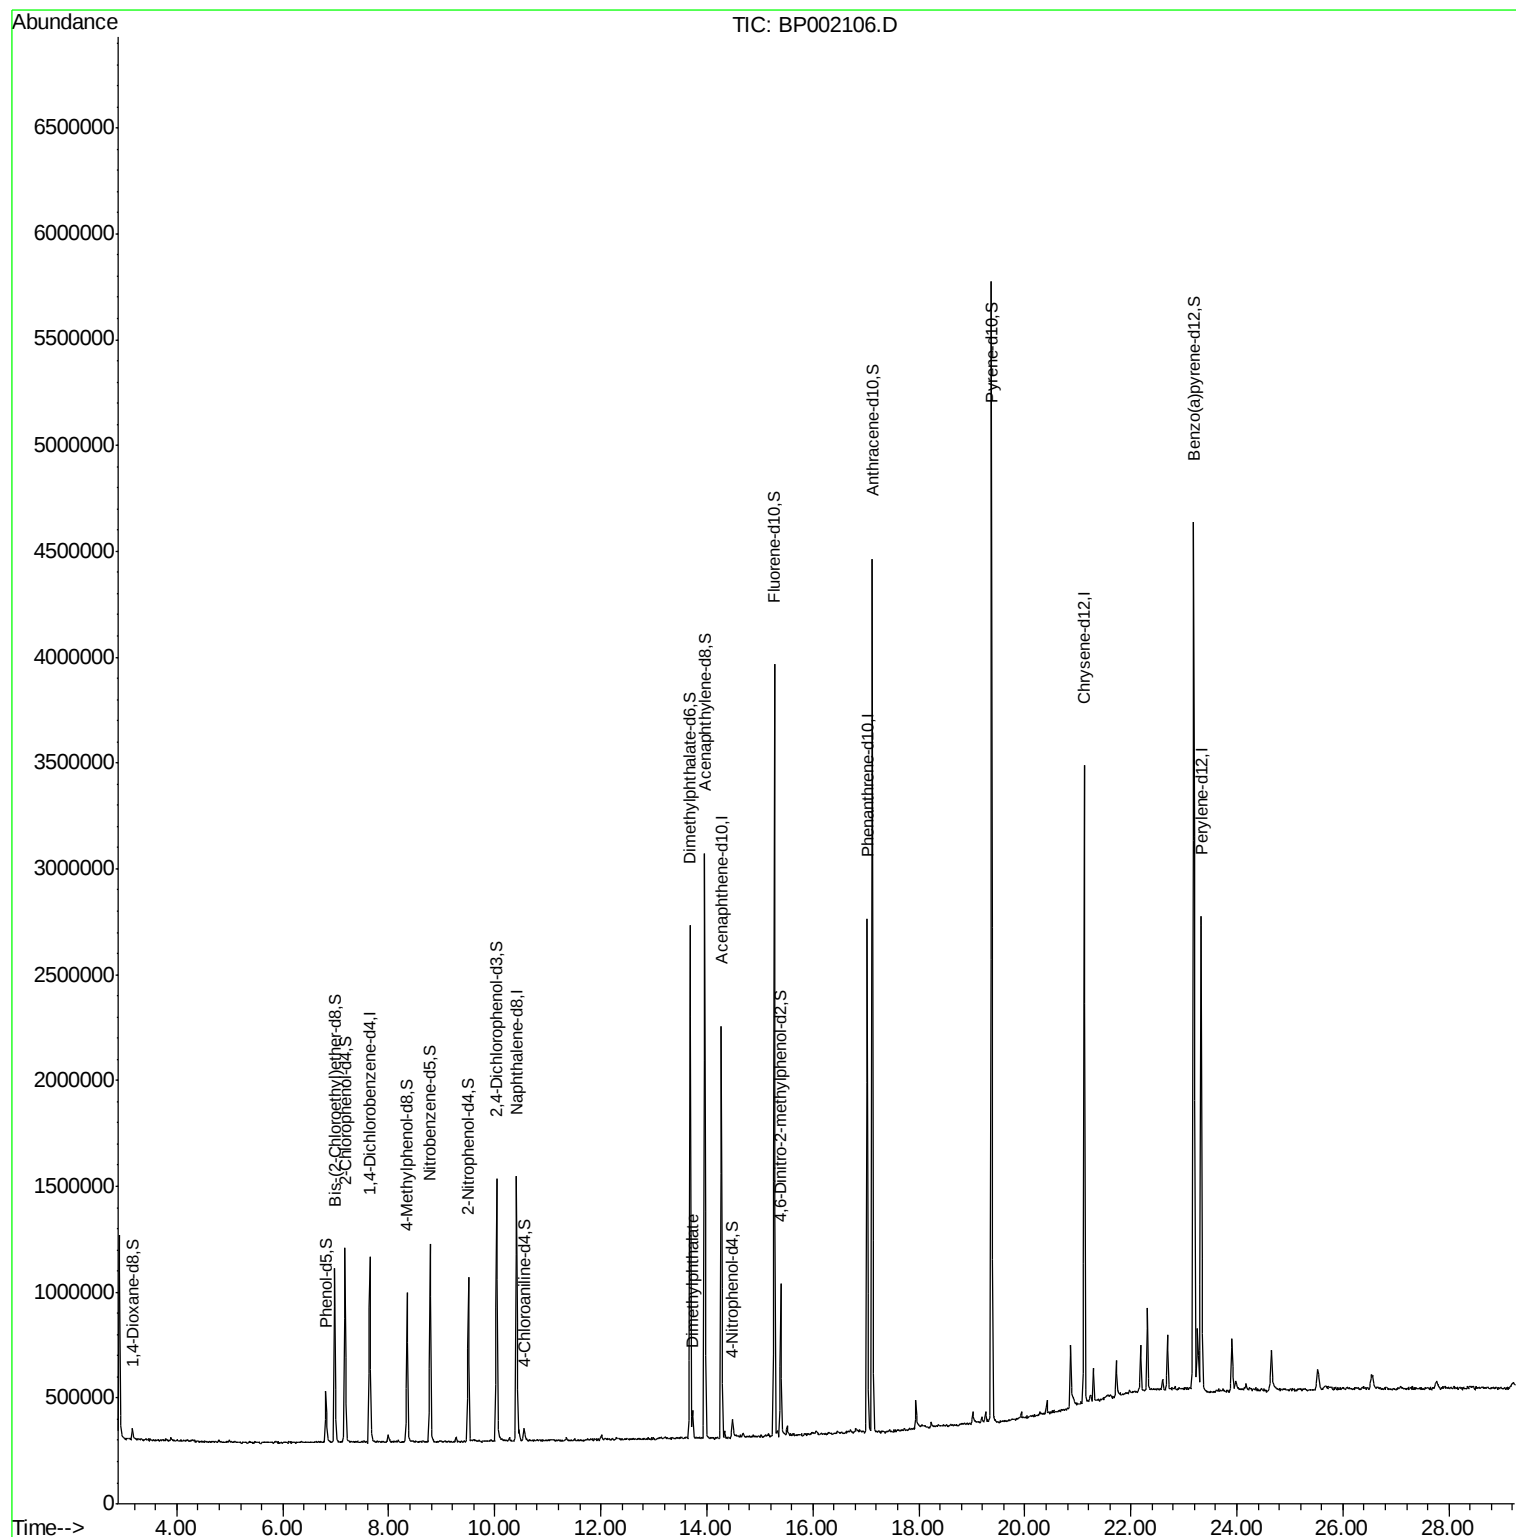

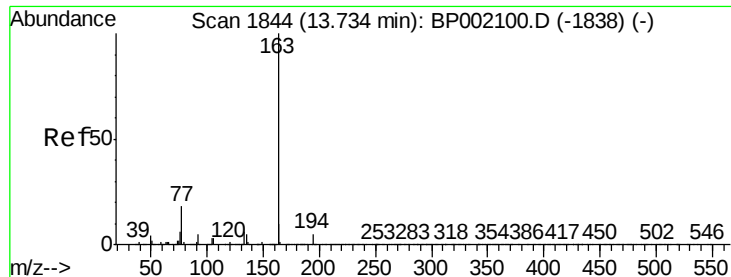

#45

Dimethylphthalate

Concen: 1.594 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002106.D

Acq: 06 Mar 2020 20:28

Instrument :

BNA_P

ClientSampleId :

C0AA5


Tot Ion:163 Resp: 86295

Ion Ratio Lower Upper

163 100

194 4.5 3.6 5.4

164 10.1 8.2 12.4

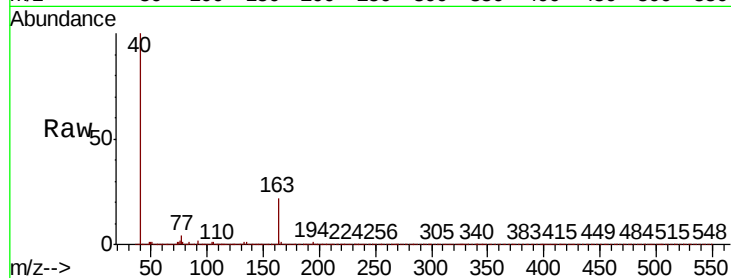

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

