

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002109.D
 Acq On : 06 Mar 2020 22:10
 Operator : CG/JU
 Sample : L1782-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA7

Quant Time: Mar 07 02:19:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	282055	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1171117	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	748296	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1609839	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1579202	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1740399	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	37311	5.69	ng/uL	0.00
5) Phenol-d5	6.82	99	150668	7.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	378516	33.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	491095	26.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	305209	17.26	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	287602	31.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	310782	30.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	588938	30.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	44123	2.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2044320	36.10	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2388015	35.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	40436	3.74	ng/ul	0.00
58) Fluorene-d10	15.27	176	1794917	36.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	221072	24.91	ng/ul	0.00
71) Anthracene-d10	17.12	188	2771257	38.30	ng/ul	0.00
79) Pyrene-d10	19.37	212	3246712	39.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3564327	40.03	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	79525	1.360	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002109.D
Acq On : 06 Mar 2020 22:10
Operator : CG/JU
Sample : L1782-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA7

Quant Time: Mar 07 02:19:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

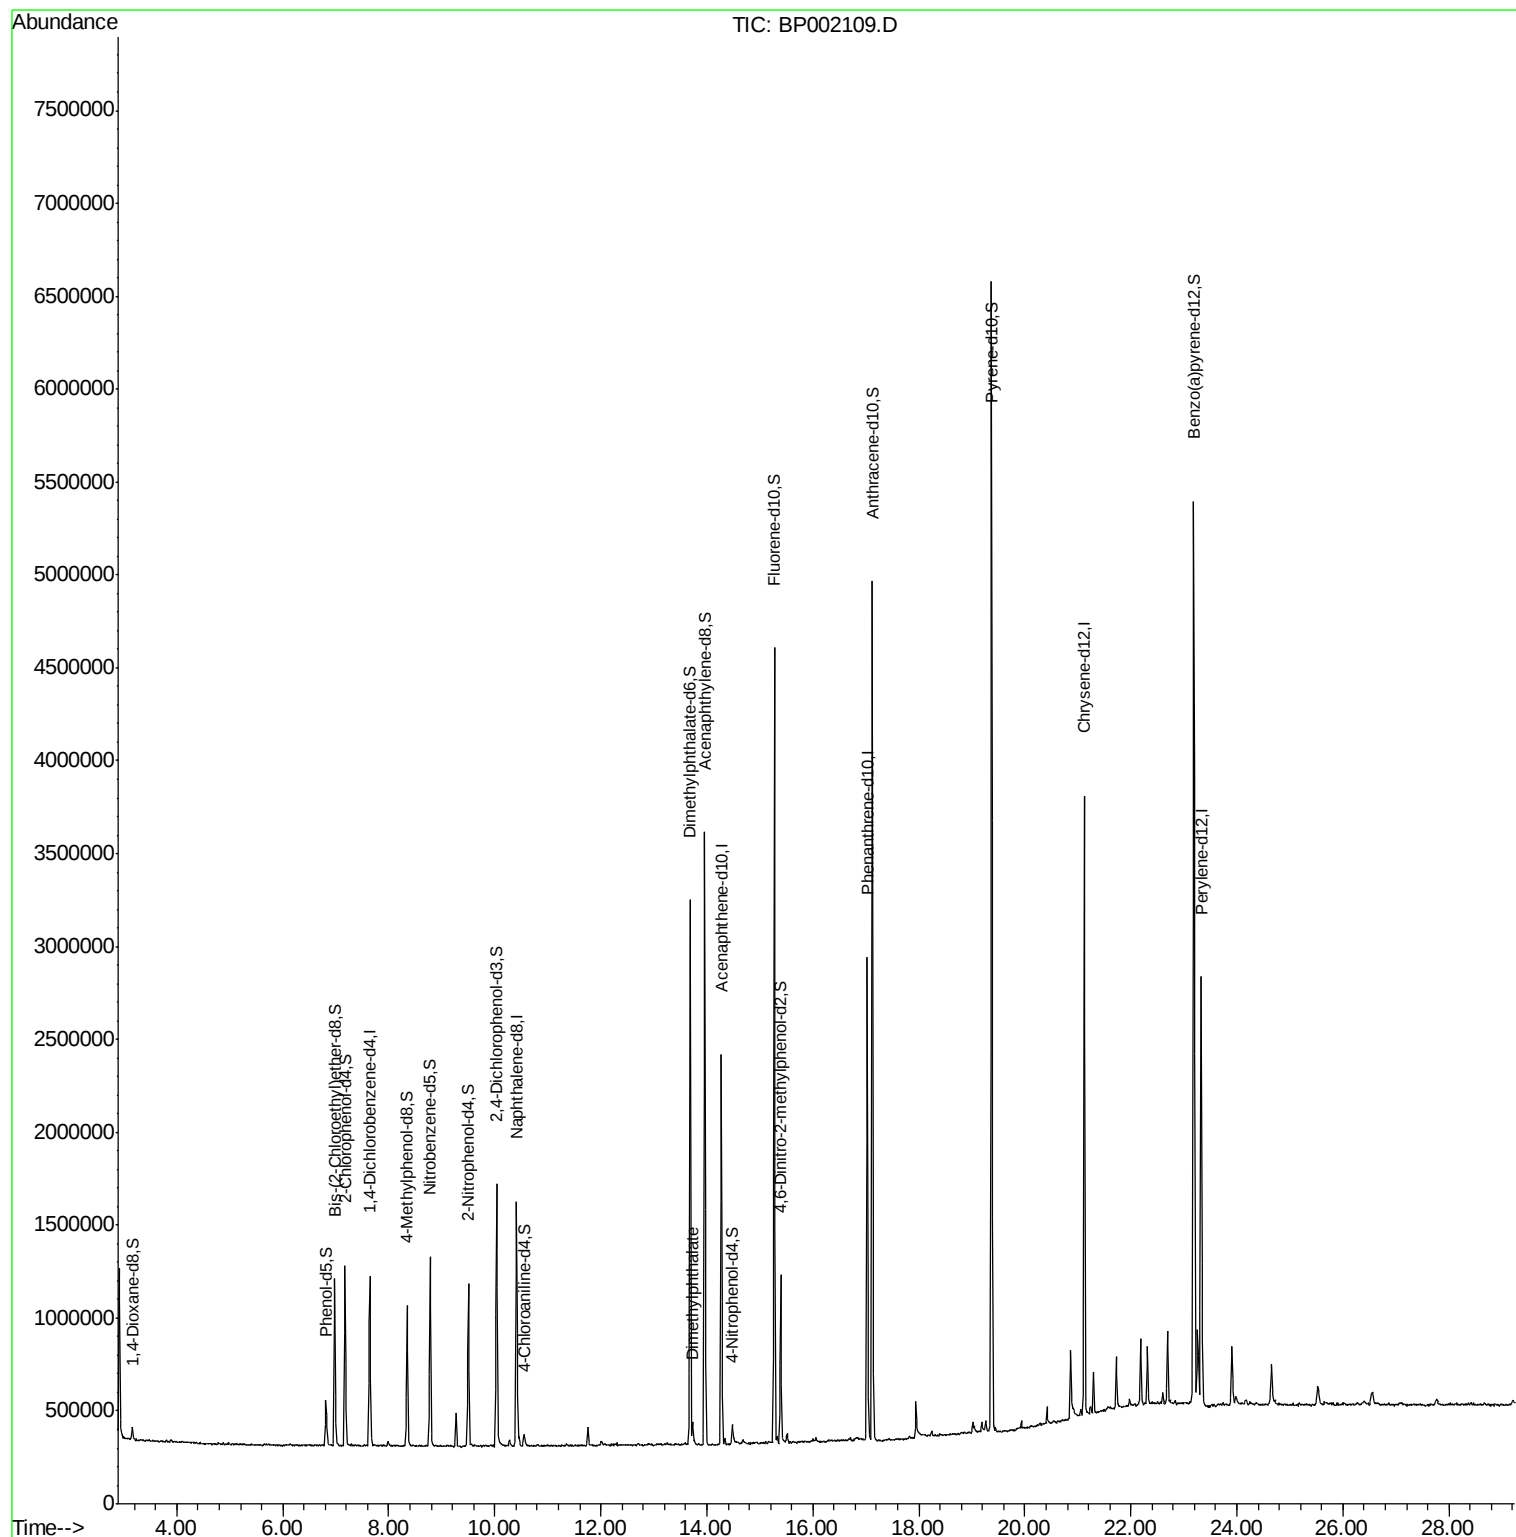

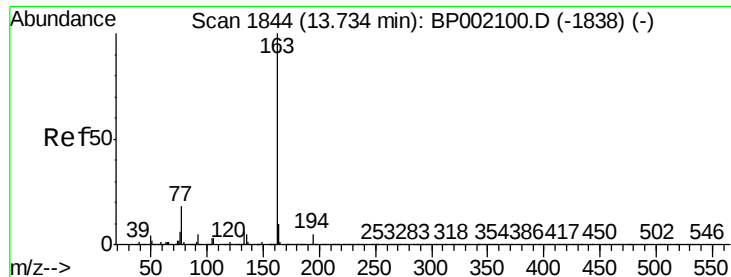

#45

Dimethylphthalate

Concen: 1.360 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002109.D

Acq: 06 Mar 2020 22:10

Instrument :

BNA_P

ClientSampleId :

C0AA7


Tot Ion:163 Resp: 79525

Ion Ratio Lower Upper

163 100

194 4.8 3.6 5.4

164 10.2 8.2 12.4

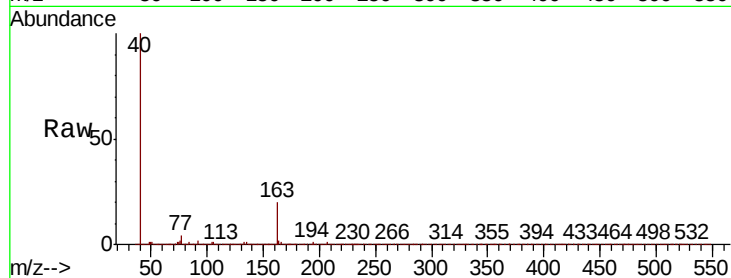

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

