

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002111.D
 Acq On : 06 Mar 2020 23:17
 Operator : CG/JU
 Sample : L1782-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Quant Time: Mar 07 02:24:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	285093	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1185630	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	752098	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1632231	20.00	ng/ul	-0.01
78) Chrysene-d12	21.12	240	1595882	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1812617	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	37460	5.65	ng/uL	0.00
5) Phenol-d5	6.82	99	154534	7.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	363217	31.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	472066	25.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	299297	16.75	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	270324	29.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	294654	28.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	553767	28.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	41507	1.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1890921	33.22	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2231201	32.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	37680	3.46	ng/ul	0.00
58) Fluorene-d10	15.27	176	1657583	33.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	194944	21.66	ng/ul	0.00
71) Anthracene-d10	17.12	188	2555084	34.83	ng/ul	0.00
79) Pyrene-d10	19.37	212	3004018	35.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3313091	35.73	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	99694	1.697	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002111.D
Acq On : 06 Mar 2020 23:17
Operator : CG/JU
Sample : L1782-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Time: Mar 07 02:24:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

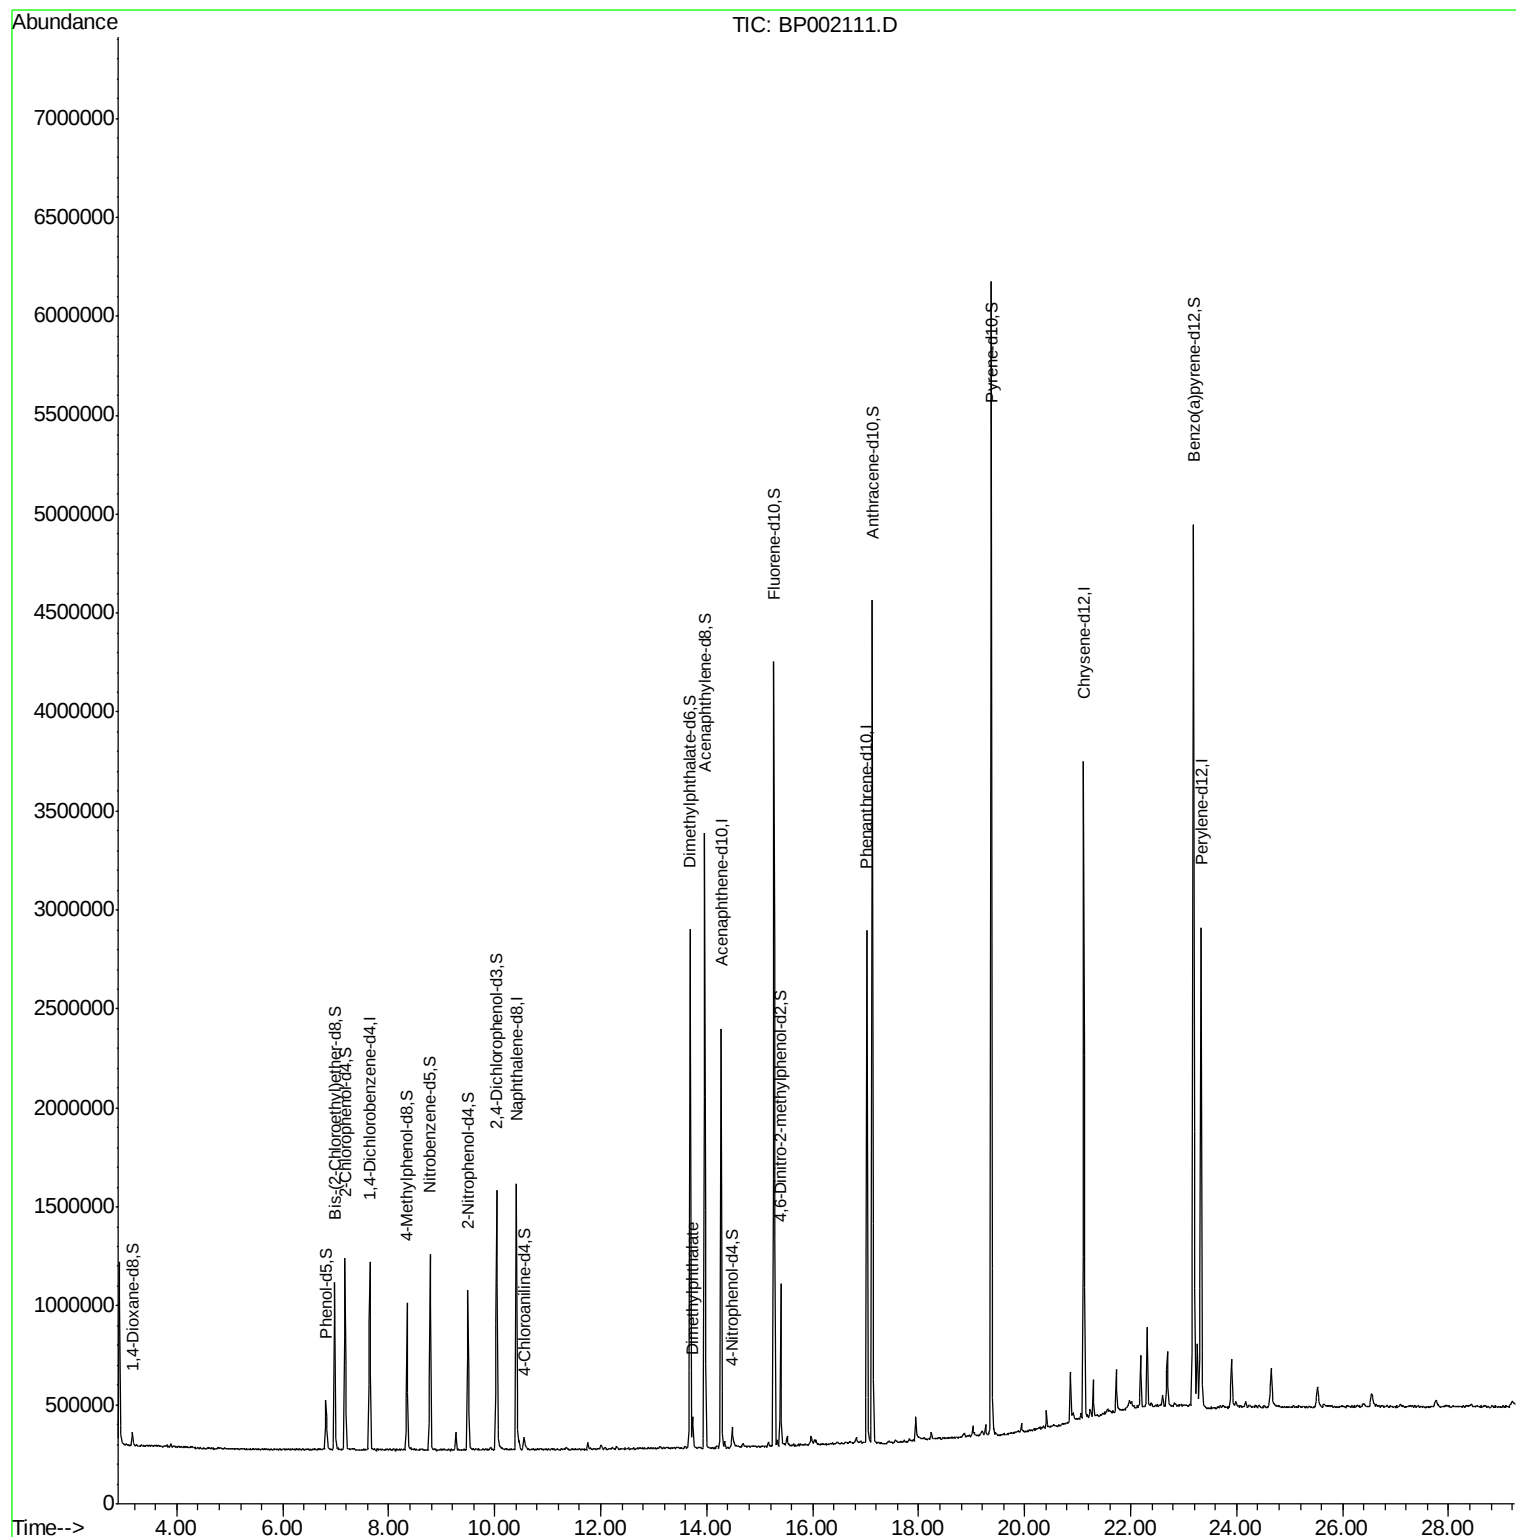

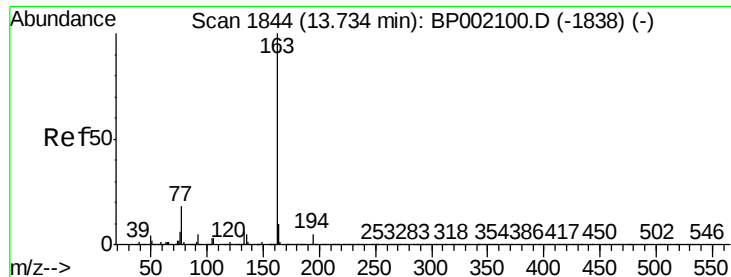

#45
 Dimethylphthalate
 Concen: 1.697 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. -0.01 min
 Lab File: BP002111.D
 Acq: 06 Mar 2020 23:17

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Tot Ion:	163	Resp:	99694
Ion	Ratio	Lower	Upper
163	100		
194	5.0	3.6	5.4
164	9.9	8.2	12.4

