

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002112.D
 Acq On : 06 Mar 2020 23:51
 Operator : CG/JU
 Sample : L1780-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DJ3

Quant Time: Mar 07 02:26:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 07 00:40:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	273883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1142760	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	740228	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1625074	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1660682	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1892838	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	35097	5.51	ng/uL	0.00
5) Phenol-d5	6.82	99	121111	5.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	312197	28.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	405459	22.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	238727	13.90	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	233299	26.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	248076	25.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	463318	24.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	33774	1.62	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1633220	29.15	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1917330	28.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	33132	3.09	ng/ul	0.00
58) Fluorene-d10	15.27	176	1492666	30.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	181290	20.24	ng/ul	0.00
71) Anthracene-d10	17.12	188	2494611	34.16	ng/ul	0.00
79) Pyrene-d10	19.37	212	2930721	33.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3296565	34.04	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	65471	1.132	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002112.D
Acq On : 06 Mar 2020 23:51
Operator : CG/JU
Sample : L1780-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0DJ3

Quant Time: Mar 07 02:26:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 07 00:40:34 2020
Response via : Initial Calibration

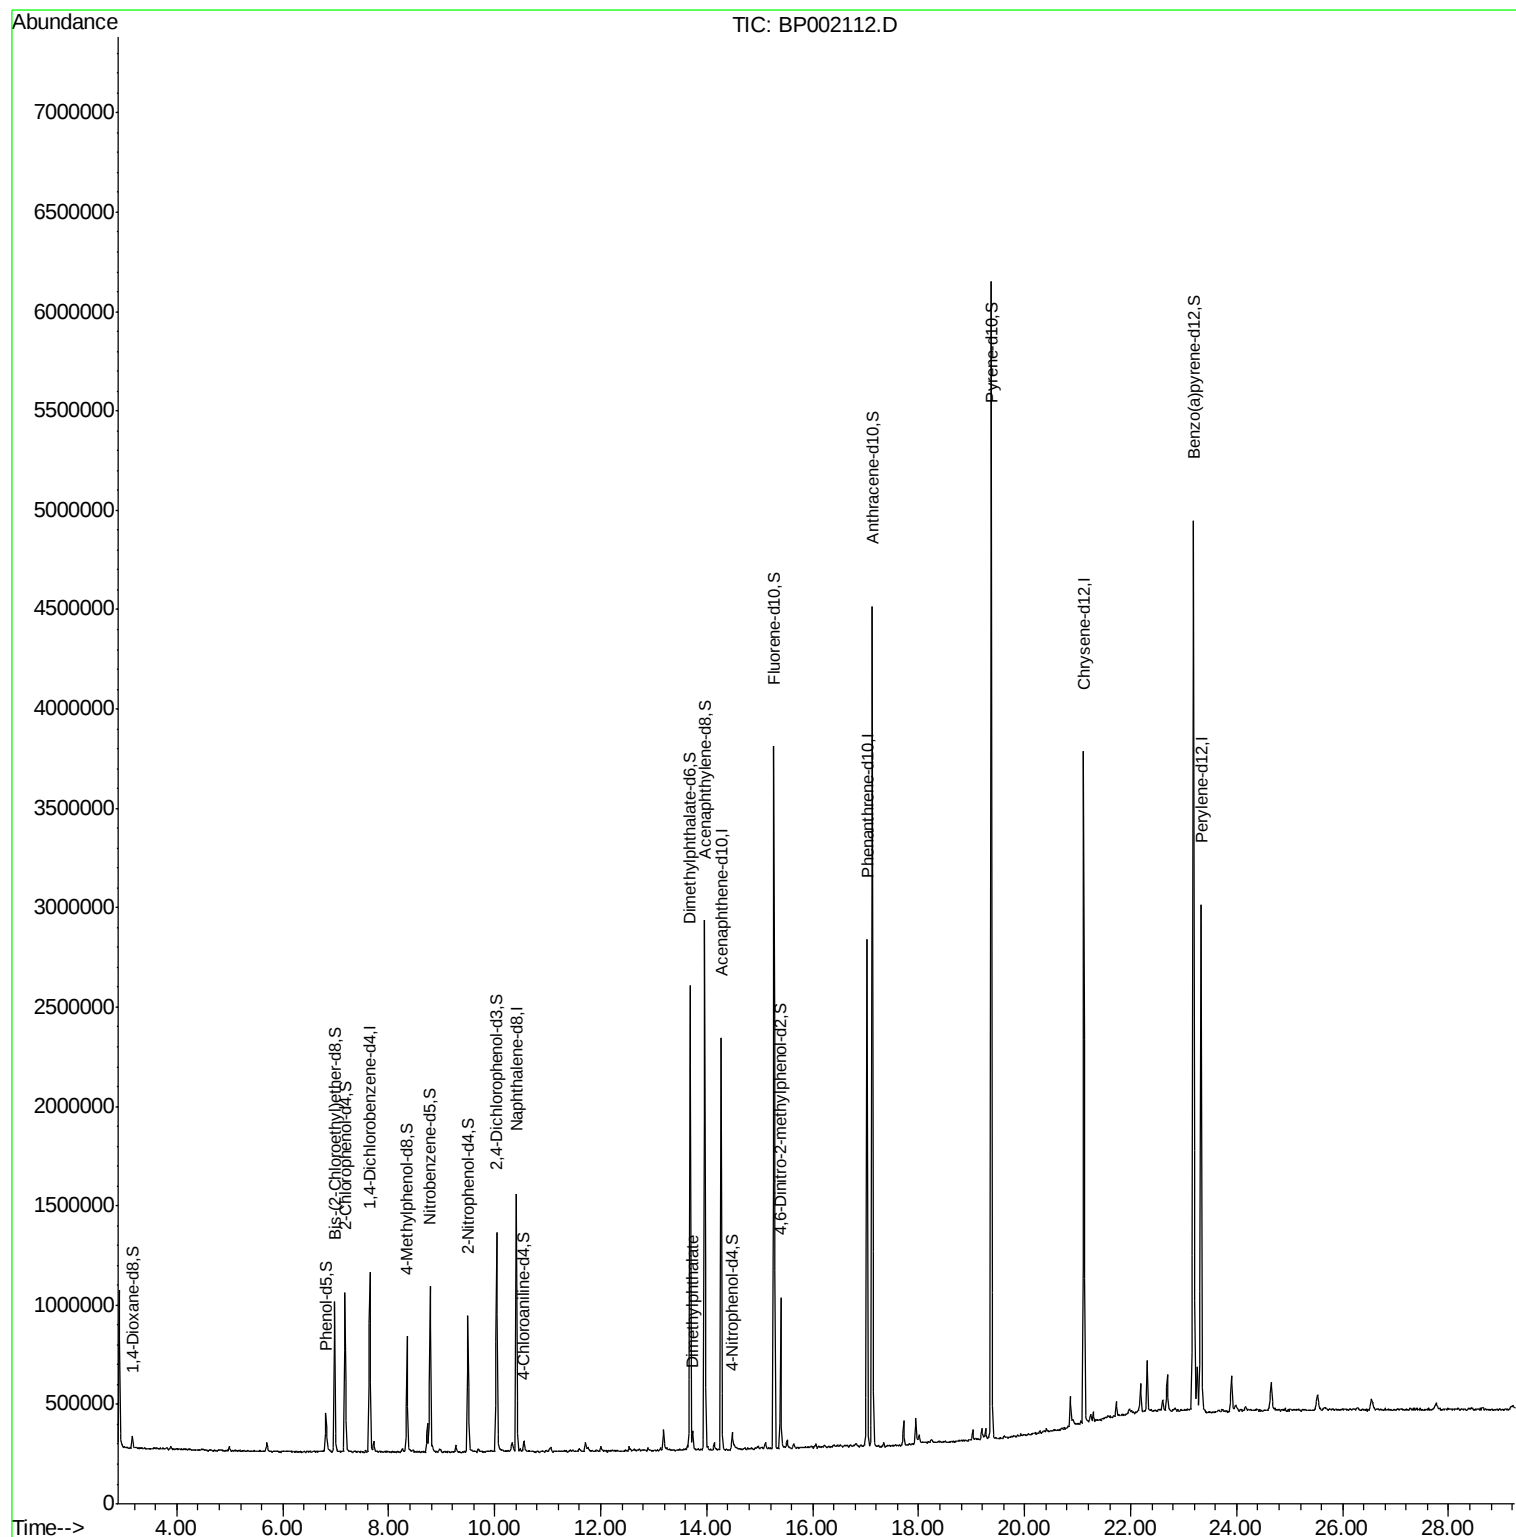

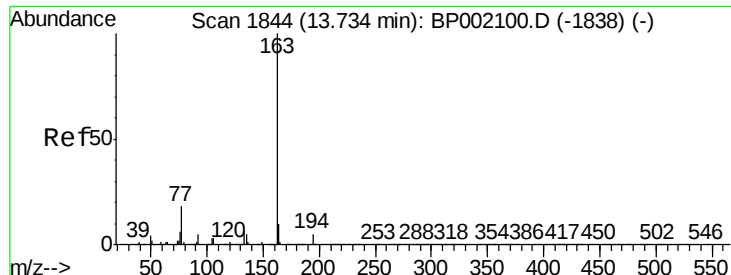

#45

Dimethylphthalate

Concen: 1.132 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002112.D

Acq: 06 Mar 2020 23:51

Instrument :

BNA_P

ClientSampleId :

C0DJ3


Tot Ion:163 Resp: 65471

Ion Ratio Lower Upper

163 100

194 4.7 3.6 5.4

164 10.6 8.2 12.4

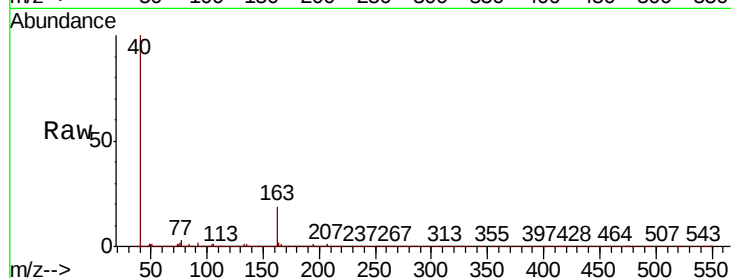

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

