

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
 Data File : BP002090.D
 Acq On : 06 Mar 2020 11:11
 Operator : CG/JU
 Sample : PB127293BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.923	3	6	10	rVB2	28560	34686	0.50%	0.053%
2	3.164	42	47	58	rVB2	65319	106826	1.54%	0.164%
3	3.811	155	157	162	rBV	5853	8202	0.12%	0.013%
4	3.893	168	171	176	rVB2	13461	18539	0.27%	0.029%
5	4.328	242	245	249	rBV2	7478	9425	0.14%	0.015%
6	4.805	324	326	330	rVB	6955	8443	0.12%	0.013%
7	5.093	371	375	377	rVB	5969	7917	0.11%	0.012%
8	5.128	377	381	382	rBV	7221	7817	0.11%	0.012%
9	5.352	414	419	421	rBV	7098	9649	0.14%	0.015%
10	5.399	424	427	430	rBV	5224	8951	0.13%	0.014%
11	5.769	487	490	493	rVB	8349	9423	0.14%	0.015%
12	6.587	627	629	632	rBV	7045	7134	0.10%	0.011%
13	6.816	660	668	680	rBV	959598	1528873	21.97%	2.353%
14	6.893	680	681	685	rVB	6912	7287	0.10%	0.011%
15	6.975	689	695	709	rVV	785578	1269520	18.24%	1.954%
16	7.069	709	711	714	rVB	7429	6994	0.10%	0.011%
17	7.175	721	729	739	rBV	1063883	1686868	24.24%	2.596%
18	7.416	766	770	771	rVB	8831	7533	0.11%	0.012%
19	7.640	801	808	814	rBV	838641	1350443	19.41%	2.079%
20	8.346	919	928	941	rBV	1217232	2011310	28.91%	3.096%
21	8.605	970	972	975	rVB	8492	7906	0.11%	0.012%
22	8.646	975	979	981	rBV	7303	7988	0.11%	0.012%
23	8.781	995	1002	1012	rVV	886280	1444652	20.76%	2.224%
24	8.952	1027	1031	1033	rVB	5276	7606	0.11%	0.012%
25	9.052	1045	1048	1052	rVB	5416	7014	0.10%	0.011%
26	9.499	1117	1124	1134	rVV	710711	1163359	16.72%	1.791%
27	9.734	1161	1164	1168	rVB	6788	8063	0.12%	0.012%
28	9.934	1197	1198	1205	rBV	5855	10697	0.15%	0.016%
29	10.034	1207	1215	1227	rVV	1259276	2118880	30.45%	3.261%
30	10.116	1227	1229	1234	rVB	10235	15727	0.23%	0.024%
31	10.410	1271	1279	1290	rVB	1183244	1982180	28.49%	3.051%
32	10.546	1290	1302	1316	rBV	1172254	2171348	31.21%	3.342%
33	10.863	1353	1356	1359	rVB	6488	8959	0.13%	0.014%
34	11.257	1419	1423	1425	rVB	6118	8063	0.12%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
 Data File : BP002090.D
 Acq On : 06 Mar 2020 11:11
 Operator : CG/JU
 Sample : PB127293BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

35	11.416	1448	1450	1456	rBV	5112	7507	0.11%	0.012%
36	11.734	1502	1504	1507	rVB	5748	7375	0.11%	0.011%
37	11.757	1507	1508	1512	rBV	8865	9054	0.13%	0.014%
38	12.022	1546	1553	1557	rBV2	18559	41000	0.59%	0.063%
39	12.351	1605	1609	1610	rVB	6682	7227	0.10%	0.011%
40	12.916	1702	1705	1709	rBV	6329	9106	0.13%	0.014%
41	13.404	1785	1788	1791	rBV	4844	9004	0.13%	0.014%
42	13.534	1808	1810	1815	rVB	5324	7194	0.10%	0.011%
43	13.640	1825	1828	1829	rBV	7999	7438	0.11%	0.011%
44	13.687	1830	1836	1846	rVB	2375672	3205668	46.07%	4.934%
45	13.963	1876	1883	1891	rBV	2735254	4007355	57.59%	6.168%
46	14.151	1913	1915	1920	rVB	7571	8306	0.12%	0.013%
47	14.275	1929	1936	1943	rVB	1845298	2725809	39.17%	4.196%
48	14.475	1963	1970	1985	rBV	603840	1069636	15.37%	1.646%
49	14.898	2038	2042	2045	rBV	8049	12154	0.17%	0.019%
50	15.275	2099	2106	2113	rBV	3637032	5246630	75.40%	8.076%
51	15.392	2121	2126	2140	rBV	584507	846042	12.16%	1.302%
52	15.516	2142	2147	2152	rVB	46942	72755	1.05%	0.112%
53	15.657	2169	2171	2175	rVB	7925	10082	0.14%	0.016%
54	15.757	2185	2188	2191	rVB	6652	9218	0.13%	0.014%
55	15.787	2191	2193	2195	rBV	7653	7113	0.10%	0.011%
56	15.839	2198	2202	2205	rBV	9135	13673	0.20%	0.021%
57	15.963	2219	2223	2226	rBV	8426	12662	0.18%	0.019%
58	16.063	2235	2240	2246	rBV	13696	24405	0.35%	0.038%
59	16.275	2274	2276	2279	rBV	7133	9193	0.13%	0.014%
60	16.381	2290	2294	2297	rBV	7338	11098	0.16%	0.017%
61	16.816	2365	2368	2372	rVB	11977	12444	0.18%	0.019%
62	17.028	2397	2404	2411	rVB	2379881	3288961	47.27%	5.062%
63	17.122	2414	2420	2431	rVB2	3889429	5505544	79.12%	8.474%
64	17.269	2442	2445	2448	rBV	6894	9465	0.14%	0.015%
65	17.334	2454	2456	2458	rBV	6450	7297	0.10%	0.011%
66	17.698	2516	2518	2522	rBV	6002	7491	0.11%	0.012%
67	17.851	2541	2544	2546	rBV	7087	8123	0.12%	0.013%
68	19.016	2739	2742	2749	rVB2	35019	51357	0.74%	0.079%
69	19.098	2754	2756	2759	rBV	8604	11229	0.16%	0.017%
70	19.263	2780	2784	2790	rVB	38033	52383	0.75%	0.081%
71	19.369	2796	2802	2814	rVB	4892352	6742946	96.90%	10.379%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002090.D
Acq On : 06 Mar 2020 11:11
Operator : CG/JU
Sample : PB127293BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK93

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Title : SVOA CALIBRATION

72	21.122	3095	3100	3113	rBV	3003336	3804201	54.67%	5.856%
73	23.192	3444	3452	3462	rBV	3831903	6958314	100.00%	10.710%
74	23.333	3469	3476	3490	rVB	2084255	4043101	58.10%	6.223%


Sum of corrected areas: 64967842

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030620\
Data File : BP002090.D
Acq On : 06 Mar 2020 11:11
Operator : CG/JU
Sample : PB127293BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

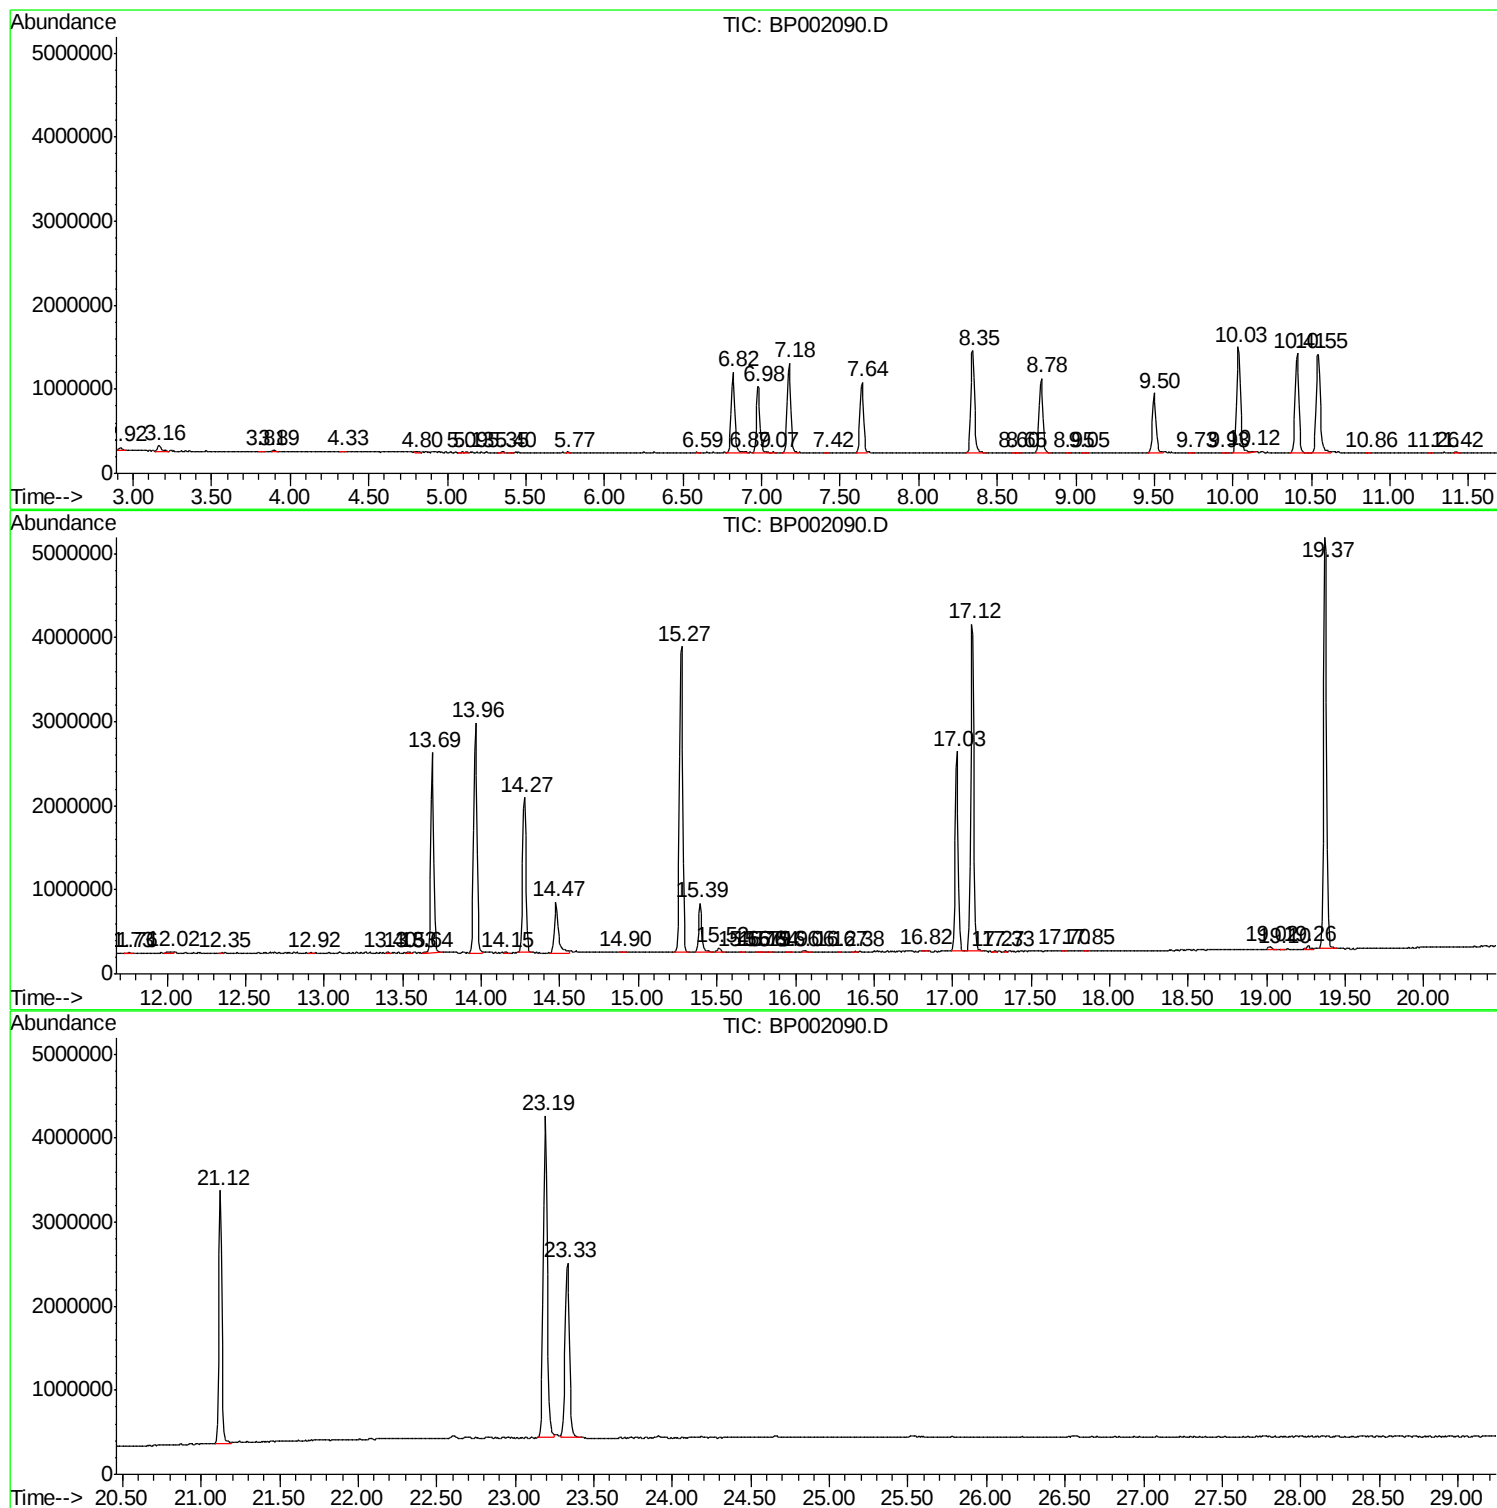

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
Data File : BP002090.D
Acq On : 06 Mar 2020 11:11
Operator : CG/JU
Sample : PB127293BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030620\
Data File : BP002090.D
Acq On : 06 Mar 2020 11:11
Operator : CG/JU
Sample : PB127293BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc