

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002119.D
 Acq On : 09 Mar 2020 14:20
 Operator : CG/JU
 Sample : L1707-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB706

Quant Time: Mar 09 15:48:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 15:02:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	256999	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1047235	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	665756	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1459363	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1448411	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1678092	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	42677	7.14	ng/uL	0.00
5) Phenol-d5	6.82	99	705500	35.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	402904	38.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	626014	36.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	589837	36.61	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	294000	36.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	317882	35.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	619291	35.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	839203	43.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1946211	38.63	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2357479	39.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	245579	25.50	ng/ul	0.00
58) Fluorene-d10	15.27	176	1745876	40.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	205625	25.56	ng/ul	0.00
71) Anthracene-d10	17.12	188	2660860	40.57	ng/ul	0.00
79) Pyrene-d10	19.37	212	3040738	40.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3397152	39.57	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	163381	3.141	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002119.D
Acq On : 09 Mar 2020 14:20
Operator : CG/JU
Sample : L1707-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB706

Quant Time: Mar 09 15:48:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 15:02:40 2020
Response via : Initial Calibration

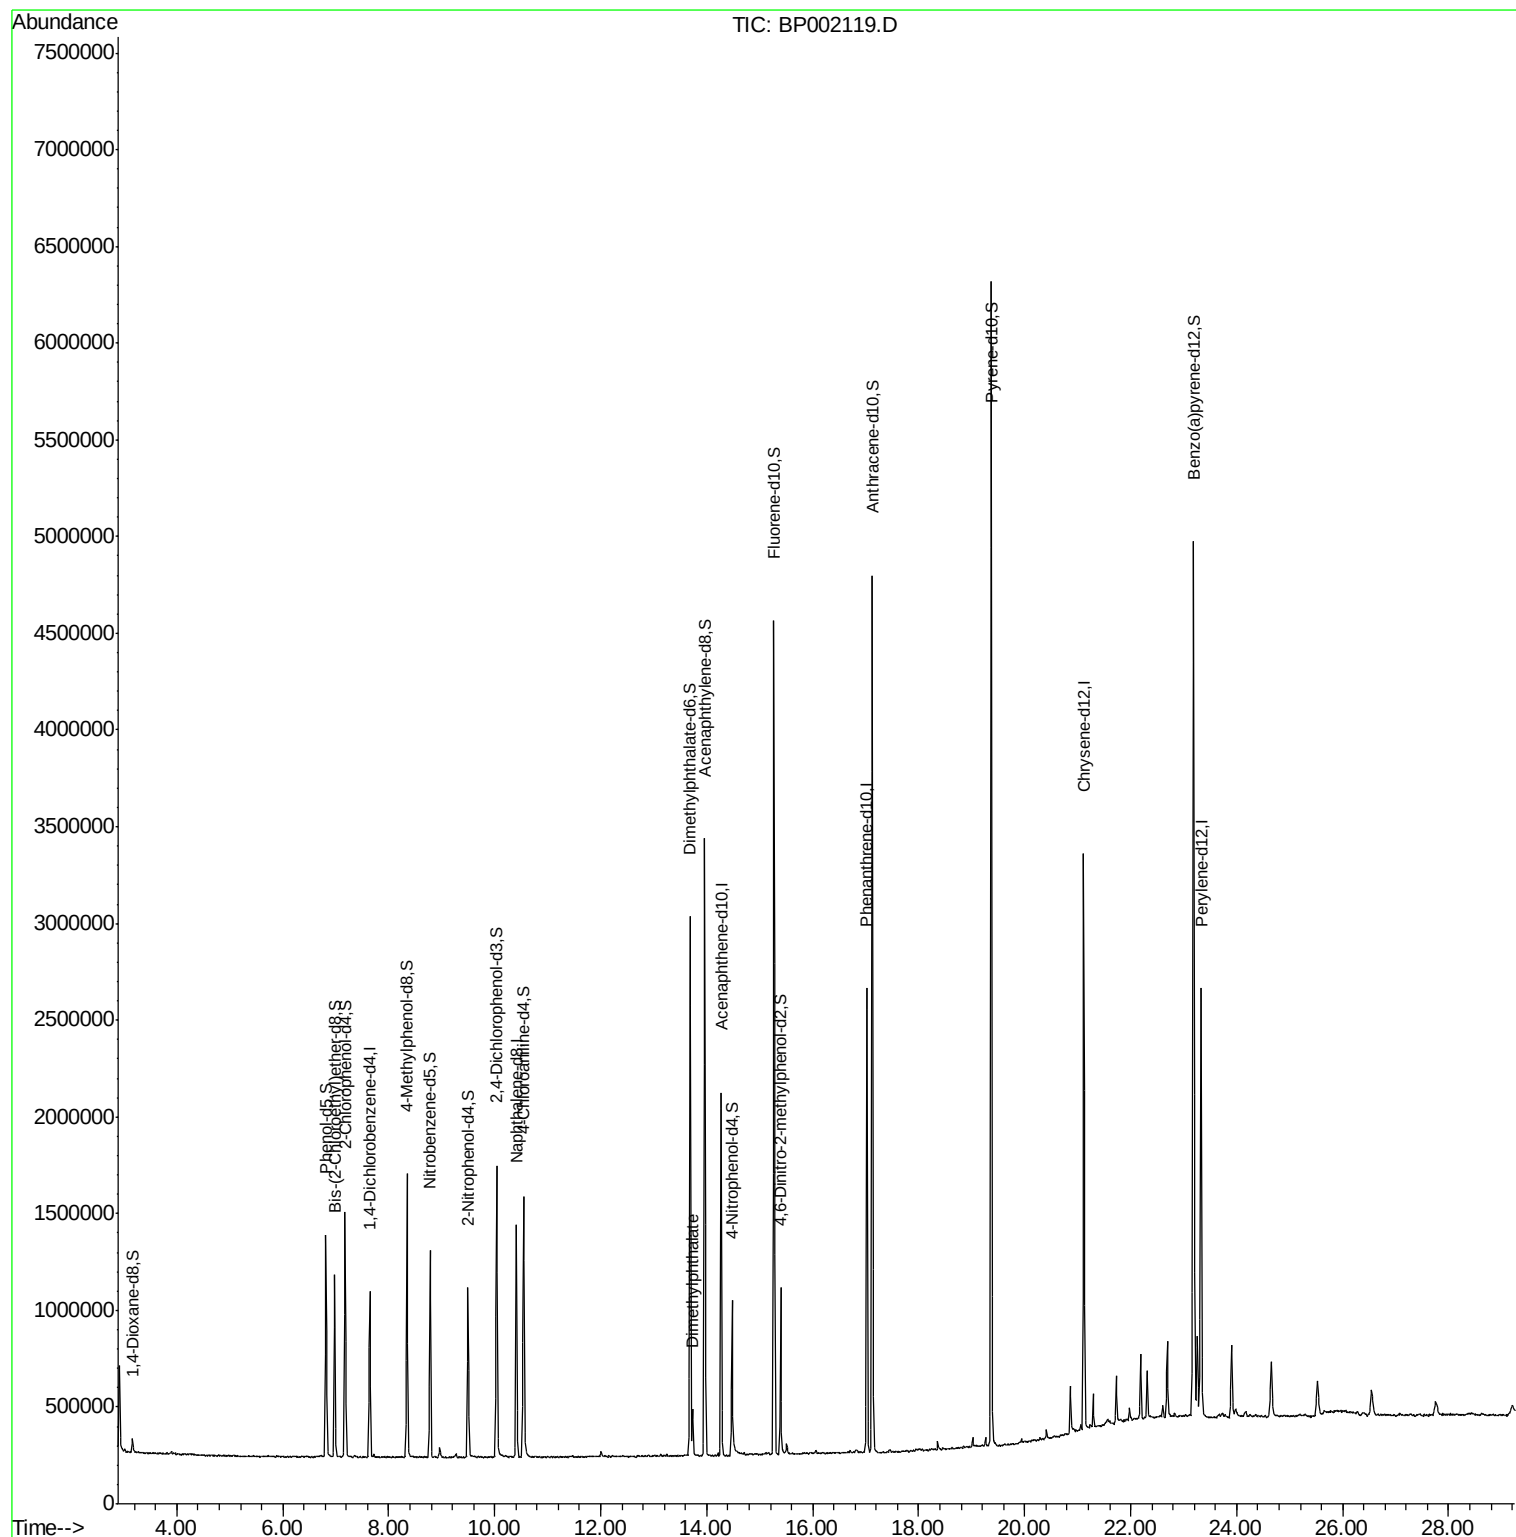

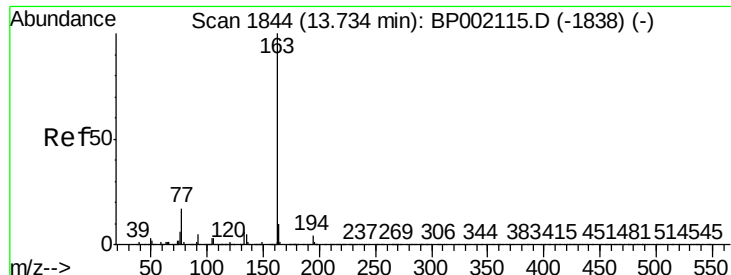

#45

Dimethylphthalate

Concen: 3.141 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.00 min

Lab File: BP002119.D

Acq: 09 Mar 2020 14:20

Instrument :

BNA_P

ClientSampleId :

CB706


Tot Ion:163 Resp: 163381

Ion Ratio Lower Upper

163 100

194 4.5 3.6 5.4

164 9.9 8.2 12.4

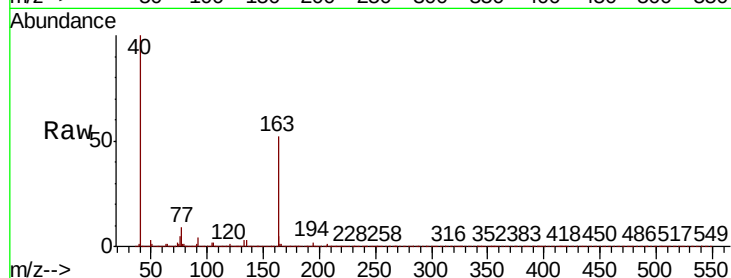

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

