

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002120.D
 Acq On : 09 Mar 2020 14:54
 Operator : CG/JU
 Sample : L1707-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB705

Quant Time: Mar 09 15:51:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 15:02:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	292065	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1201533	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	767687	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1679076	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1669816	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1889729	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	43543	6.41	ng/uL	0.00
5) Phenol-d5	6.82	99	725834	32.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	414684	35.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	643987	33.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	622325	33.99	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	310119	33.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	337340	32.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	653459	32.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	870726	39.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2051720	35.31	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2494783	35.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	260252	23.43	ng/ul	0.00
58) Fluorene-d10	15.27	176	1840495	36.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	223568	24.15	ng/ul	0.00
71) Anthracene-d10	17.12	188	2770708	36.72	ng/ul	0.00
79) Pyrene-d10	19.37	212	3209439	36.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3597385	37.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	302331	5.041	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002120.D
Acq On : 09 Mar 2020 14:54
Operator : CG/JU
Sample : L1707-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB705

Quant Time: Mar 09 15:51:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 15:02:40 2020
Response via : Initial Calibration

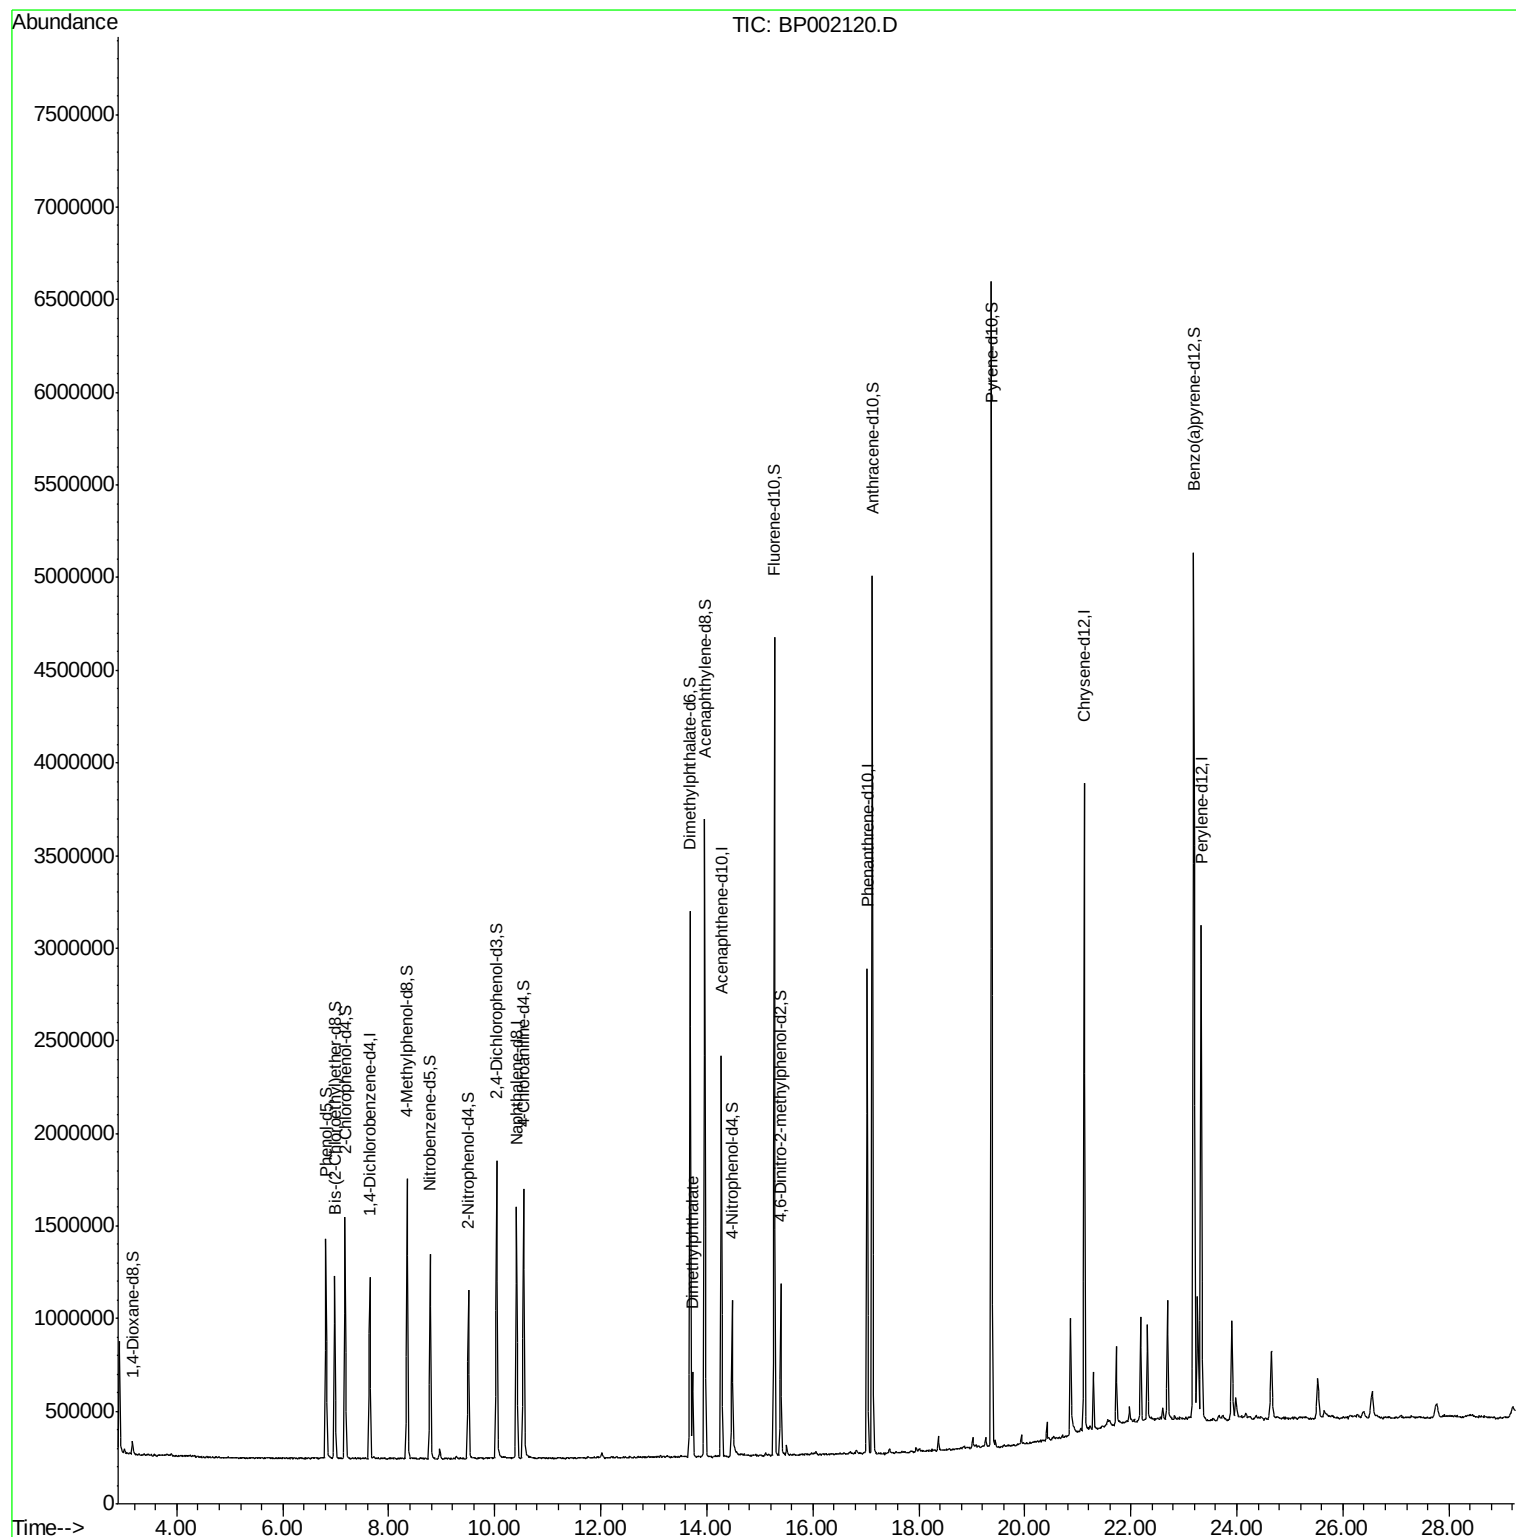

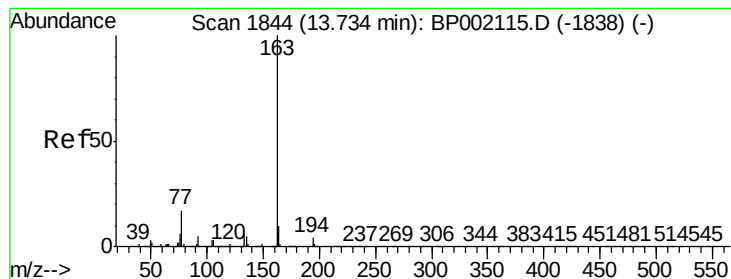

#45

Dimethylphthalate

Concen: 5.041 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.00 min

Lab File: BP002120.D

Acq: 09 Mar 2020 14:54

Instrument :

BNA_P

ClientSampleId :

CB705


Tot Ion:163 Resp: 302331

Ion Ratio Lower Upper

163 100

194 4.5 3.6 5.4

164 9.9 8.2 12.4

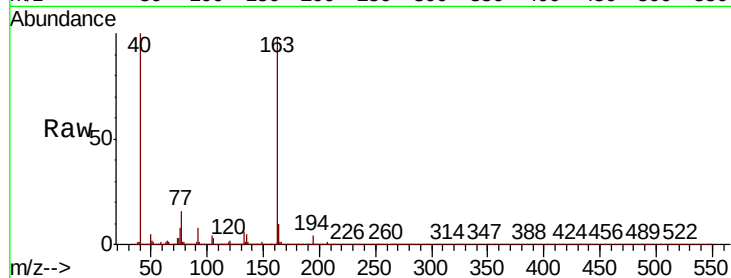

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

