

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002121.D
 Acq On : 09 Mar 2020 15:28
 Operator : CG/JU
 Sample : L1707-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB704

Quant Time: Mar 09 16:01:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 15:02:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	259735	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1067196	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	688924	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1484158	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1475400	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1690671	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	41533	6.87	ng/uL	0.00
5) Phenol-d5	6.82	99	684012	34.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	397588	37.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	611128	35.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	576878	35.43	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	290518	35.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	314526	34.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	603814	33.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	819555	42.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1919286	36.81	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2321125	37.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	241574	24.24	ng/ul	0.00
58) Fluorene-d10	15.27	176	1713478	37.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	202381	24.73	ng/ul	0.00
71) Anthracene-d10	17.12	188	2568434	38.50	ng/ul	0.00
79) Pyrene-d10	19.37	212	2939794	38.06	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3240706	37.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	68519	1.273	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002121.D
Acq On : 09 Mar 2020 15:28
Operator : CG/JU
Sample : L1707-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB704

Quant Time: Mar 09 16:01:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 15:02:40 2020
Response via : Initial Calibration

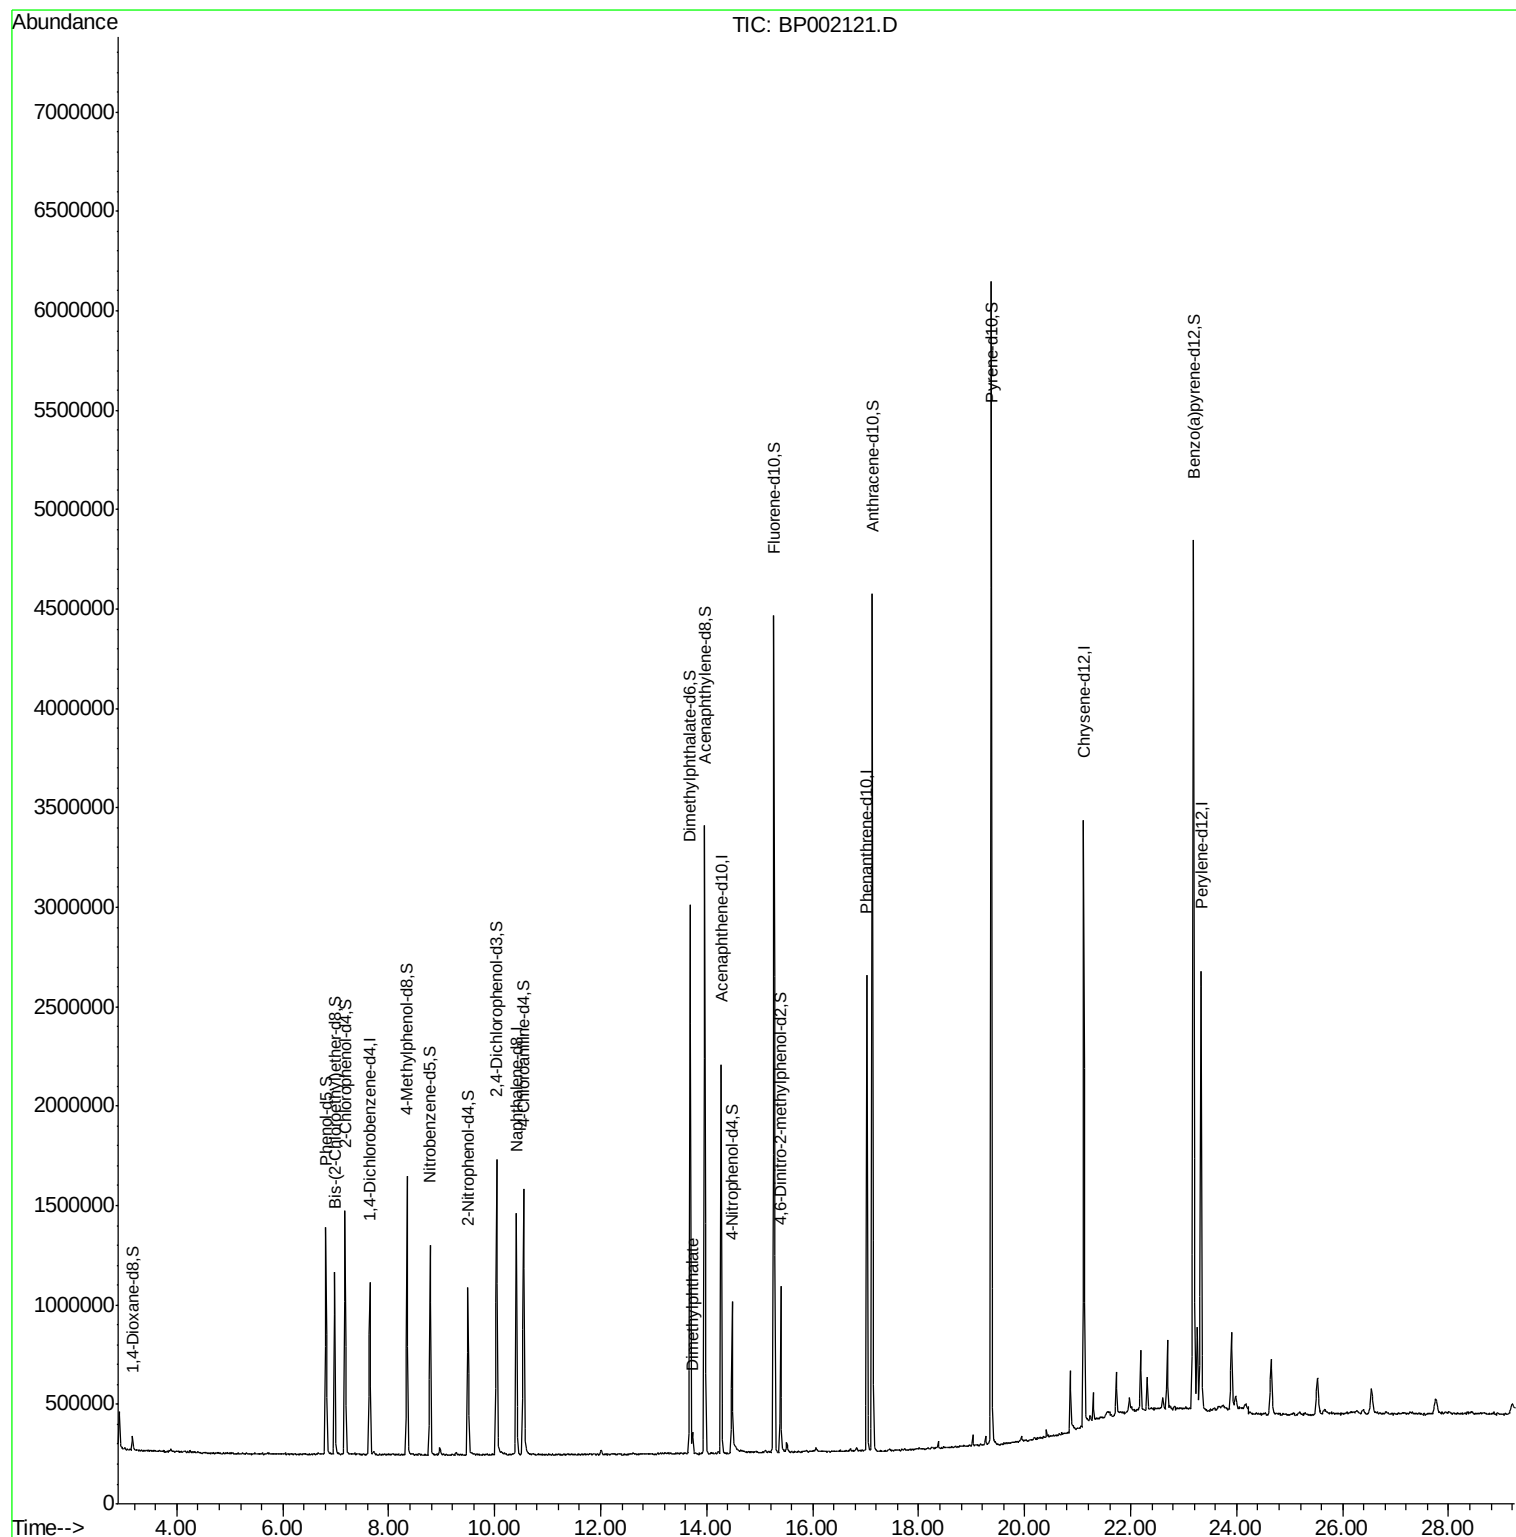

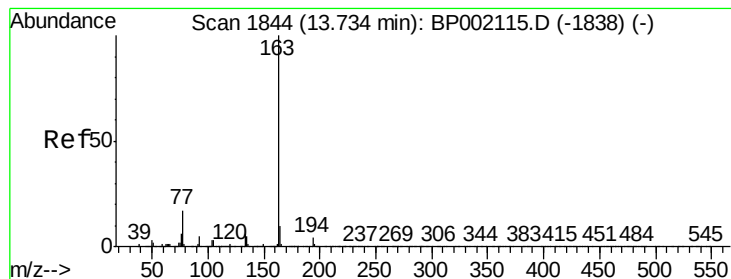

#45
 Dimethylphthalate
 Concen: 1.273 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BP002121.D
 Acq: 09 Mar 2020 15:28

Instrument :
 BNA_P
 ClientSampleId :
 CB704

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.2	3.6	5.4
164	10.6	8.2	12.4

