

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002125.D
 Acq On : 09 Mar 2020 17:48
 Operator : CG/JU
 Sample : L1834-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DJ9

Quant Time: Mar 09 18:24:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 15:02:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	272184	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1111563	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	727012	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1571438	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1590136	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1857390	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	34041	5.38	ng/uL	0.00
5) Phenol-d5	6.82	99	119620	5.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	341407	31.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	428410	23.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	242219	14.20	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	251319	29.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	270808	28.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	499741	27.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	28734	1.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1838655	33.42	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2140242	32.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	27488	2.61	ng/ul	0.00
58) Fluorene-d10	15.27	176	1670650	35.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	201694	23.28	ng/ul	0.00
71) Anthracene-d10	17.12	188	2669595	37.80	ng/ul	0.00
79) Pyrene-d10	19.37	212	3076387	36.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3471005	36.53	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	104043	1.832	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002125.D
Acq On : 09 Mar 2020 17:48
Operator : CG/JU
Sample : L1834-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0DJ9

Quant Time: Mar 09 18:24:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 15:02:40 2020
Response via : Initial Calibration

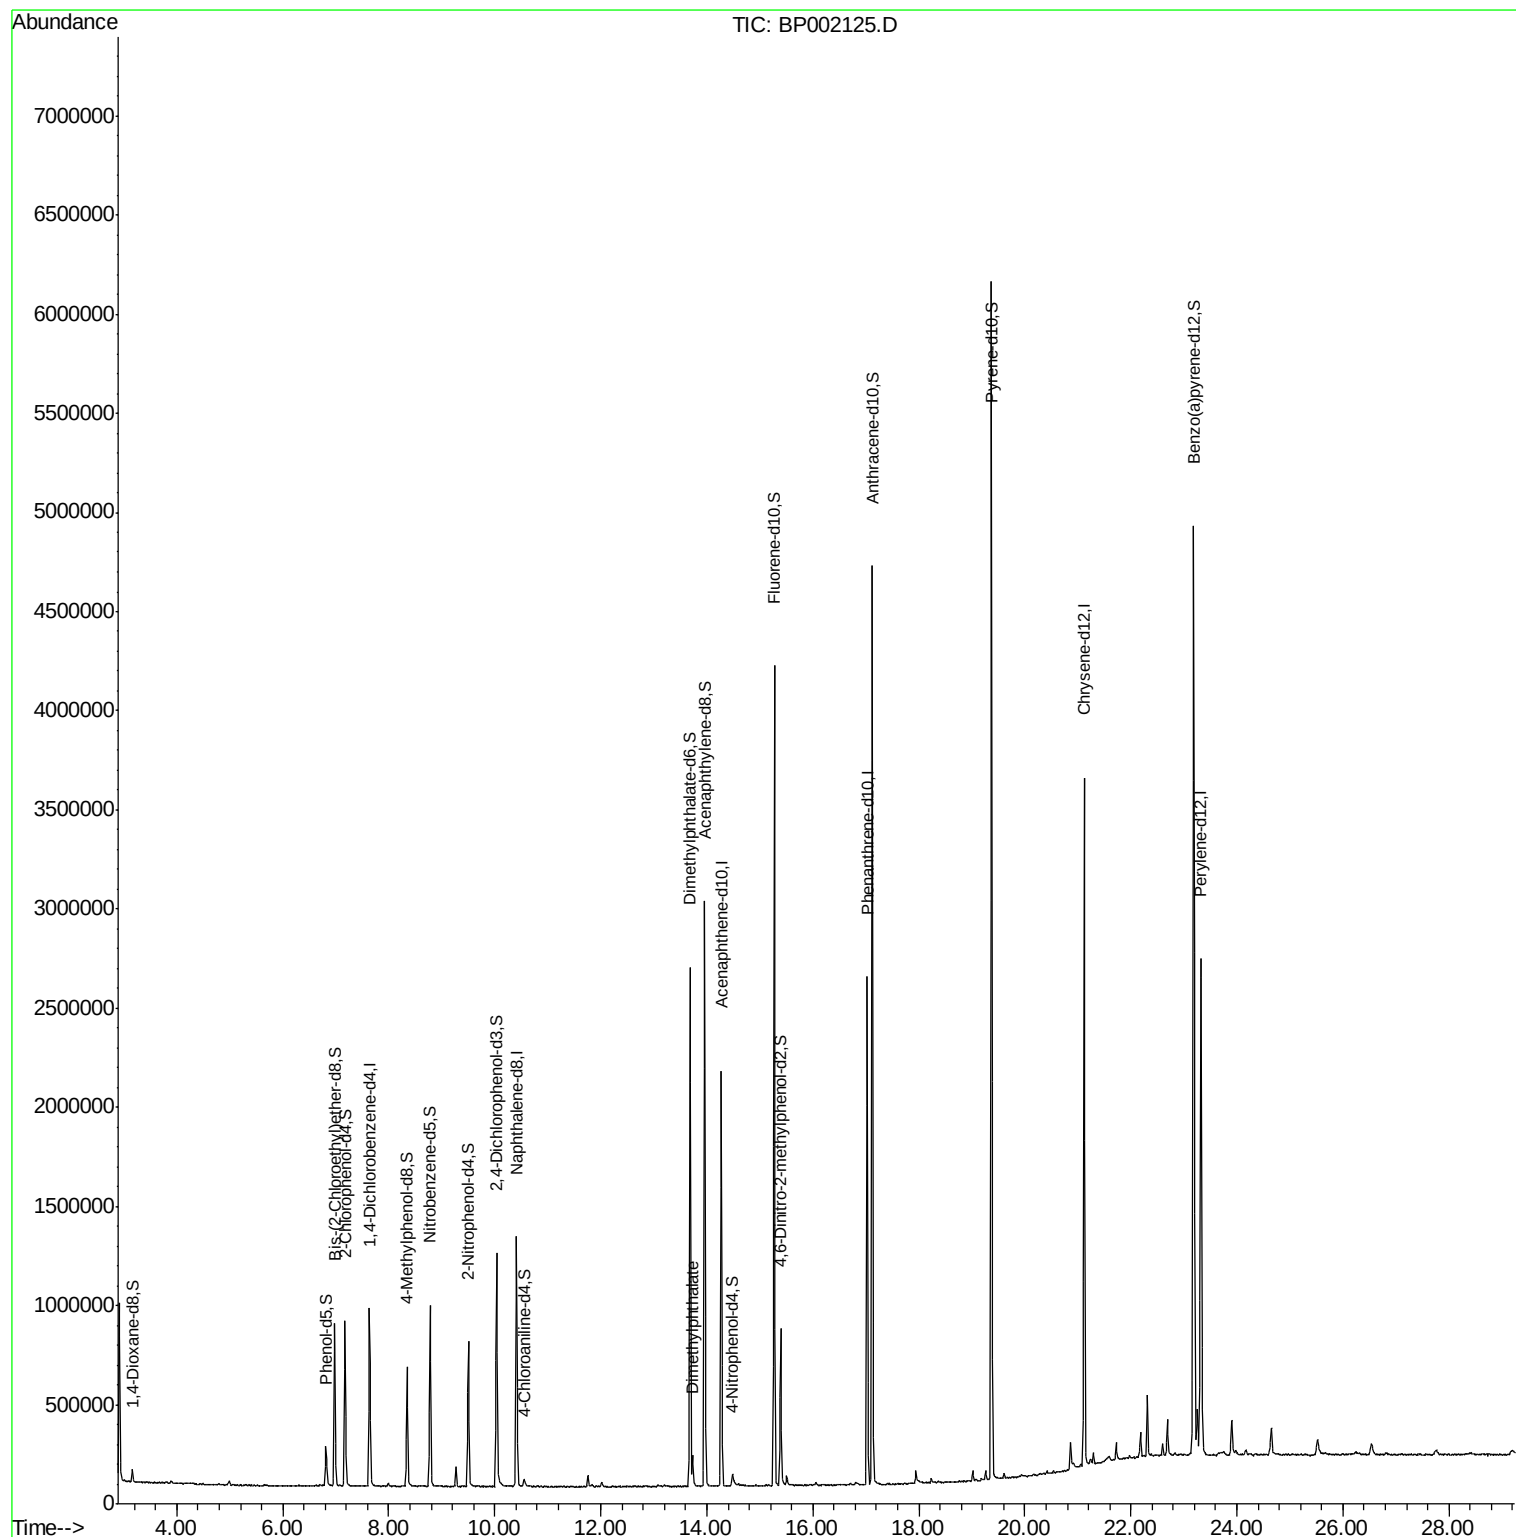


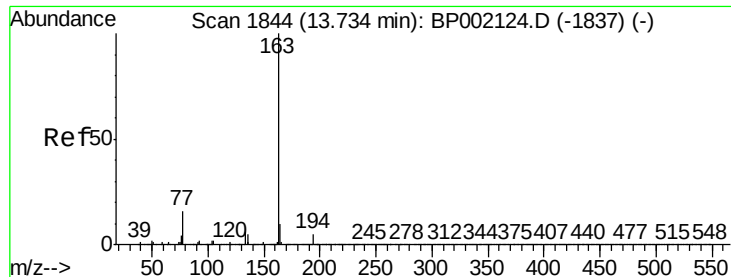

#45
 Dimethylphthalate
 Concen: 1.832 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. 0.00 min
 Lab File: BP002125.D
 Acq: 09 Mar 2020 17:48

Instrument :
 BNA_P
 ClientSampleId :
 C0DJ9

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.8	3.6	5.4
164	10.0	8.2	12.4

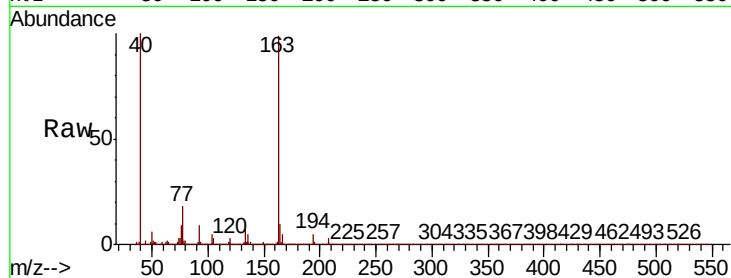

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

