

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002127.D
 Acq On : 09 Mar 2020 18:56
 Operator : CG/JU
 Sample : L1834-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DK0

Quant Time: Mar 09 23:45:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 15:02:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	271471	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1099480	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	700695	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1532686	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1598567	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1831692	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	30560	4.84	ng/uL	0.00
5) Phenol-d5	6.82	99	108159	5.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	333820	30.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	408256	22.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	222828	13.09	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	242546	28.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	261827	27.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	480144	26.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	26571	1.32	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1721662	32.47	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2041734	32.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	22701	2.24	ng/ul	0.01
58) Fluorene-d10	15.27	176	1587616	34.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	182864	21.64	ng/ul	0.00
71) Anthracene-d10	17.12	188	2555975	37.10	ng/ul	0.00
79) Pyrene-d10	19.37	212	3005586	35.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3410705	36.39	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	83014	1.517	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002127.D
Acq On : 09 Mar 2020 18:56
Operator : CG/JU
Sample : L1834-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0DK0

Quant Time: Mar 09 23:45:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 15:02:40 2020
Response via : Initial Calibration

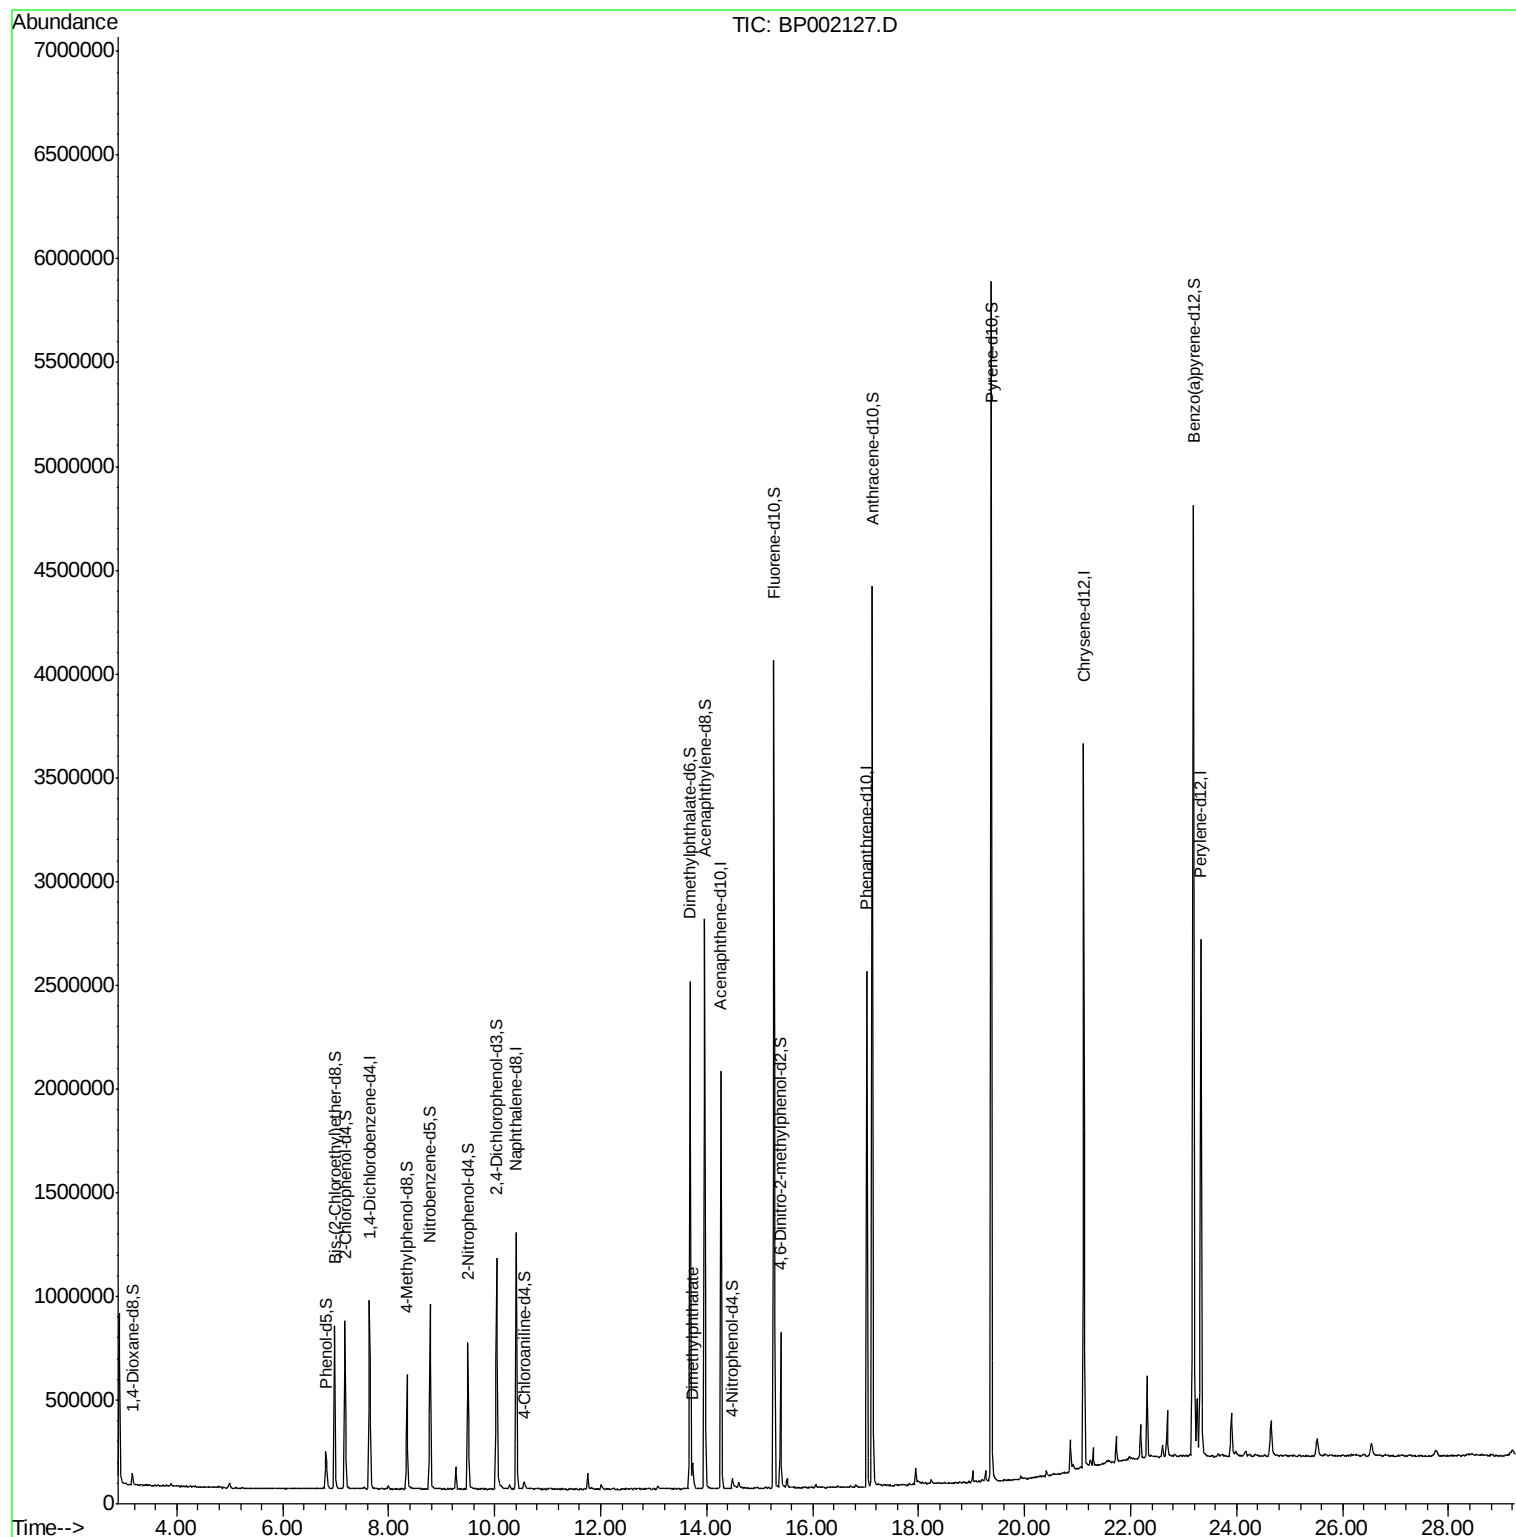

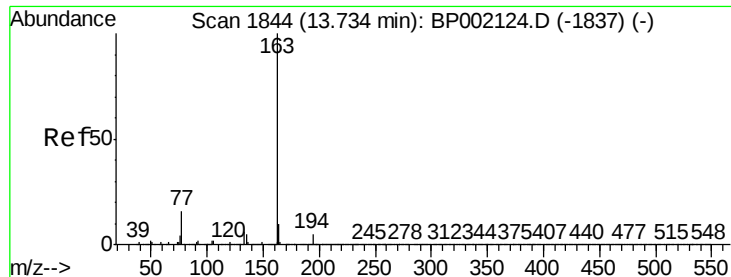

#45
 Dimethylphthalate
 Concen: 1.517 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BP002127.D
 Acq: 09 Mar 2020 18:56

Instrument :
 BNA_P
 ClientSampleId :
 C0DK0

Tot Ion:163	Resp: 83014
Ion Ratio	Lower Upper
163 100	
194 4.1	3.6 5.4
164 10.3	8.2 12.4

