

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030920\
 Data File : BP002134.D
 Acq On : 09 Mar 2020 22:54
 Operator : CG/JU
 Sample : L1834-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0DK8

Manual Integrations
 APPROVED

mohammad
 3/10/2020 2:46:22 PM

Quant Time: Mar 09 23:43:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 09 21:43:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	297654	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1242698	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	812345	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1755761	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1709112	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1960595	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	33309	4.81	ng/uL	0.00
5) Phenol-d5	6.82	99	119806	5.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	331080	27.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	412323	20.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	242723	13.01	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	244676	25.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	260541	24.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	489059	23.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	57628	2.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1821074	29.62	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2091434	28.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	35765m	3.04	ng/ul	0.00
58) Fluorene-d10	15.27	176	1613582	30.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	210807	21.78	ng/ul	0.00
71) Anthracene-d10	17.12	188	2730869	34.61	ng/ul	0.00
79) Pyrene-d10	19.37	212	3196350	35.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	3526522	35.16	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.73	163	545214	8.591	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030920\
Data File : BP002134.D
Acq On : 09 Mar 2020 22:54
Operator : CG/JU
Sample : L1834-15
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
C0DK8

Quant Time: Mar 09 23:43:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 09 21:43:02 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
3/10/2020 2:46:22 PM

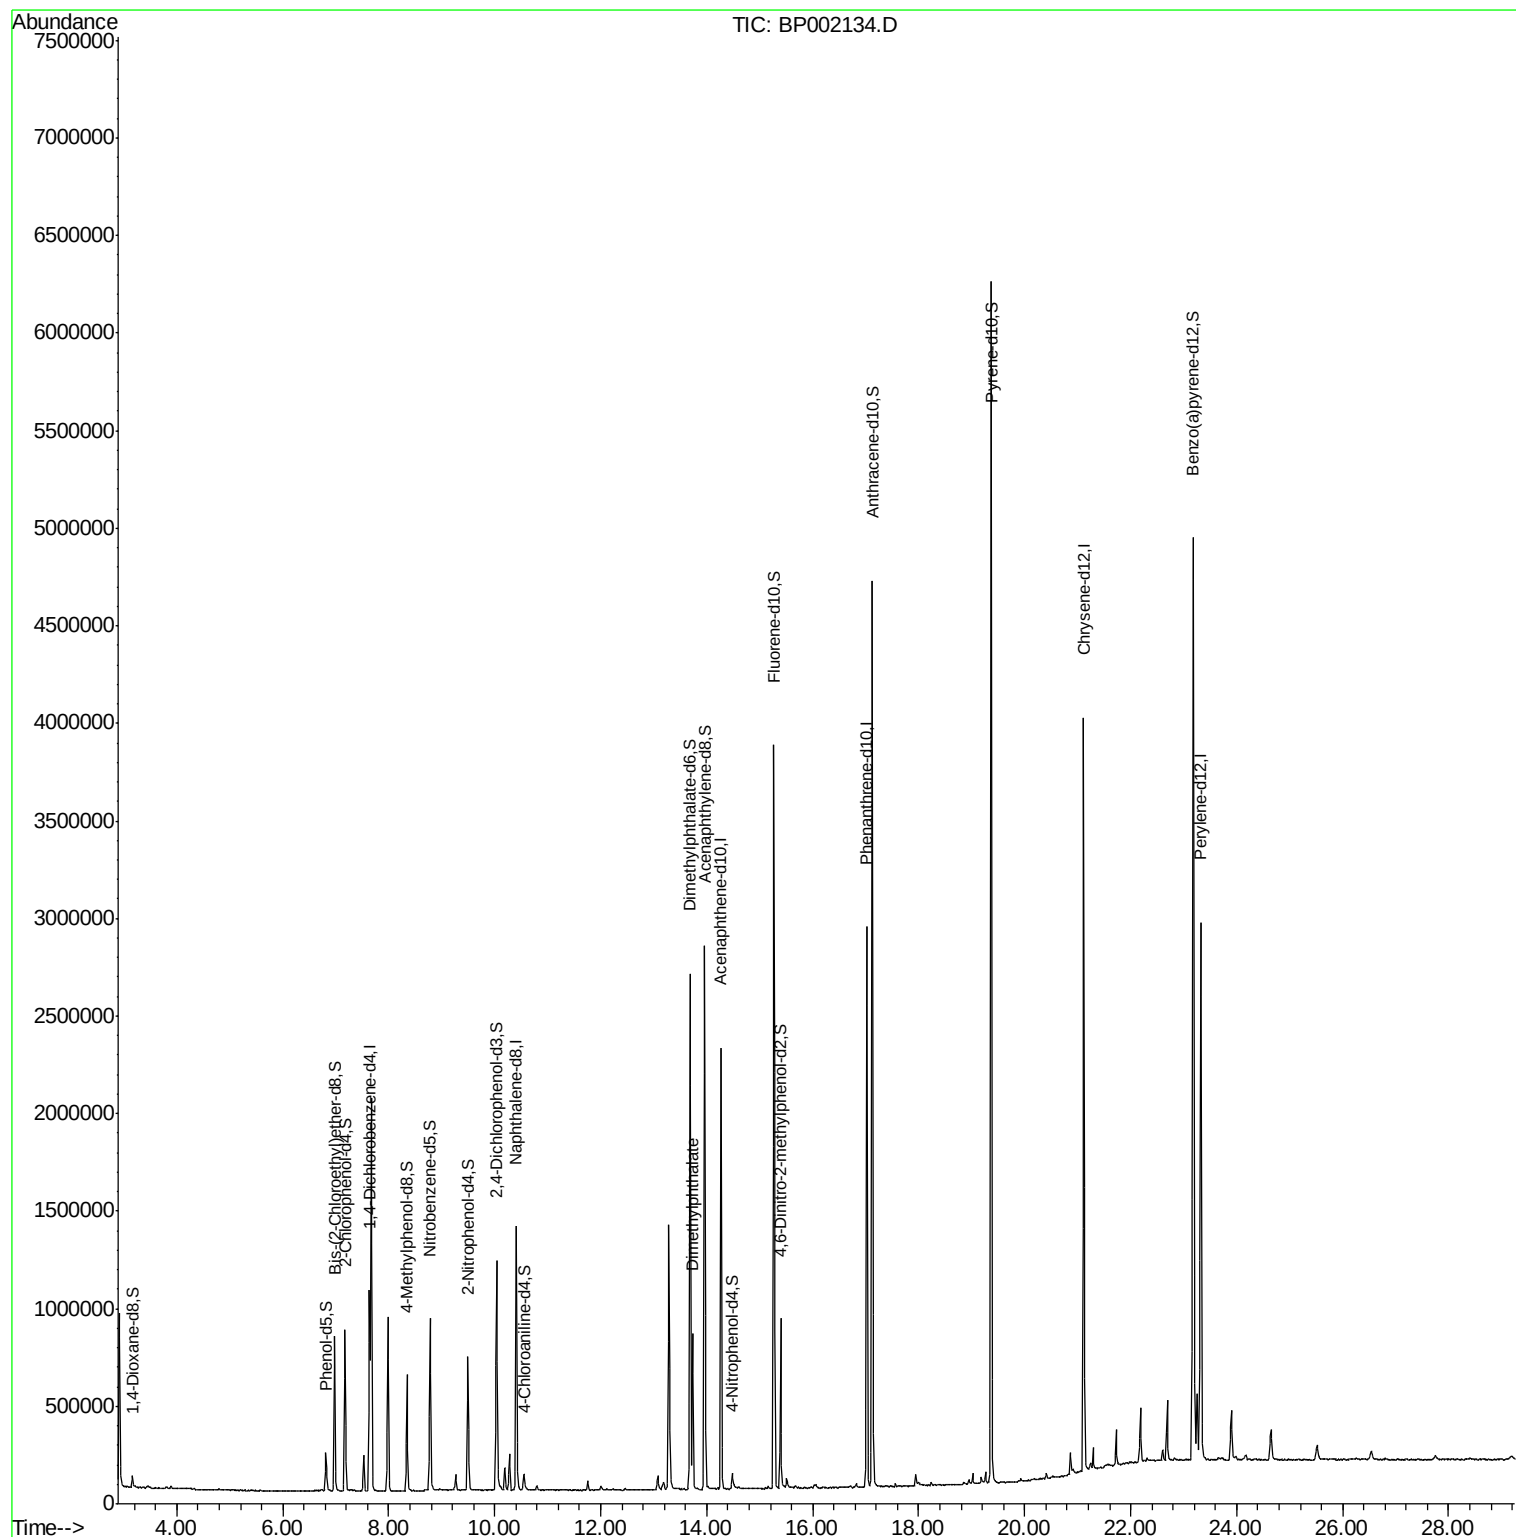

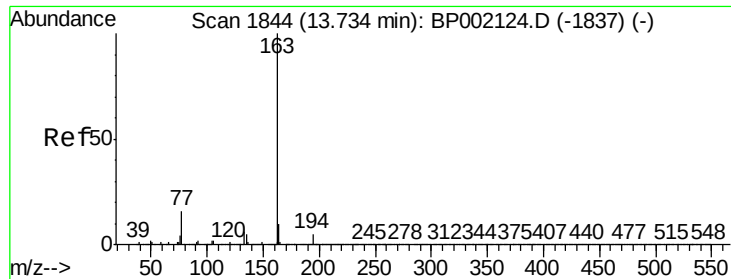


#45
 Dimethylphthalate
 Concen: 8.591 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. -0.00 min
 Lab File: BP002134.D
 Acq: 09 Mar 2020 22:54

Instrument :
 BNA_P
 ClientSampleId :
 C0DK8

Tot Ion:	163	Resp:	545214
Ion Ratio	Lower	Upper	
163	100		
194	4.4	3.6	5.4
164	10.2	8.2	12.4

Manual Integrations
 APPROVED

mohammad
 3/10/2020 2:46:22 PM

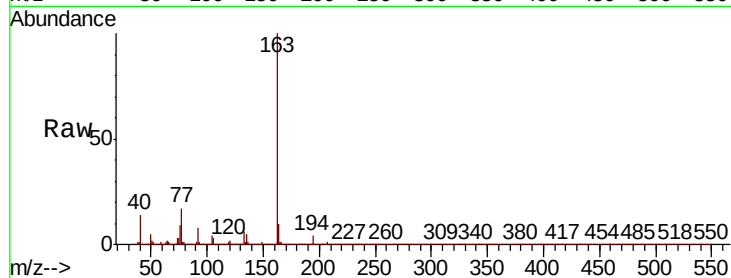

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

