

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031020\
 Data File : BP002165.D
 Acq On : 10 Mar 2020 23:37
 Operator : CG/JU
 Sample : L1843-01DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB5S6DL

Quant Time: Mar 11 01:42:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 11 00:28:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	365508	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1544778	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	1005919	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	2207606	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	2187372	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	2536760	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	849	0.10	ng/uL	0.00
5) Phenol-d5	6.83	99	13090	0.47	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.98	67	25655	1.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	35736	1.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	22330	0.97	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	15874	1.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	13004	0.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	38016	1.48	ng/ul	0.01
29) 4-Chloroaniline-d4	10.55	131	47030	1.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	144848	1.90	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	151815	1.67	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
58) Fluorene-d10	15.27	176	129739	1.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	2701	0.22	ng/ul	0.00
71) Anthracene-d10	17.12	188	213607	2.15	ng/ul	0.00
79) Pyrene-d10	19.37	212	236955	2.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	239743	1.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.20	88	106777	11.778	ng/uL#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031020\
Data File : BP002165.D
Acq On : 10 Mar 2020 23:37
Operator : CG/JU
Sample : L1843-01DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB5S6DL

Quant Time: Mar 11 01:42:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 11 00:28:36 2020
Response via : Initial Calibration

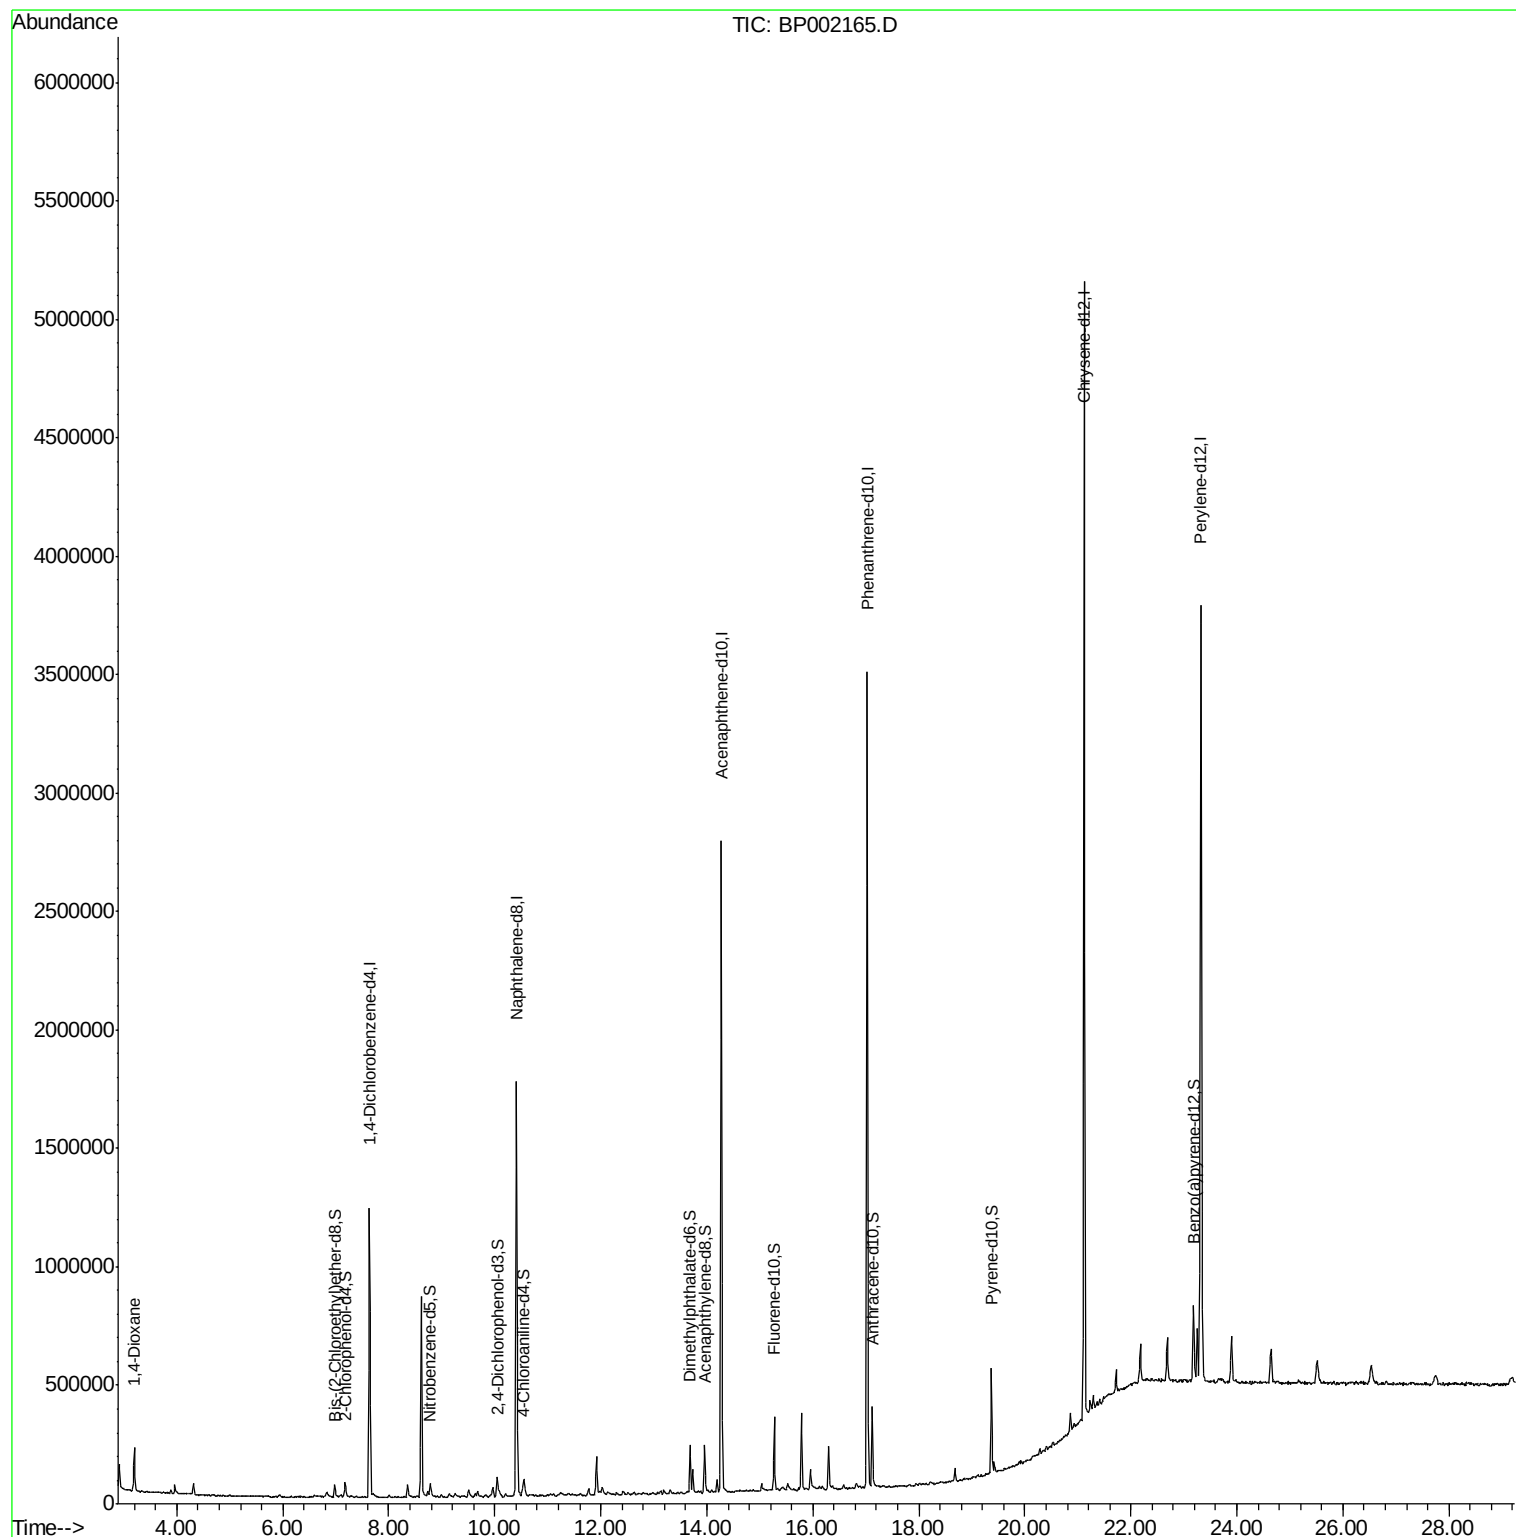

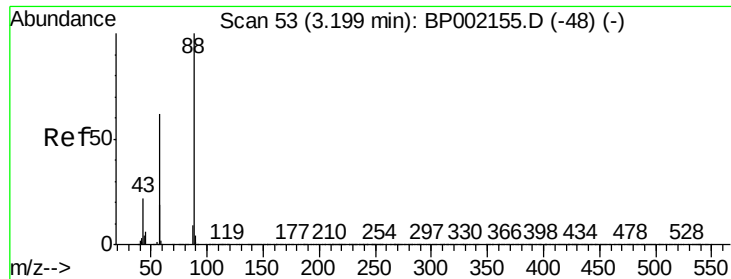

#2

1,4-Dioxane

Concen: 11.778 ng/uL

RT: 3.20 min Scan# 53

Delta R.T. 0.00 min

Lab File: BP002165.D

Acq: 10 Mar 2020 23:37

Instrument :

BNA_P

ClientSampleId :

CB5S6DL

Tot Ion: 88 Resp: 106777

Ion Ratio Lower Upper

88 100

43 22.0 22.6 34.0#

58 61.8 49.6 74.4

