

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031020\
 Data File : BP002172.D
 Acq On : 11 Mar 2020 10:48
 Operator : CG/JU
 Sample : L1786-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC1

Quant Time: Mar 12 01:35:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 12 01:18:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	335626	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1411095	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	885881	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1911241	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1781520	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	2014197	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	32962	4.22	ng/uL	0.00
5) Phenol-d5	6.82	99	625874	24.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	367868	27.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	552838	24.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	497589	23.65	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	247206	22.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	254615	20.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	536391	22.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	727350	28.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1579874	23.57	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1948240	24.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	136240	10.63	ng/ul	0.01
58) Fluorene-d10	15.27	176	1465169	25.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	106783	10.13	ng/ul	0.00
71) Anthracene-d10	17.12	188	2195470	25.56	ng/ul	0.00
79) Pyrene-d10	19.37	212	2472645	26.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2542699	24.67	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.73	163	274301	3.964	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031020\
Data File : BP002172.D
Acq On : 11 Mar 2020 10:48
Operator : CG/JU
Sample : L1786-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC1

Quant Time: Mar 12 01:35:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 12 01:18:11 2020
Response via : Initial Calibration

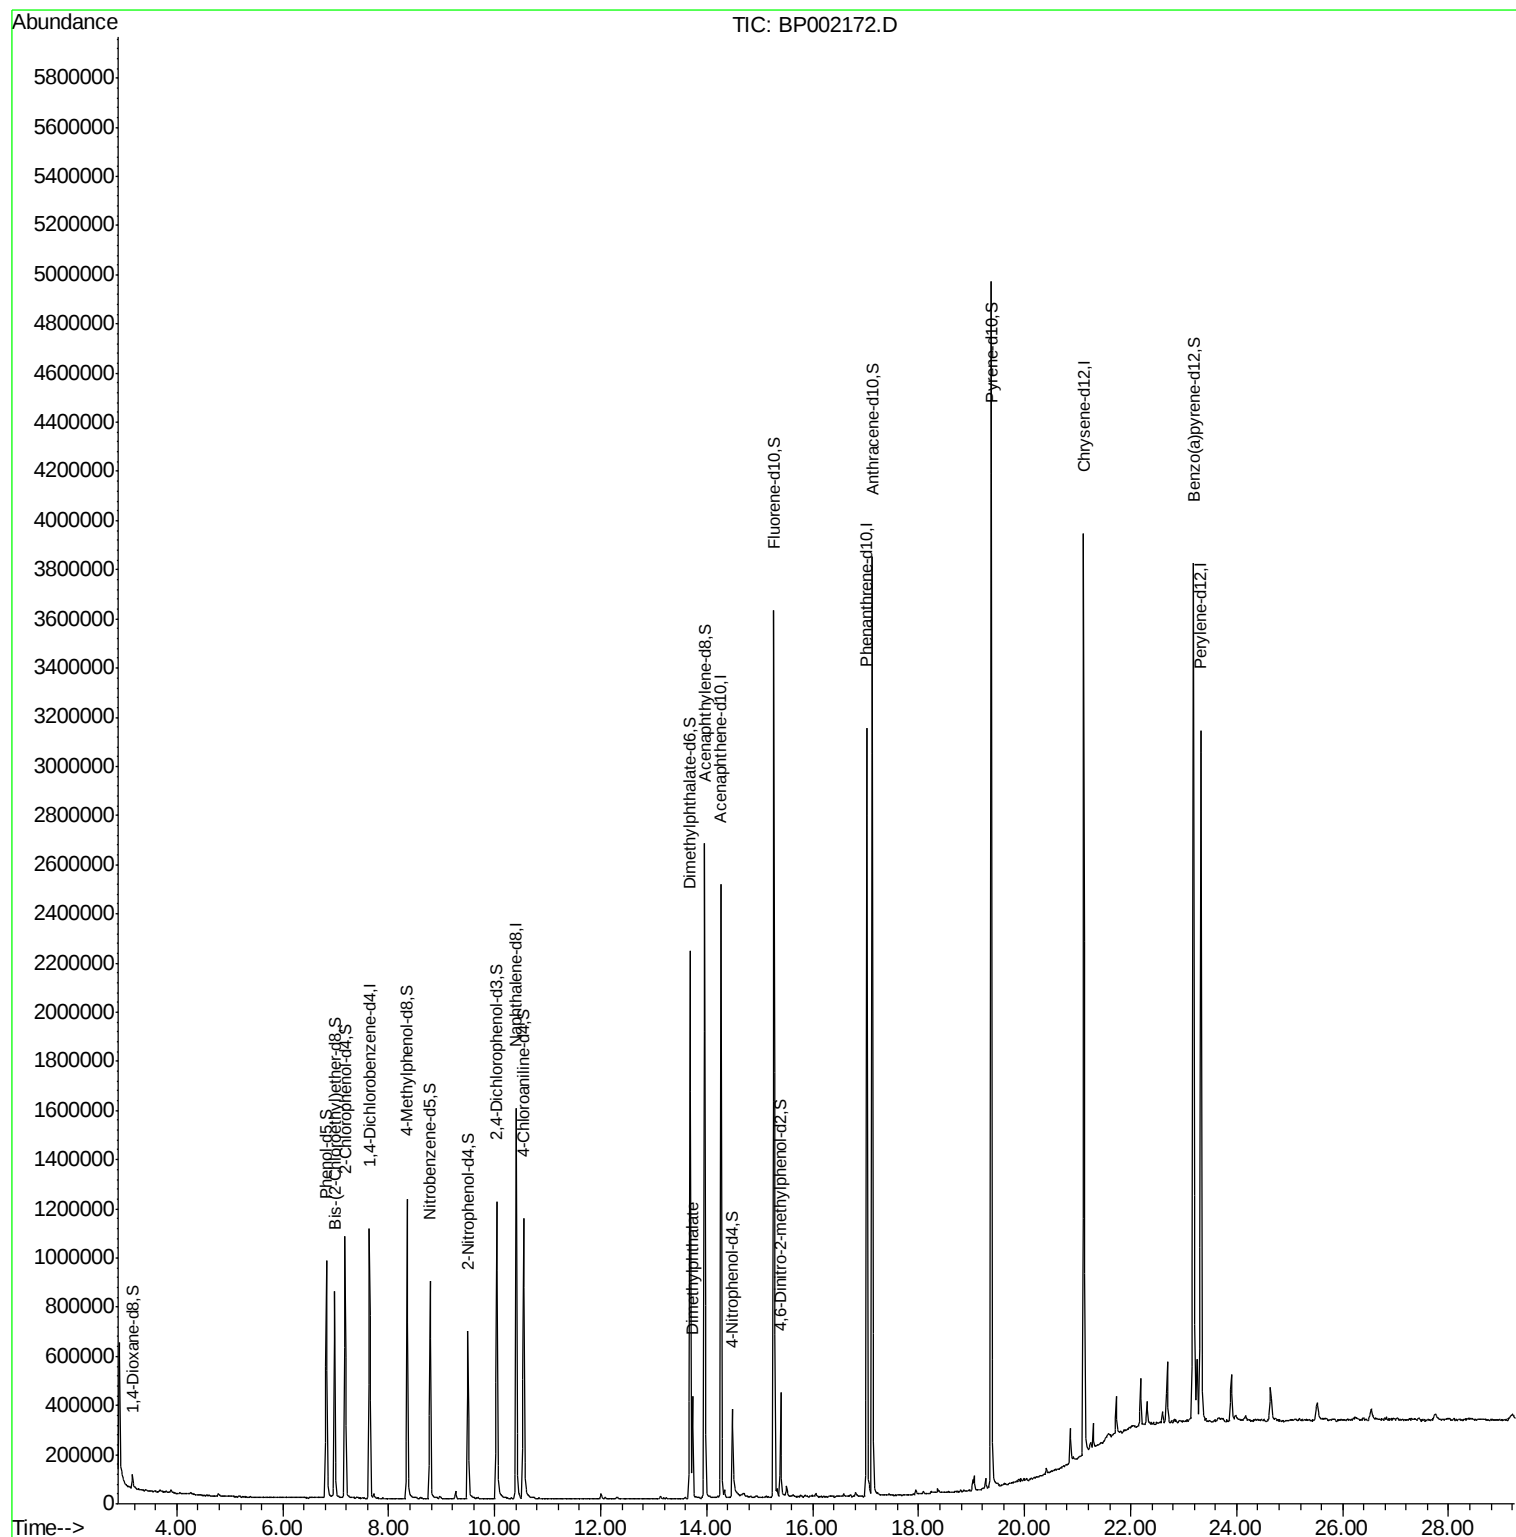

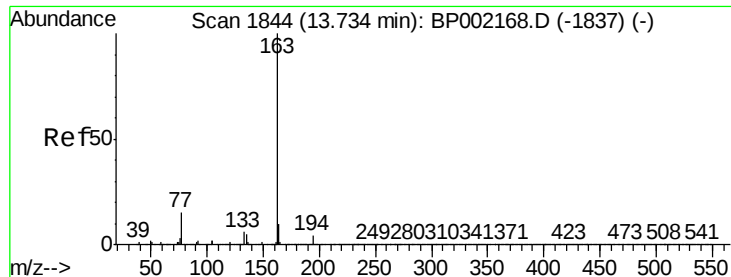

#45

Dimethylphthalate

Concen: 3.964 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.00 min

Lab File: BP002172.D

Acq: 11 Mar 2020 10:48

Instrument :

BNA_P

ClientSampleId :

C0AC1

Tot Ion:163 Resp: 274301

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.3 8.2 12.4

