

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031020\
 Data File : BP002144.D
 Acq On : 10 Mar 2020 11:43
 Operator : CG/JU
 Sample : L1828-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.987	14	17	19	rBV	19348	25329	0.58%	0.128%
2	3.116	37	39	41	rVB	8518	6671	0.15%	0.034%
3	3.140	41	43	47	rBV	6388	7360	0.17%	0.037%
4	3.416	87	90	92	rBV	7100	7768	0.18%	0.039%
5	3.446	92	95	98	rBV2	7910	11426	0.26%	0.058%
6	3.728	141	143	145	rBV	6787	7263	0.17%	0.037%
7	3.893	168	171	173	rBV3	9423	10501	0.24%	0.053%
8	4.116	206	209	212	rBV	5993	7230	0.17%	0.037%
9	4.663	300	302	304	rVB	6672	6669	0.15%	0.034%
10	4.893	340	341	346	rVV	6181	6572	0.15%	0.033%
11	4.934	346	348	351	rVB	6262	6920	0.16%	0.035%
12	4.969	351	354	356	rBV	8816	9223	0.21%	0.047%
13	5.057	366	369	370	rVV	6578	7536	0.17%	0.038%
14	5.263	400	404	407	rBV	6870	9158	0.21%	0.046%
15	5.434	431	433	436	rVB	7270	7585	0.17%	0.038%
16	5.510	443	446	447	rBV2	6213	6272	0.14%	0.032%
17	5.581	454	458	461	rBV2	3993	6337	0.14%	0.032%
18	5.634	465	467	470	rBV	6056	6828	0.16%	0.035%
19	5.781	487	492	494	rBV	7778	8945	0.20%	0.045%
20	6.099	545	546	549	rBV	6297	6361	0.15%	0.032%
21	6.140	551	553	557	rVB	6203	7837	0.18%	0.040%
22	6.210	561	565	566	rBV	4781	6269	0.14%	0.032%
23	6.346	583	588	591	rVB	6367	8995	0.21%	0.045%
24	6.446	602	605	609	rVV	5196	7481	0.17%	0.038%
25	6.646	636	639	641	rBV	6831	9329	0.21%	0.047%
26	6.952	686	691	693	rVB	4034	6518	0.15%	0.033%
27	7.081	710	713	715	rBV	6053	6811	0.16%	0.034%
28	7.169	727	728	732	rVB	7062	7250	0.17%	0.037%
29	7.281	744	747	750	rBV	10230	11268	0.26%	0.057%
30	7.340	756	757	762	rVB	7114	9716	0.22%	0.049%
31	7.399	762	767	768	rBV	8124	11672	0.27%	0.059%
32	7.634	800	807	821	rBV	893142	1535351	35.07%	7.762%
33	7.722	821	822	826	rVV	8164	8837	0.20%	0.045%
34	7.793	830	834	837	rVB	5201	8520	0.19%	0.043%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031020\
 Data File : BP002144.D
 Acq On : 10 Mar 2020 11:43
 Operator : CG/JU
 Sample : L1828-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

35	7.922	854	856	858	rBV	6950	7071	0.16%	0.036%
36	7.951	860	861	865	rVB	6481	6474	0.15%	0.033%
37	8.346	925	928	933	rBV	4179	6841	0.16%	0.035%
38	8.422	940	941	944	rVB	7928	6553	0.15%	0.033%
39	8.457	944	947	951	rBV	6696	7890	0.18%	0.040%
40	8.598	966	971	974	rBV	5150	8483	0.19%	0.043%
41	8.669	979	983	984	rBV	6683	6766	0.15%	0.034%
42	8.893	1019	1021	1024	rBV	6456	8691	0.20%	0.044%
43	8.928	1024	1027	1029	rVV	7536	10068	0.23%	0.051%
44	8.975	1031	1035	1038	rVV	7295	12995	0.30%	0.066%
45	8.998	1038	1039	1043	rVV	6976	7928	0.18%	0.040%
46	9.051	1046	1048	1052	rVB	4985	6412	0.15%	0.032%
47	9.093	1052	1055	1059	rBV	6417	11274	0.26%	0.057%
48	9.134	1059	1062	1065	rBV	6933	8840	0.20%	0.045%
49	9.175	1065	1069	1073	rVV	6778	13144	0.30%	0.066%
50	9.234	1075	1079	1081	rVB	7661	8713	0.20%	0.044%
51	9.263	1081	1084	1090	rBV	5521	12373	0.28%	0.063%
52	9.351	1094	1099	1101	rVB	5530	8324	0.19%	0.042%
53	9.381	1101	1104	1107	rBV	6432	8414	0.19%	0.043%
54	9.740	1164	1165	1168	rVB	9040	6636	0.15%	0.034%
55	9.887	1187	1190	1192	rVB	8621	8217	0.19%	0.042%
56	9.945	1196	1200	1203	rVB	6153	8404	0.19%	0.042%
57	10.010	1207	1211	1213	rBV	5383	6834	0.16%	0.035%
58	10.045	1213	1217	1220	rVB	6509	6871	0.16%	0.035%
59	10.110	1225	1228	1231	rBV	7506	10703	0.24%	0.054%
60	10.145	1231	1234	1238	rVV	4974	7607	0.17%	0.038%
61	10.410	1271	1279	1289	rBV	1228038	2130478	48.67%	10.770%
62	10.575	1306	1307	1312	rVB	10341	10620	0.24%	0.054%
63	10.610	1312	1313	1315	rBV	8874	6977	0.16%	0.035%
64	10.722	1327	1332	1334	rBV	8015	10245	0.23%	0.052%
65	10.751	1334	1337	1341	rBV	5359	7848	0.18%	0.040%
66	10.892	1357	1361	1364	rBV	5295	6965	0.16%	0.035%
67	11.092	1392	1395	1398	rBV	4856	7471	0.17%	0.038%
68	11.157	1403	1406	1409	rVV	4935	6864	0.16%	0.035%
69	11.251	1420	1422	1423	rBV	6832	6462	0.15%	0.033%
70	11.492	1461	1463	1466	rVB	9186	10056	0.23%	0.051%
71	11.528	1466	1469	1471	rBV	8349	9387	0.21%	0.047%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031020\
 Data File : BP002144.D
 Acq On : 10 Mar 2020 11:43
 Operator : CG/JU
 Sample : L1828-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

72	11.557	1471	1474	1476	rBV	9542	10389	0.24%	0.053%
73	11.628	1484	1486	1488	rBV	7574	6448	0.15%	0.033%
74	11.839	1518	1522	1524	rBV	6618	8809	0.20%	0.045%
75	12.134	1569	1572	1574	rVB	6376	7542	0.17%	0.038%
76	12.151	1574	1575	1580	rVB	6331	7014	0.16%	0.035%
77	12.357	1608	1610	1613	rBV	4936	6658	0.15%	0.034%
78	12.428	1619	1622	1625	rVB	7595	8603	0.20%	0.043%
79	12.469	1625	1629	1630	rBV	7842	8691	0.20%	0.044%
80	12.698	1666	1668	1671	rBV	6483	8047	0.18%	0.041%
81	12.845	1689	1693	1696	rBV	4074	6783	0.15%	0.034%
82	13.245	1758	1761	1763	rVB	6338	6572	0.15%	0.033%
83	14.010	1889	1891	1894	rVB	7108	9302	0.21%	0.047%
84	14.045	1894	1897	1899	rBV	8014	9594	0.22%	0.049%
85	14.181	1918	1920	1923	rBV	8315	7448	0.17%	0.038%
86	14.216	1923	1926	1928	rVB	7136	7016	0.16%	0.035%
87	14.275	1928	1936	1950	rBV2	1934290	3110861	71.06%	15.726%
88	14.475	1968	1970	1974	rBV	6448	8697	0.20%	0.044%
89	15.222	2095	2097	2101	rVB	9476	11367	0.26%	0.057%
90	15.263	2101	2104	2105	rBV	9179	10382	0.24%	0.052%
91	15.398	2125	2127	2129	rBV	6336	6337	0.14%	0.032%
92	15.727	2180	2183	2185	rBV	5769	7079	0.16%	0.036%
93	16.310	2278	2282	2285	rBV	7937	11522	0.26%	0.058%
94	16.369	2288	2292	2294	rBV	8738	9519	0.22%	0.048%
95	16.739	2353	2355	2359	rVV	6091	8394	0.19%	0.042%
96	16.810	2364	2367	2370	rBV2	14967	23501	0.54%	0.119%
97	17.022	2397	2403	2416	rBV	2342891	3676452	83.99%	18.586%
98	18.010	2569	2571	2574	rBV	9710	11520	0.26%	0.058%
99	21.121	3095	3100	3111	rBV	3210356	4135283	94.47%	20.905%
100	23.327	3468	3475	3492	rVB	2330386	4377492	100.00%	22.130%




Sum of corrected areas: 19781029

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031020\
Data File : BP002144.D
Acq On : 10 Mar 2020 11:43
Operator : CG/JU
Sample : L1828-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

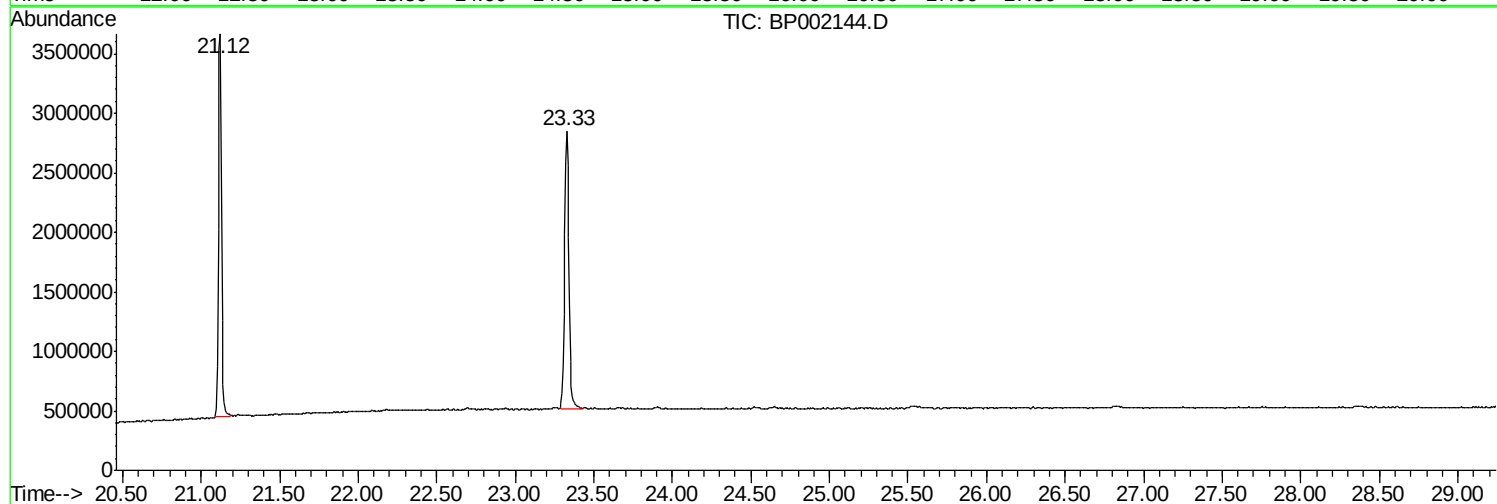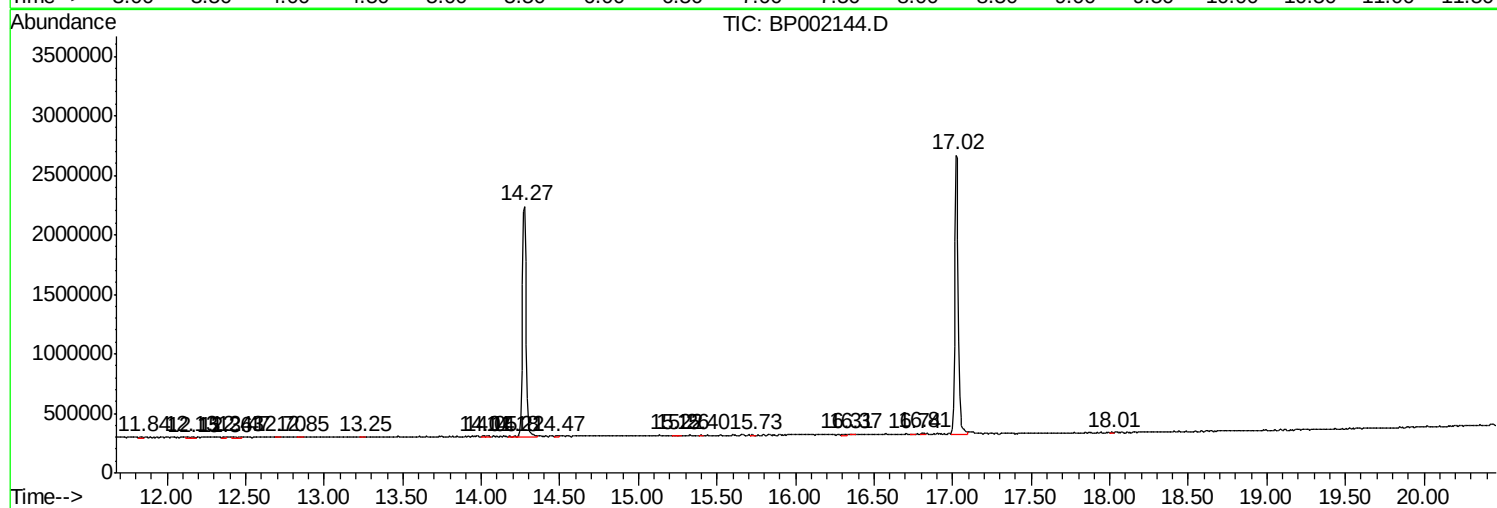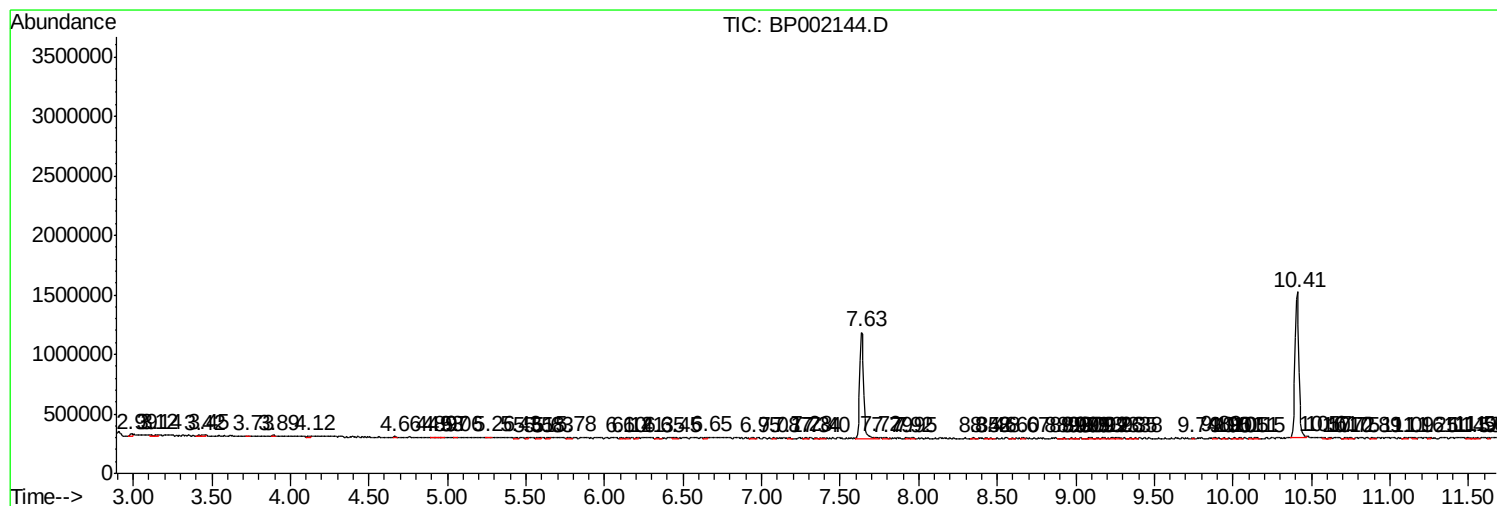

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031020\
Data_File : BP002144.D
Acq_On : 10-Mar-2020 11:433
Operator : CG/JUU
Sample : L1828-100
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
