


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031723\
 Data File : BP014114.D
 Acq On : 17 Mar 2023 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 18 00:19:43 2023

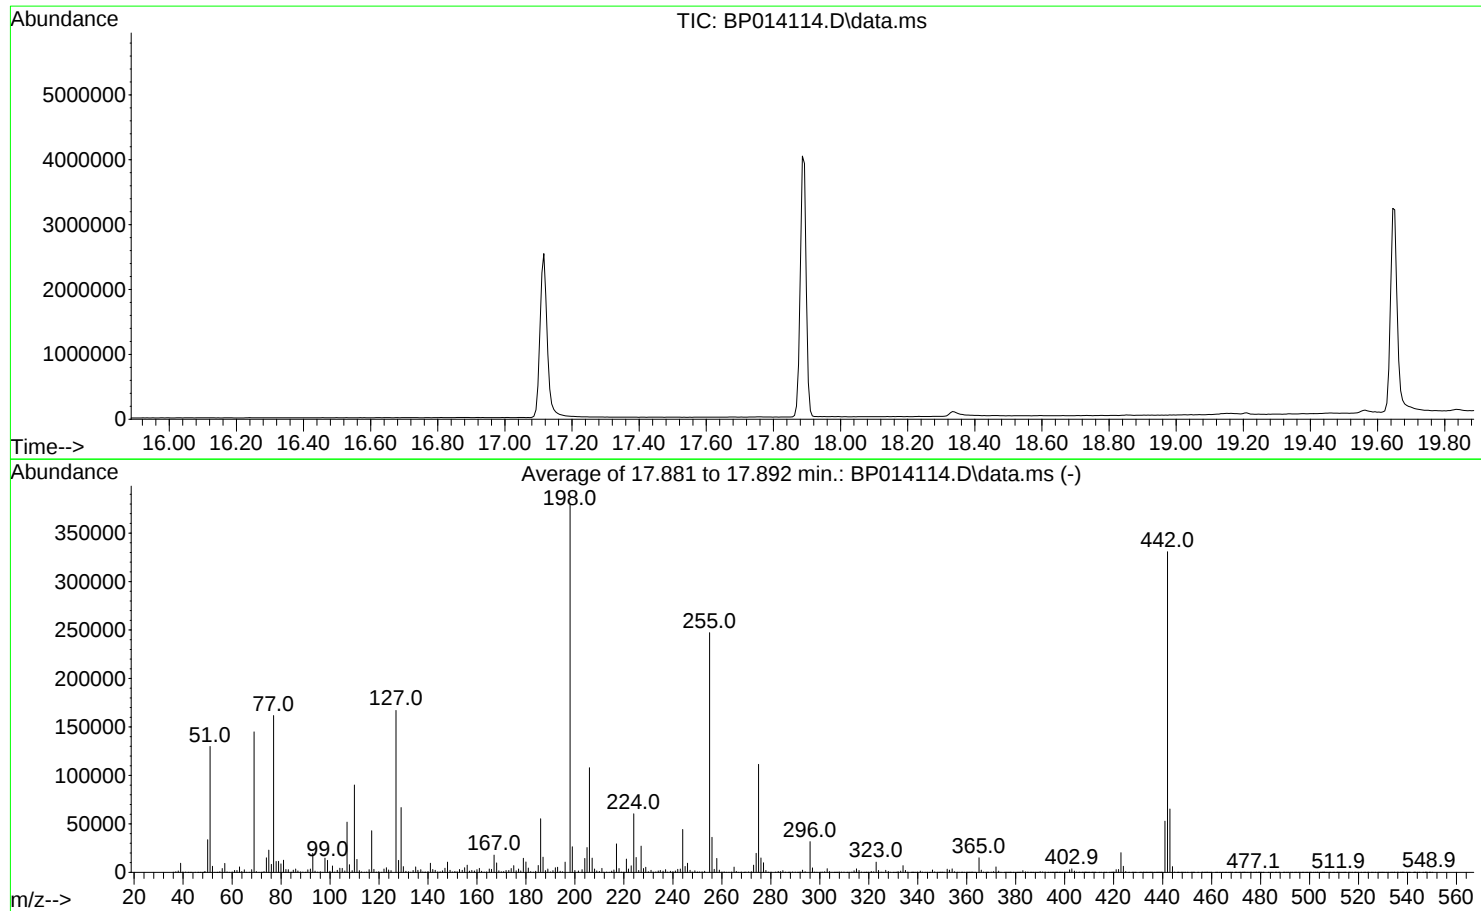

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	129867	PASS
68	69	0.00	2	2.0	2889	PASS
69	198	0.00	100	38.2	144891	PASS
70	69	0.00	2	0.6	812	PASS
127	198	10	80	44.0	167121	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	379499	PASS
199	198	5	9	6.9	26363	PASS
275	198	10	60	29.4	111444	PASS
365	198	1	100	4.0	15050	PASS
441	198	0.01	100	13.9	52789	PASS
442	442	100	100	100.0	330795	PASS
443	442	15	24	19.8	65392	PASS