
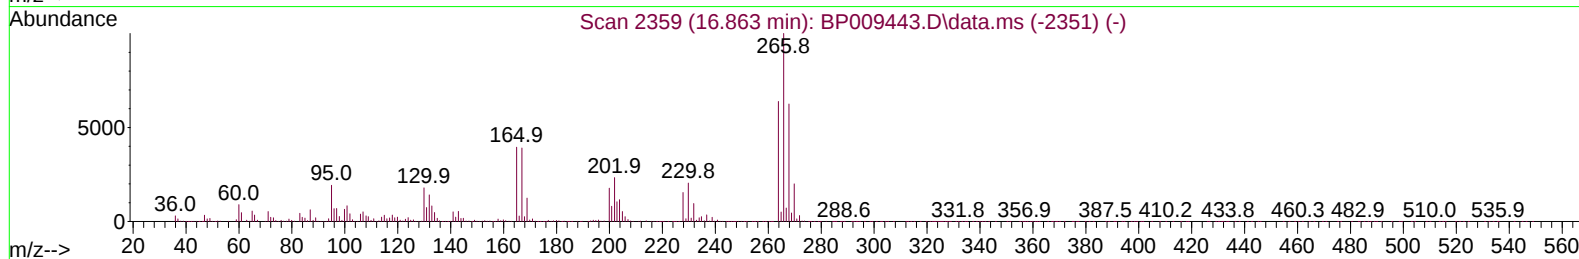
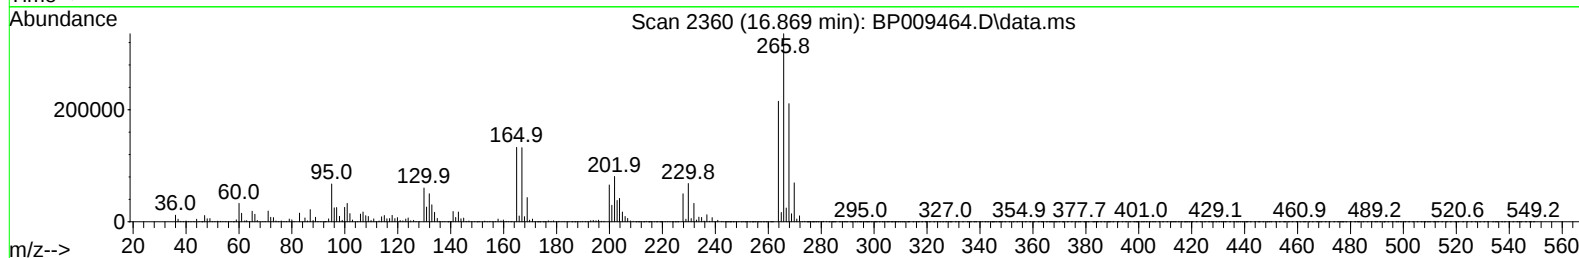


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
Data File : BP009464.D
Acq On : 21 Mar 2022 08:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 14:12:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

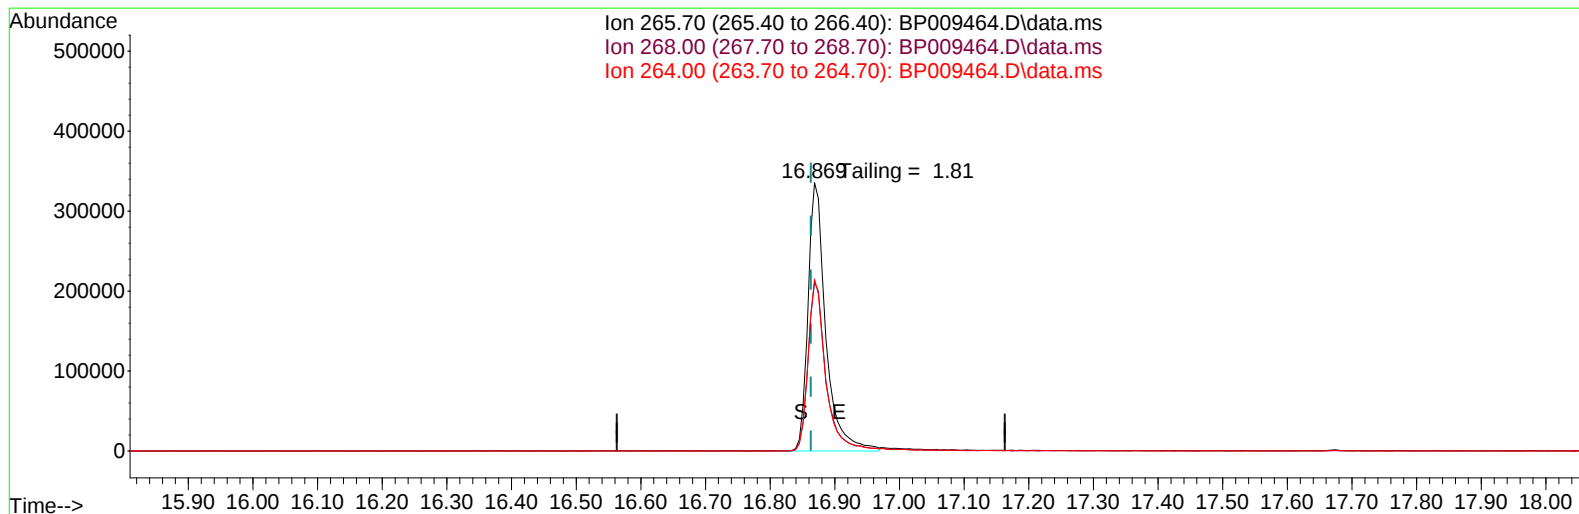

TIC: BP009464.D\data.ms

(70) Pentachlorophenol (C)




16.869min (+ 0.006) 38728.96 ng

response 652512

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.78
264.00	63.60	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
Data File : BP009464.D
Acq On : 21 Mar 2022 08:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 14:12:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

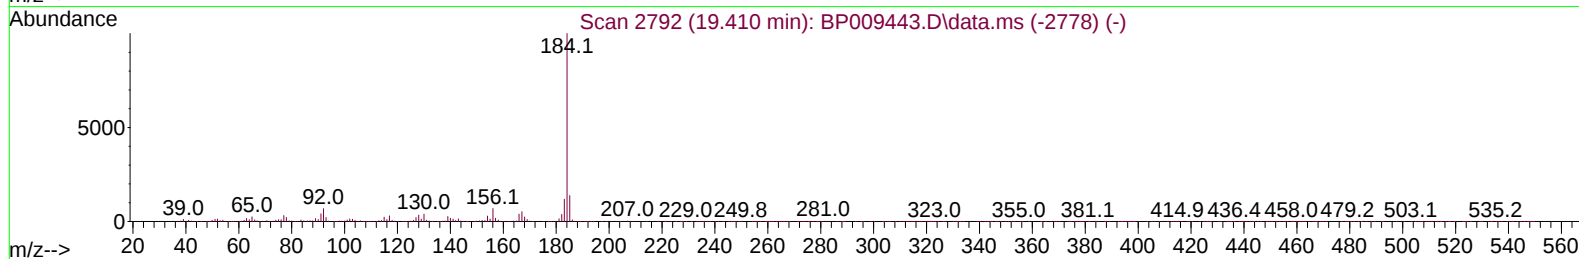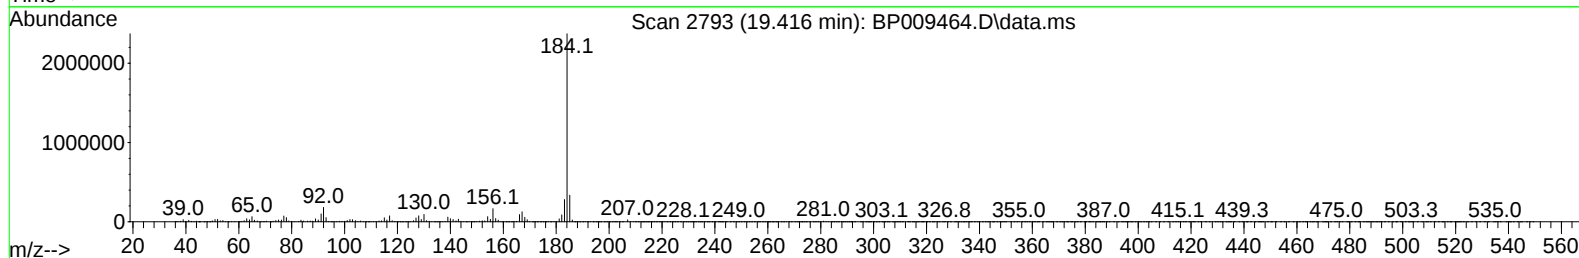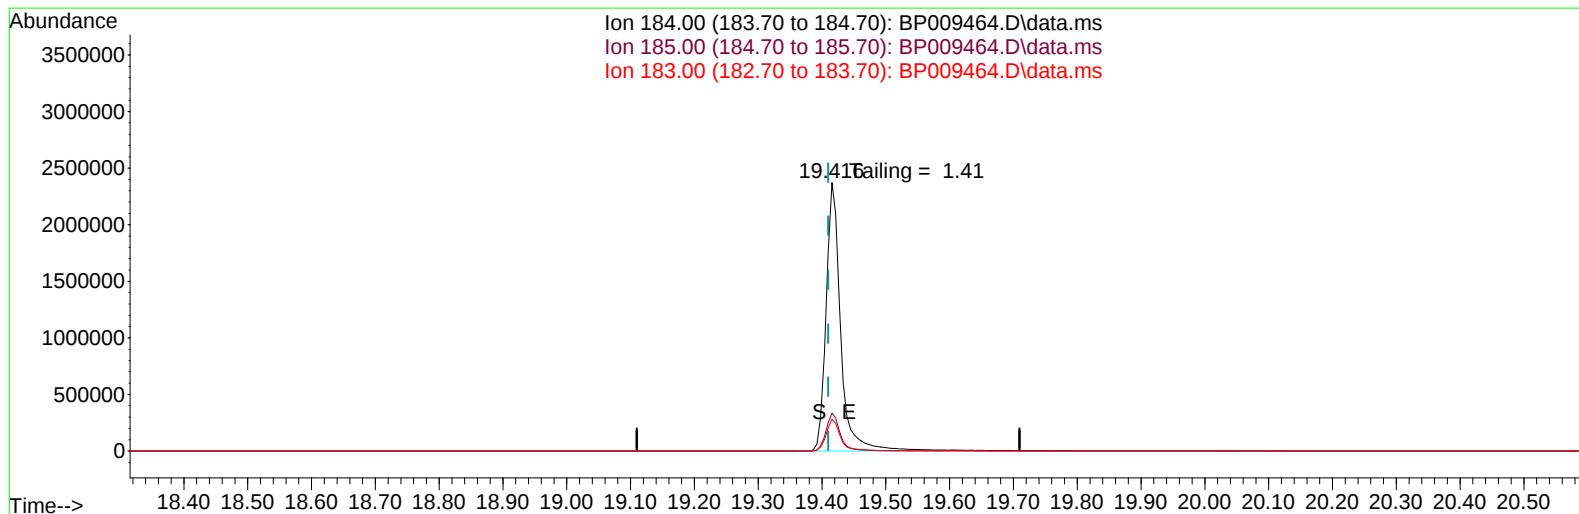

TIC: BP009464.D\data.ms

(77) Benzidine**19.416min (+ 0.006) 2116.86 ng****response 3765541**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	11.70	11.85
0.00	0.00	0.00