

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
 Data File : BP009466.D
 Acq On : 21 Mar 2022 12:32
 Operator : CG/JU
 Sample : PB143444BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143444BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	404	411	439	rBV	6908622	11649943	56.07%	11.310%
2	6.993	673	681	712	rBV	6118074	11515951	55.42%	11.180%
3	7.799	811	818	833	rBV	1385615	2390944	11.51%	2.321%
4	8.957	1007	1015	1040	rBV	3875511	7487482	36.04%	7.269%
5	10.598	1284	1294	1324	rBV	1383081	3208360	15.44%	3.115%
6	13.069	1704	1714	1751	rBV	10368508	17344190	83.48%	16.838%
7	14.445	1940	1948	1971	rBV	2201950	4049928	19.49%	3.932%
8	15.945	2195	2203	2247	rBV	6568626	11883788	57.20%	11.537%
9	17.210	2411	2418	2440	rBV	2217218	4450503	21.42%	4.321%
10	19.786	2850	2856	2871	rBV	15220124	20777669	100.00%	20.172%
11	21.327	3112	3118	3132	rBV	2475295	4343737	20.91%	4.217%
12	23.733	3520	3527	3540	rVB2	1565394	3900807	18.77%	3.787%




Sum of corrected areas: 103003302

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
Data File : BP009466.D
Acq On : 21 Mar 2022 12:32
Operator : CG/JU
Sample : PB143444BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143444BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

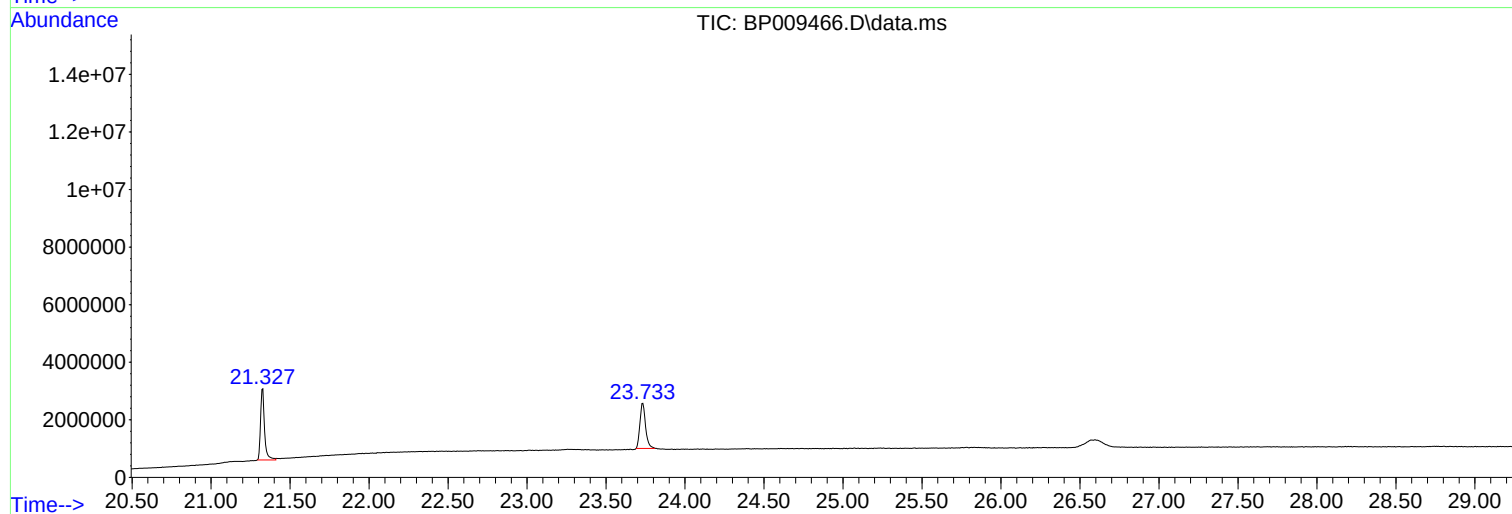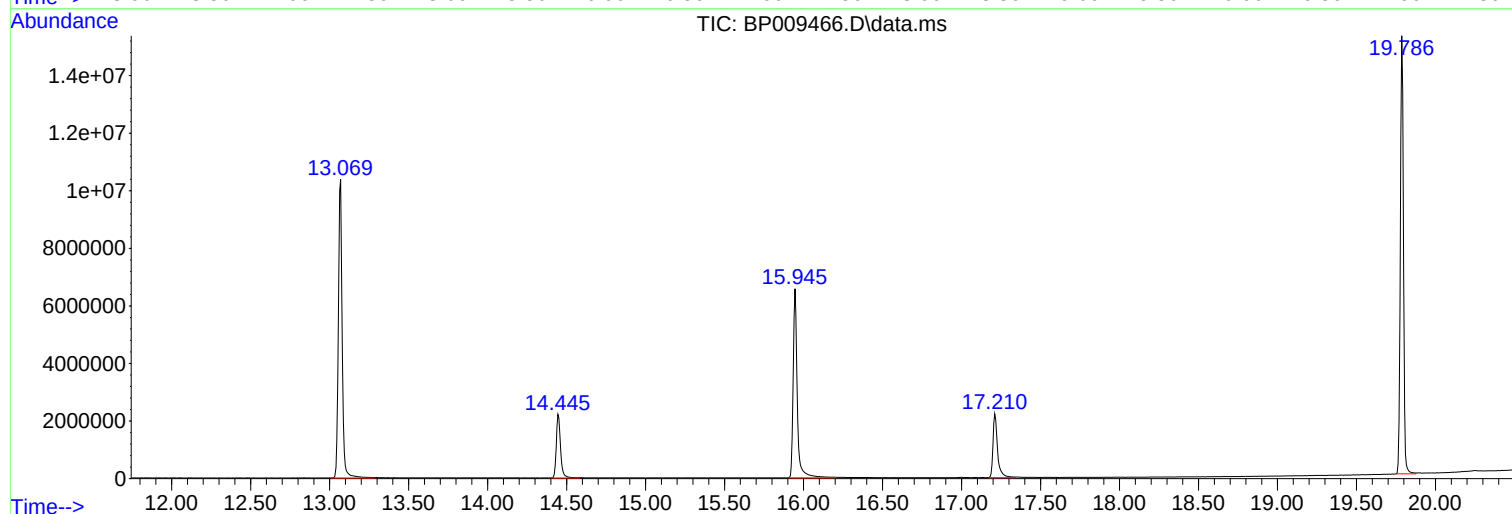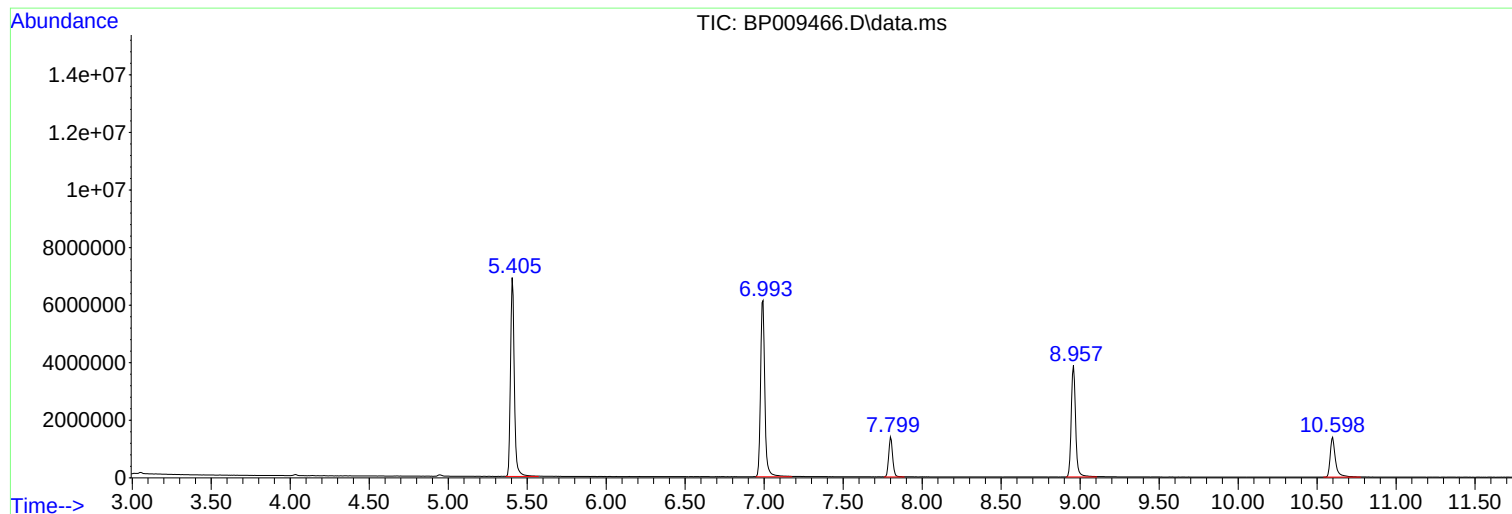

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
Data File : BP009466.D
Acq On : 21 Mar 2022 12:32
Operator : CG/JU
Sample : PB143444BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143444BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032122\
Data File : BP009466.D
Acq On : 21 Mar 2022 12:32
Operator : CG/JU
Sample : PB143444BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143444BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------