
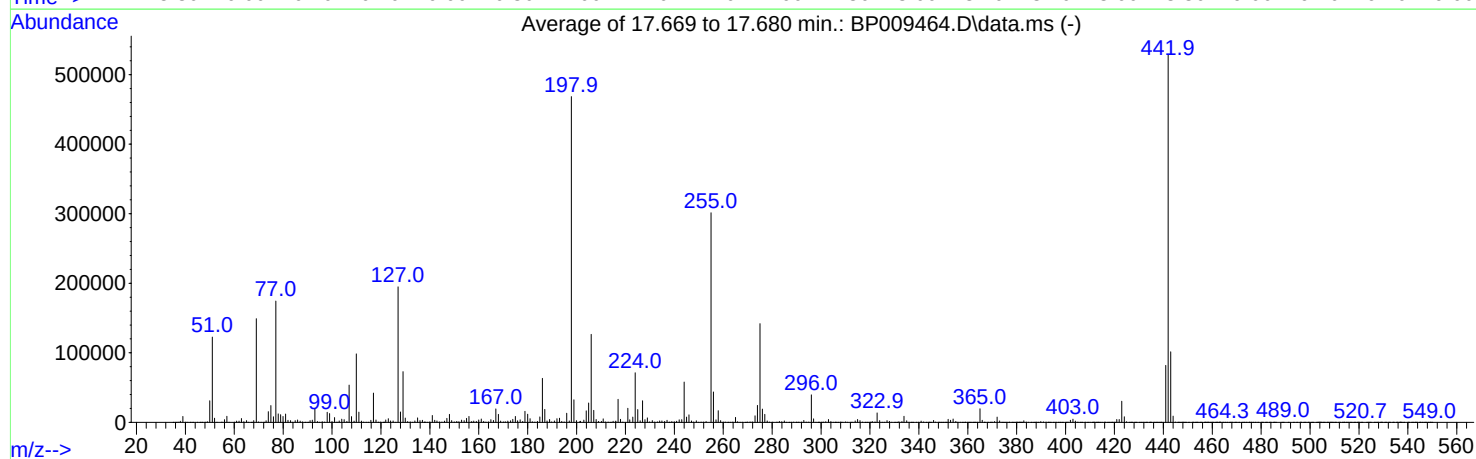


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032122\  
 Data File : BP009464.D  
 Acq On : 21 Mar 2022 08:30  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Mar 17 18:26:53 2022

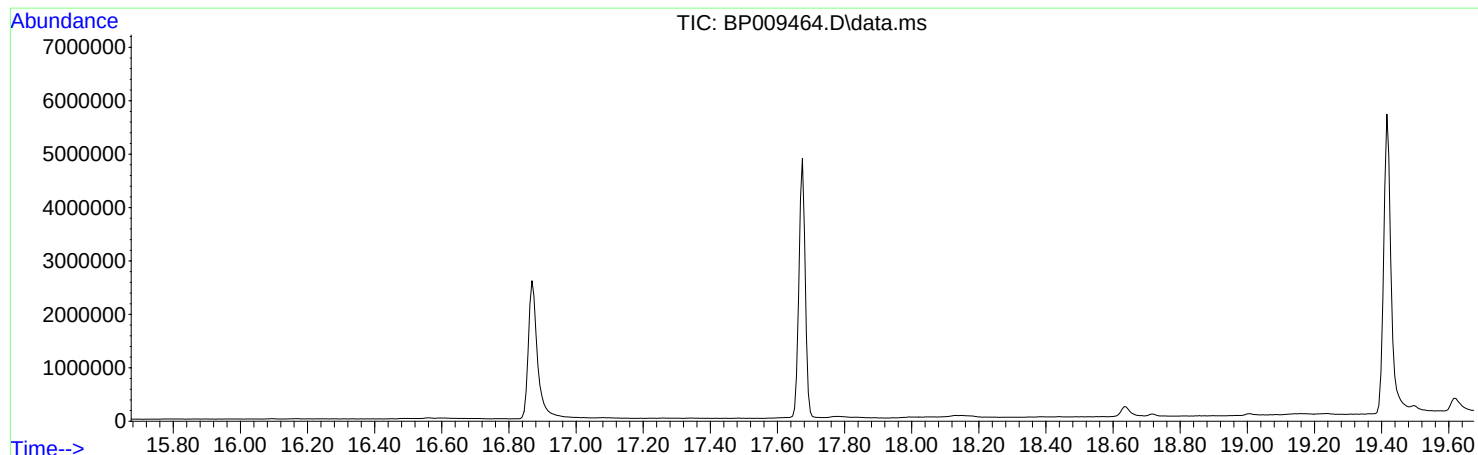




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2486

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 26.2         | 122721     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 2501       | PASS                |
| 69             | 198             | 0.00            | 100             | 31.8         | 149152     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 793        | PASS                |
| 127            | 198             | 10              | 80              | 41.6         | 194916     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 2158       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 468519     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 32360      | PASS                |
| 275            | 198             | 10              | 60              | 30.3         | 141904     | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 19509      | PASS                |
| 441            | 198             | 0.01            | 100             | 17.5         | 81902      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 528953     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 101377     | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032122\  
 Data File : BP009464.D  
 Acq On : 21 Mar 2022 08:30  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 21 14:12:46 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Mar 17 18:26:53 2022  
 Response via : Initial Calibration

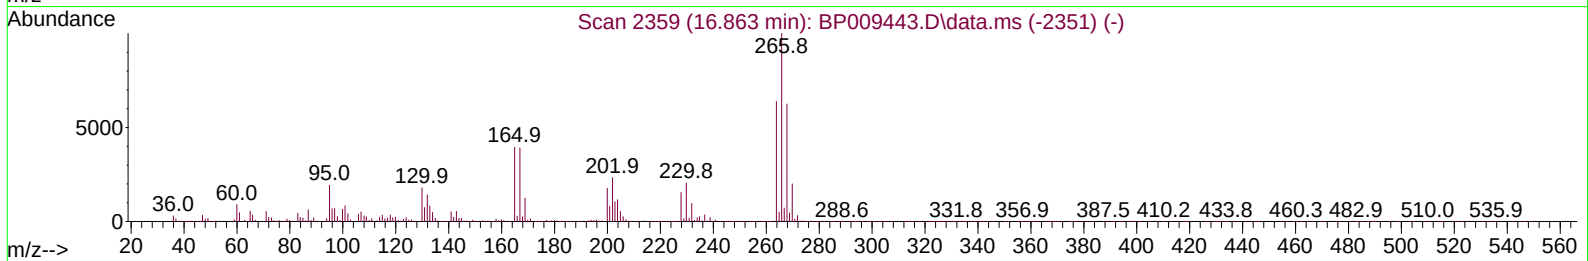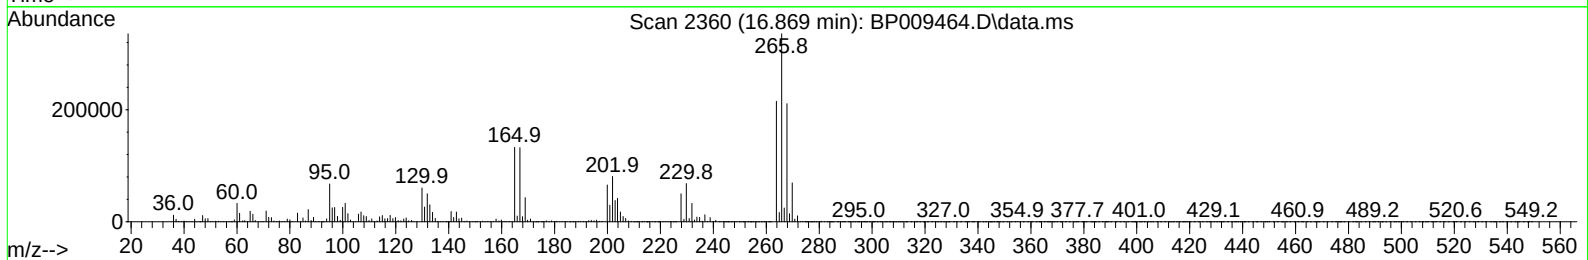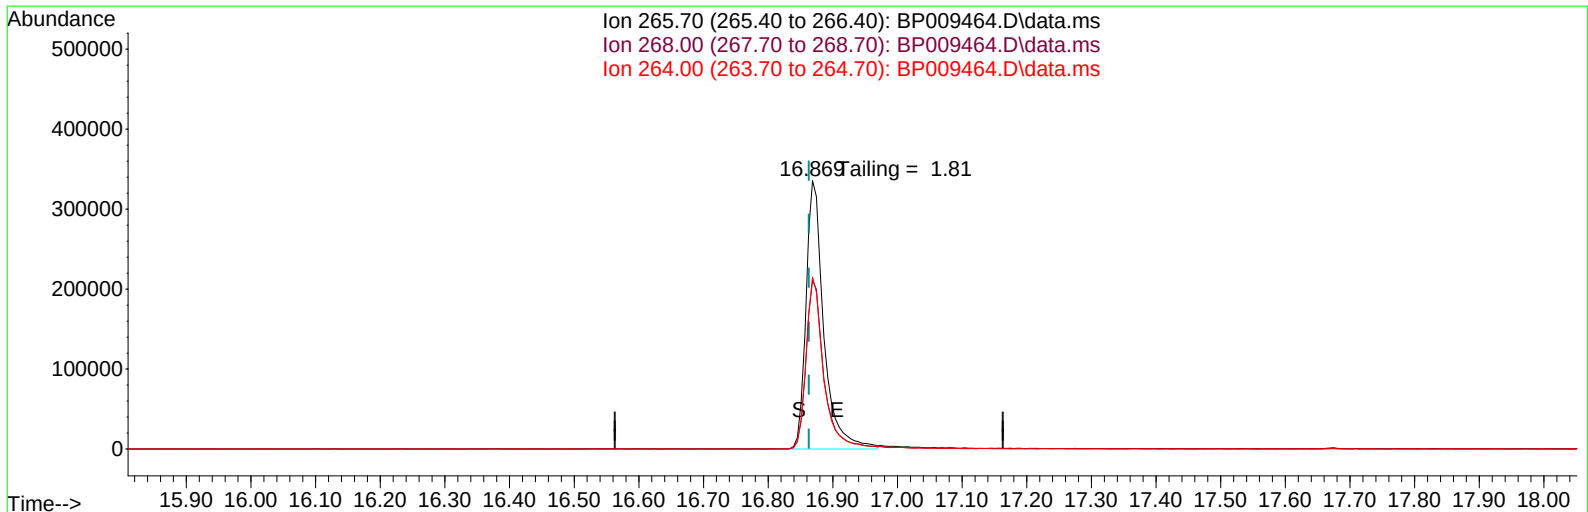

TIC: BP009464.D\data.ms

**(70) Pentachlorophenol (C)**

16.869min (+ 0.006) 38728.96 ng




response 652512

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.30  | 62.78  |
| 264.00 | 63.60  | 64.10  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032122\  
Data File : BP009464.D  
Acq On : 21 Mar 2022 08:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Mar 21 14:12:46 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 17 18:26:53 2022  
Response via : Initial Calibration

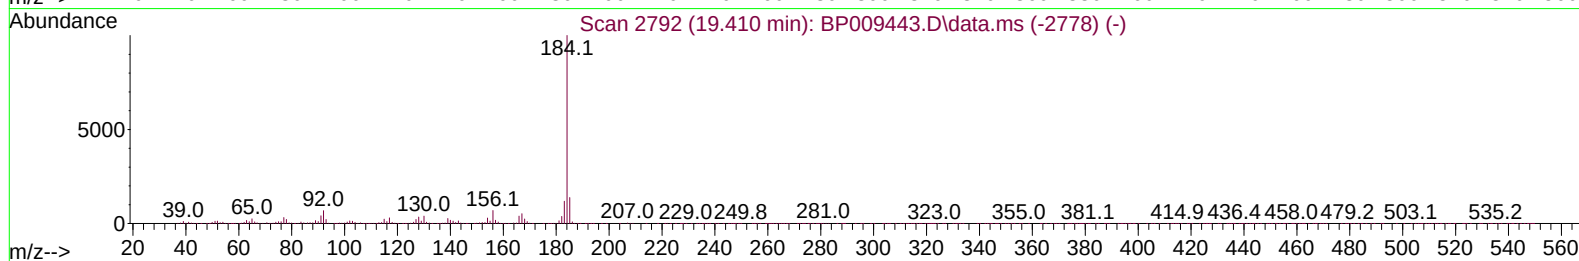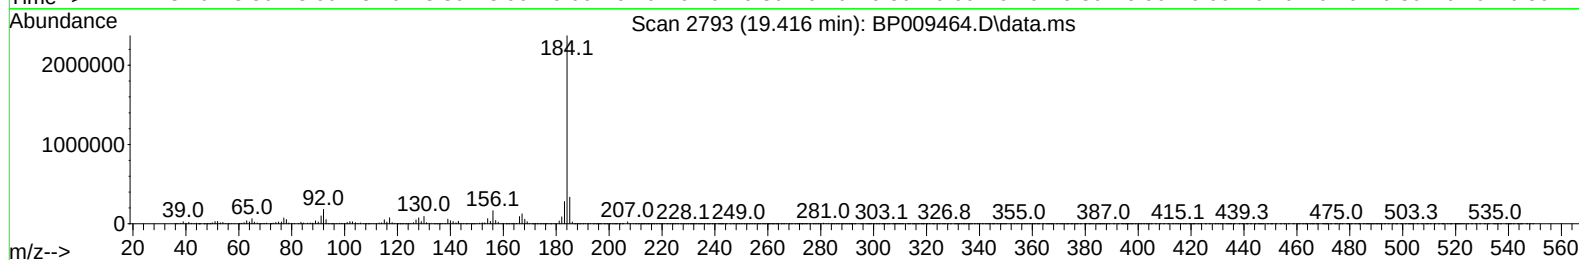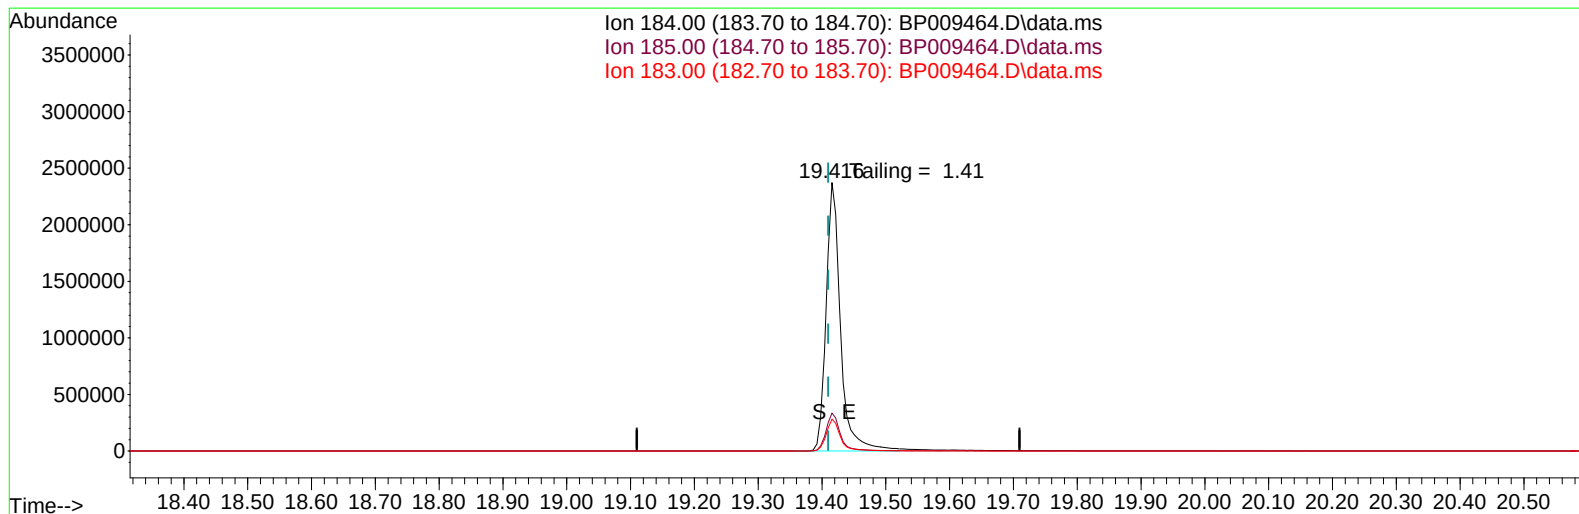

TIC: BP009464.D\data.ms

**(77) Benzidine**

**19.416min (+ 0.006) 2116.86 ng**

**response 3765541**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.15  |
| 183.00 | 11.70  | 11.85  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/21/2022     | BNA_P            | <u>BP009464.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1819819          | 20.62              |
| DDD           | 10796            | 20.19              |
| DDE           | 2804             | 19.7               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13600         | 1833419          | 0.74               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP