

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009524.D
 Acq On : 24 Mar 2022 01:22
 Operator : CG/JU
 Sample : N2071-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PILE

Quant Time: Mar 24 02:15:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 01:19:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	437965	20.000	ng	0.00
21) Naphthalene-d8	10.581	136	1815488	20.000	ng	0.00
39) Acenaphthene-d10	14.434	164	1209936	20.000	ng	0.00
64) Phenanthrene-d10	17.198	188	2418881	20.000	ng	0.00
76) Chrysene-d12	21.316	240	1804748	20.000	ng	0.00
86) Perylene-d12	23.721	264	1904069	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.399	112	213427	8.508	ng	0.00
7) Phenol-d6	6.981	99	280893	8.280	ng	0.00
23) Nitrobenzene-d5	8.951	82	184204	5.392	ng	0.00
42) 2,4,6-Tribromophenol	15.933	330	128633	6.443	ng	0.00
45) 2-Fluorobiphenyl	13.051	172	491132	5.627	ng	0.00
79) Terphenyl-d14	19.774	244	680431	6.767	ng	0.00
Target Compounds						
						Qvalue
15) Benzyl Alcohol	8.040	79	318193	11.764	ng	99
78) Pyrene	19.574	202	301110	2.532	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009524.D
Acq On : 24 Mar 2022 01:22
Operator : CG/JU
Sample : N2071-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PILE

Quant Time: Mar 24 02:15:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 01:19:11 2022
Response via : Initial Calibration




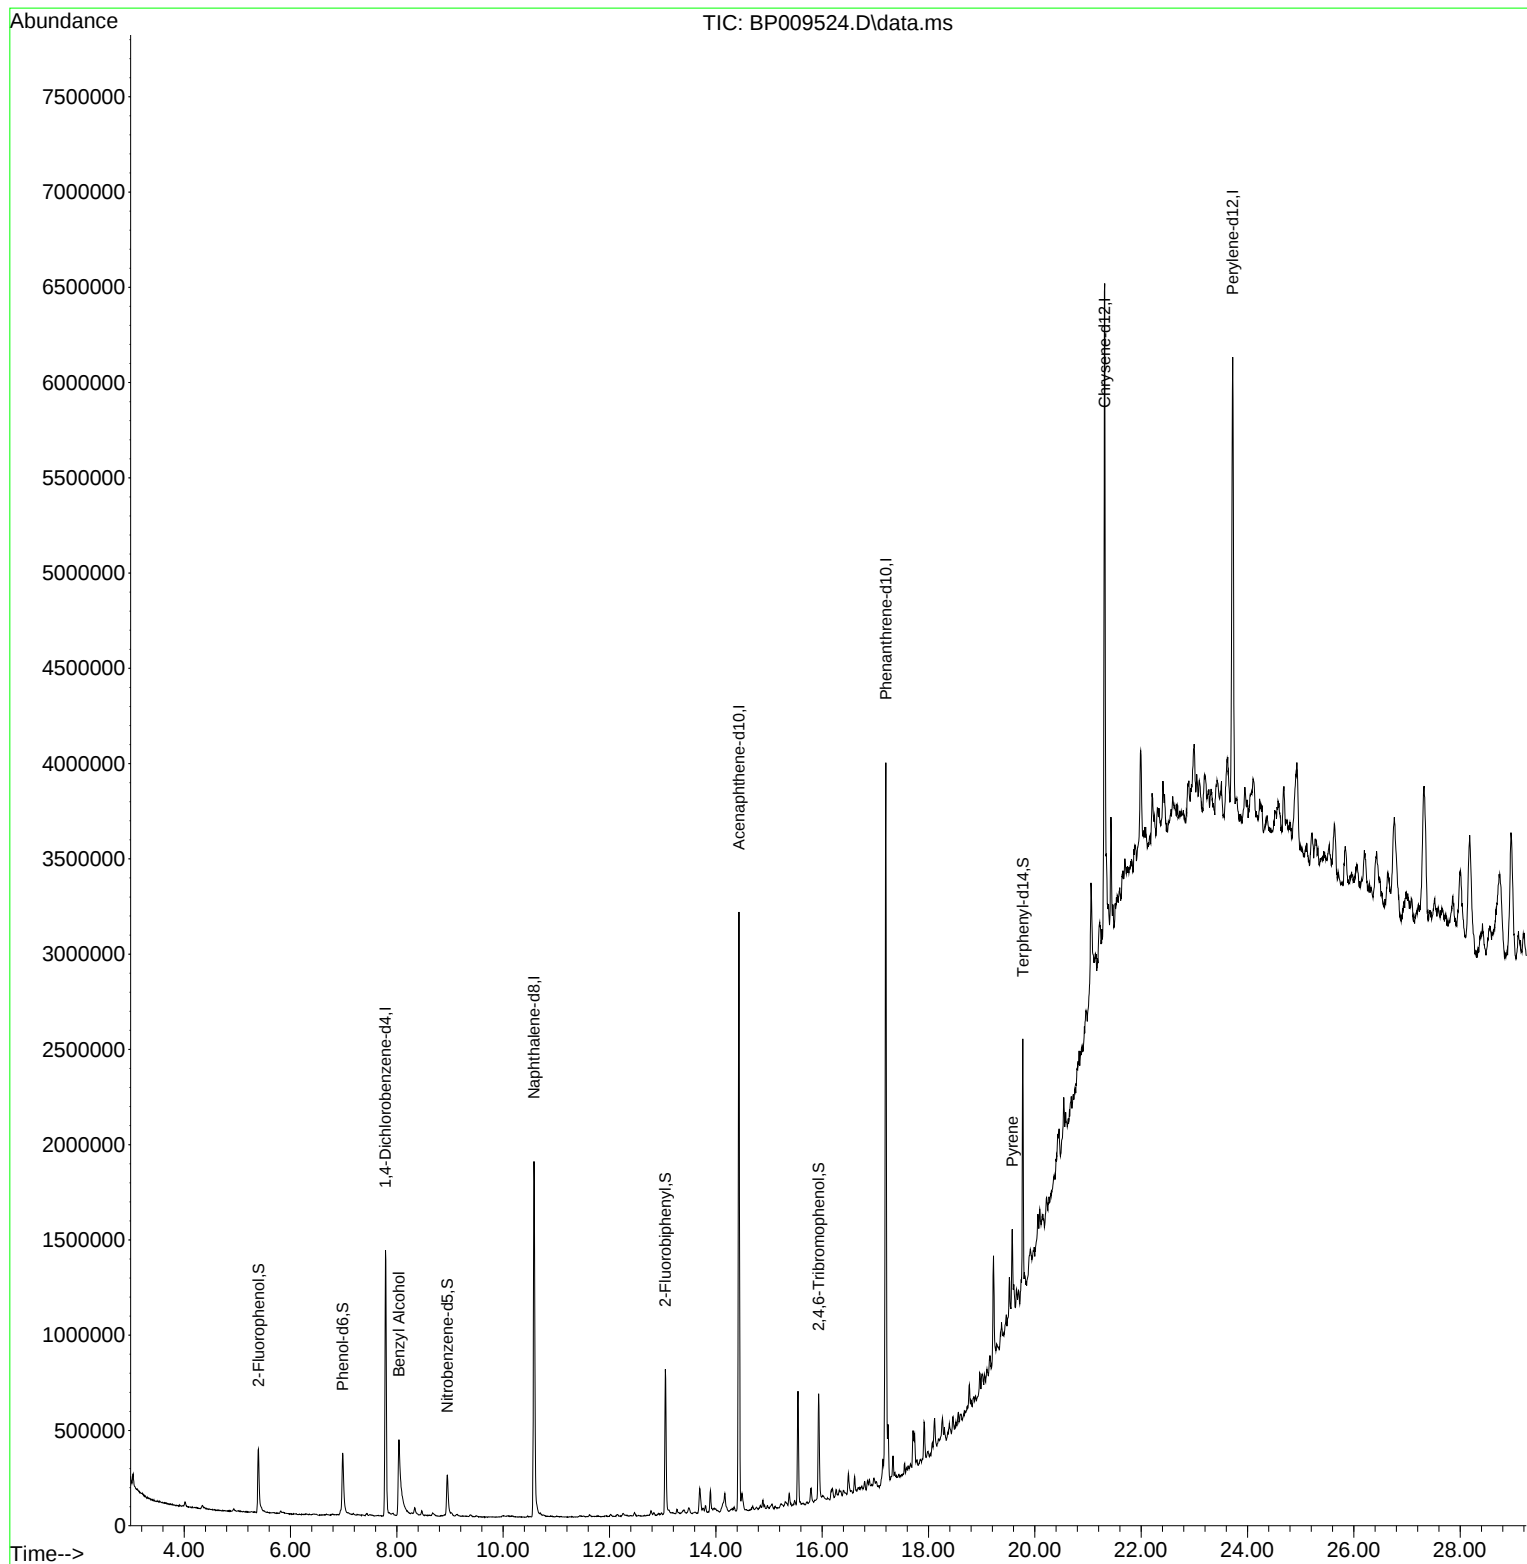


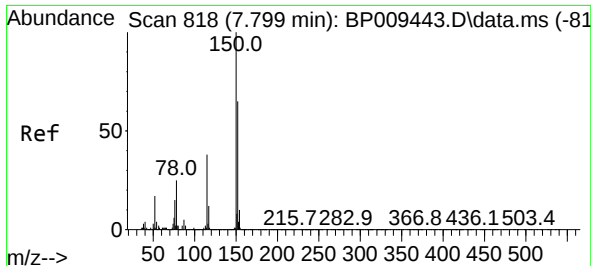

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.787 min Scan# 81
Delta R.T. -0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22




Instrument :
BNA_P
ClientSampleId :
PILE


Tgt Ion:152 Resp: 437965
Ion Ratio Lower Upper
152 100
150 157.0 124.5 186.7
115 58.5 48.2 72.4

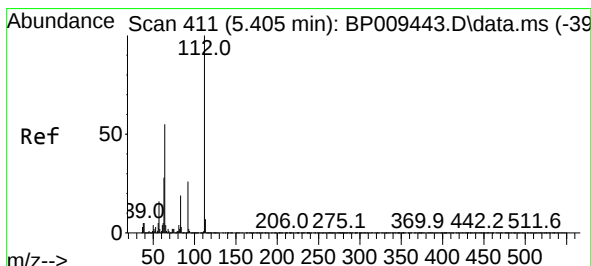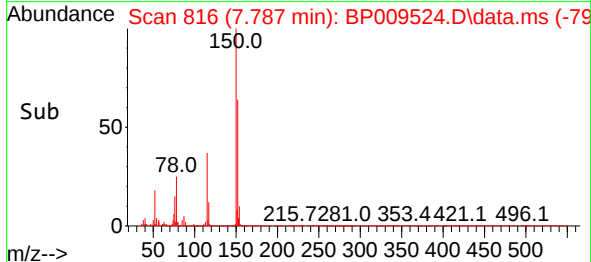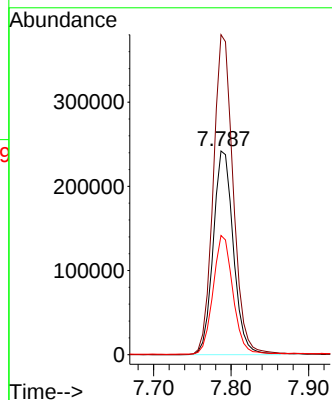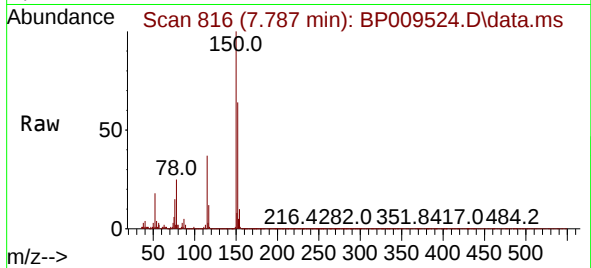

#5
2-Fluorophenol
Concen: 8.508 ng
RT: 5.399 min Scan# 410
Delta R.T. 0.006 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22

Tgt Ion:112 Resp: 213427
Ion Ratio Lower Upper
112 100
64 55.7 45.0 67.4
63 27.2 23.0 34.6


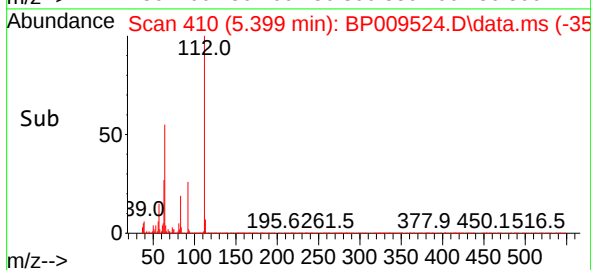
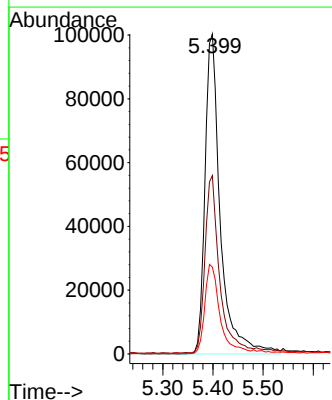
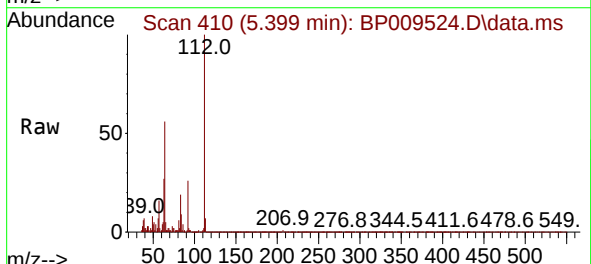


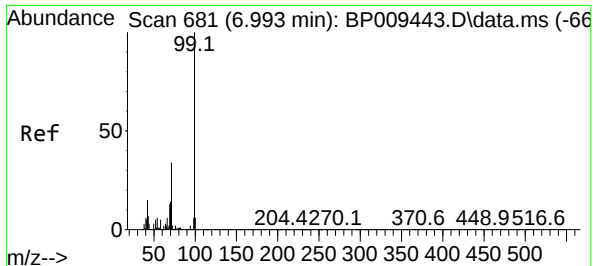

#7
Phenol-d6
Concen: 8.280 ng
RT: 6.981 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22




Instrument :
BNA_P
ClientSampleId :
PILE


Tgt Ion: 99 Resp: 280893
Ion Ratio Lower Upper
99 100
42 15.7 12.8 19.2
71 32.6 26.3 39.5

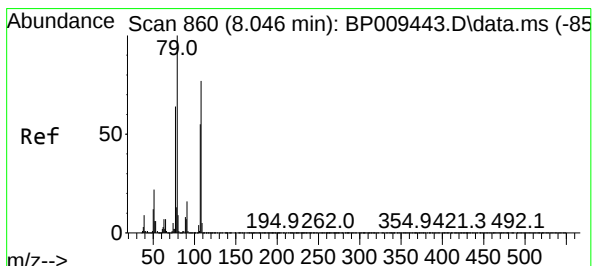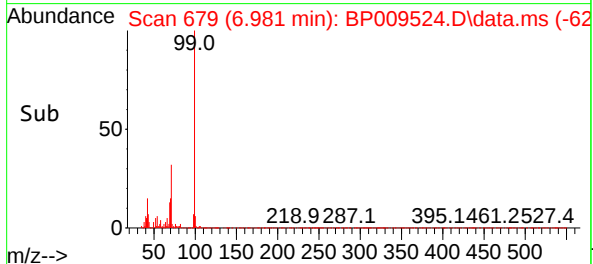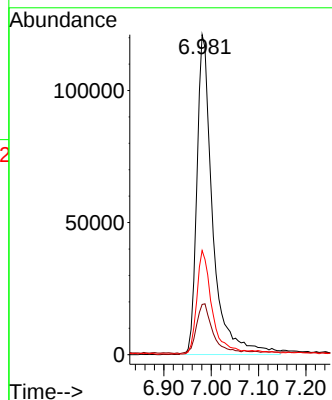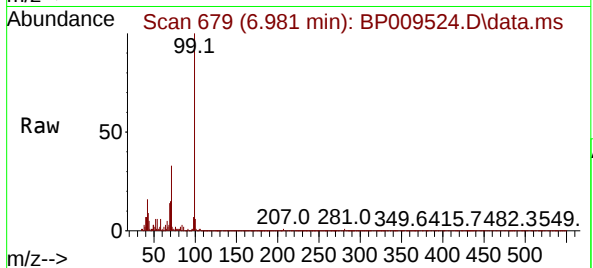

#15
Benzyl Alcohol
Concen: 11.764 ng
RT: 8.040 min Scan# 859
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22

Tgt Ion: 79 Resp: 318193
Ion Ratio Lower Upper
79 100
108 78.8 62.5 93.7
77 65.9 51.7 77.5

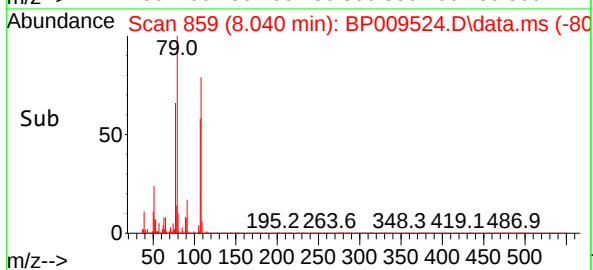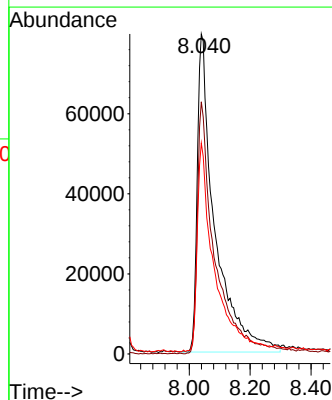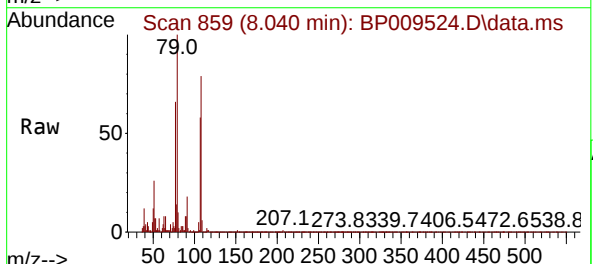

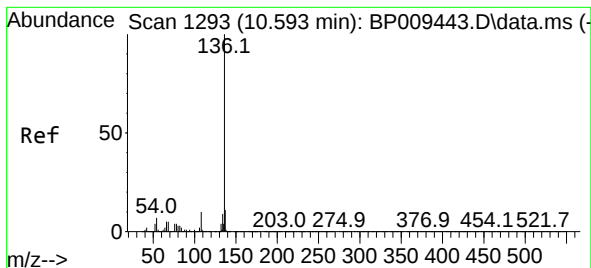

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.581 min Scan# 1014

Delta R.T. 0.000 min

Lab File: BP009524.D

Acq: 24 Mar 2022 01:22

Instrument :

BNA_P

ClientSampleId :

PILE

Tgt Ion:136 Resp: 1815488





Ion Ratio Lower Upper

136 100

137 11.0 8.6 12.8

54 7.1 5.8 8.8

68 6.1 5.2 7.8

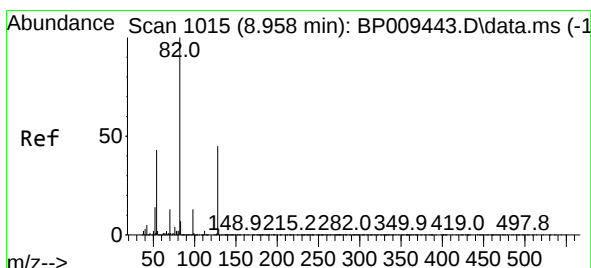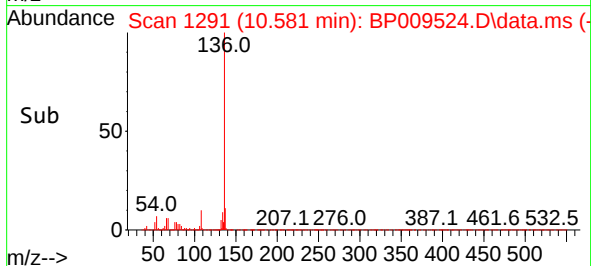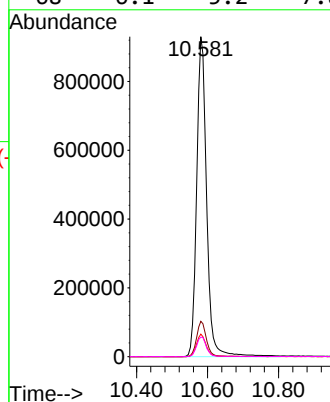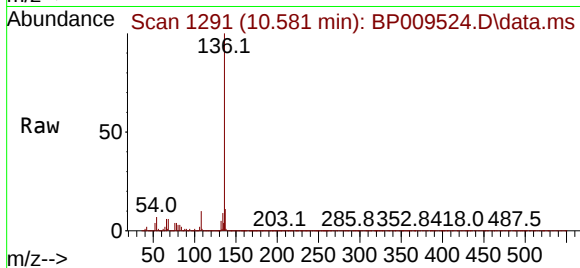

#23

Nitrobenzene-d5

Concen: 5.392 ng

RT: 8.951 min Scan# 1014

Delta R.T. 0.006 min

Lab File: BP009524.D

Acq: 24 Mar 2022 01:22




Tgt Ion: 82 Resp: 184204


Ion Ratio Lower Upper

82 100

128 42.2 34.2 51.4

54 42.2 34.7 52.1


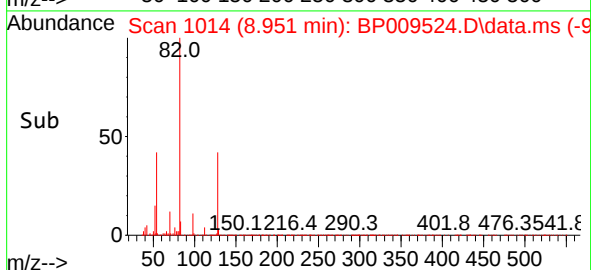
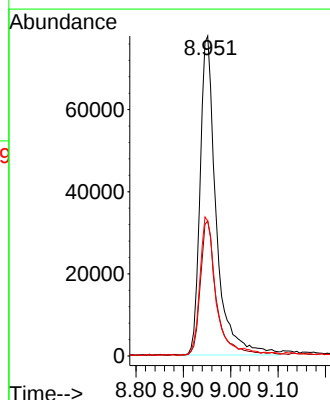
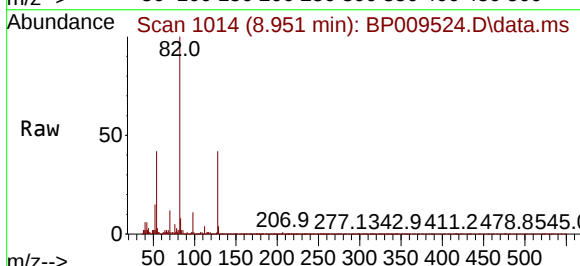


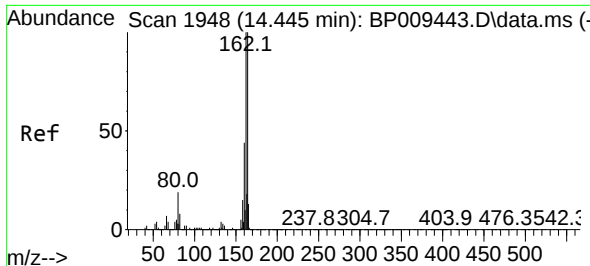

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.434 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22




Instrument :
BNA_P
ClientSampleId :
PILE


Tgt Ion:164 Resp: 1209936
Ion Ratio Lower Upper
164 100
162 100.8 79.1 118.7
160 44.2 34.9 52.3

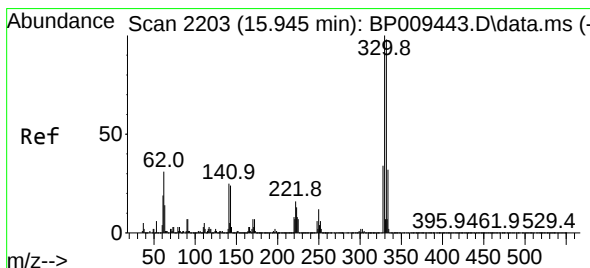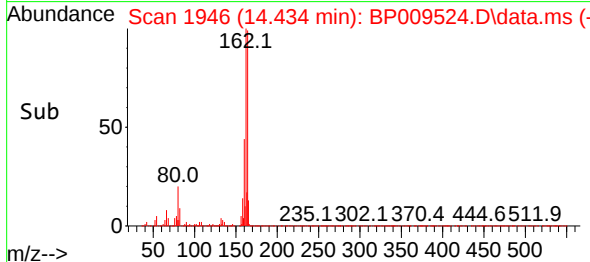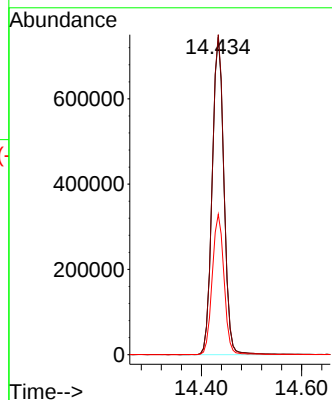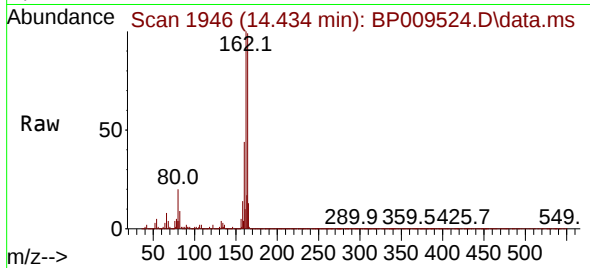

#42
2,4,6-Tribromophenol
Concen: 6.443 ng
RT: 15.933 min Scan# 2201
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22

Tgt Ion:330 Resp: 128633
Ion Ratio Lower Upper
330 100
332 97.1 77.0 115.6
141 29.5 27.6 41.4


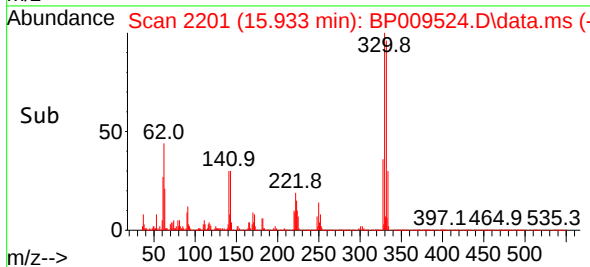
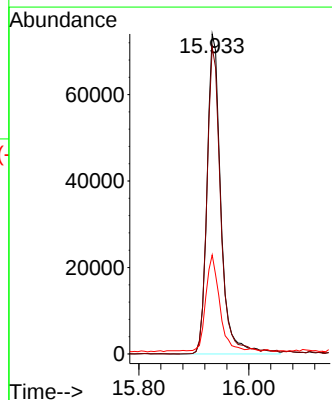
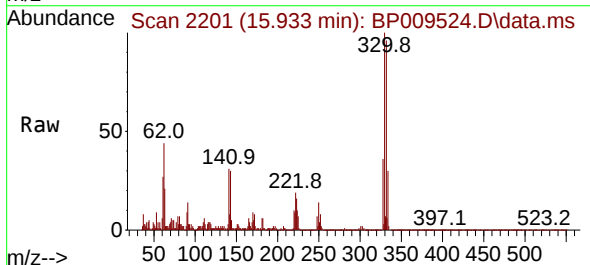


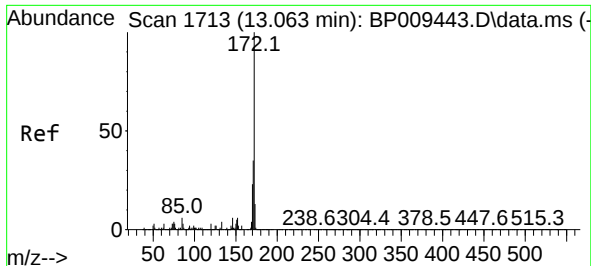

#45
2-Fluorobiphenyl
Concen: 5.627 ng
RT: 13.051 min Scan# 1711
Delta R.T. -0.006 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22




Instrument :
BNA_P
ClientSampleId :
PILE


Tgt Ion:172 Resp: 491132
Ion Ratio Lower Upper
172 100
171 34.7 28.0 42.0
170 24.4 18.6 27.8

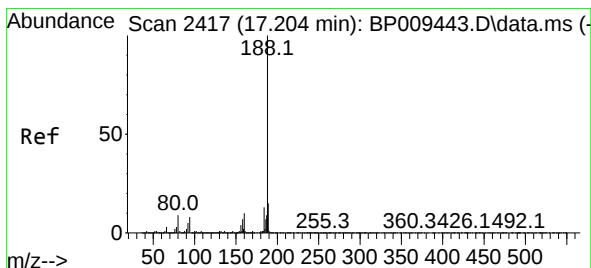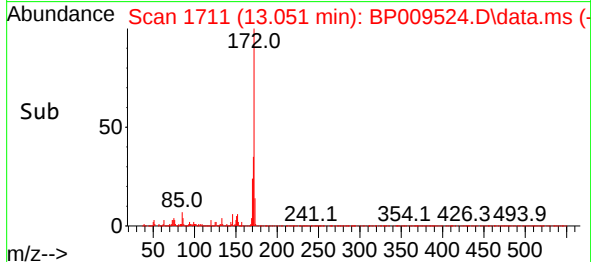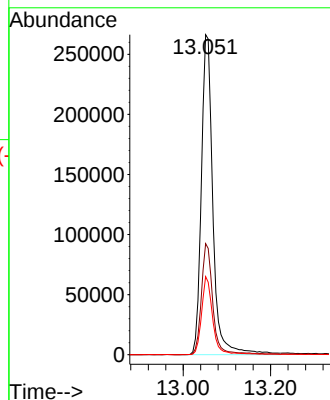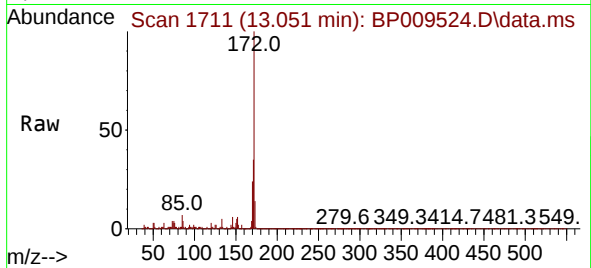

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.198 min Scan# 2416
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22

Tgt Ion:188 Resp: 2418881
Ion Ratio Lower Upper
188 100
94 8.7 7.9 11.9
80 9.7 8.8 13.2


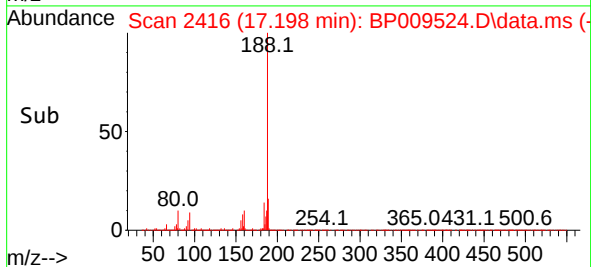
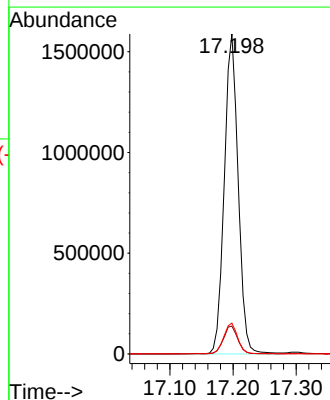
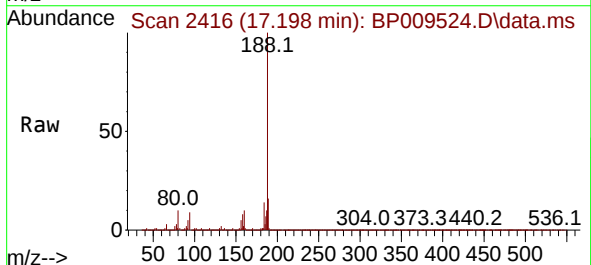


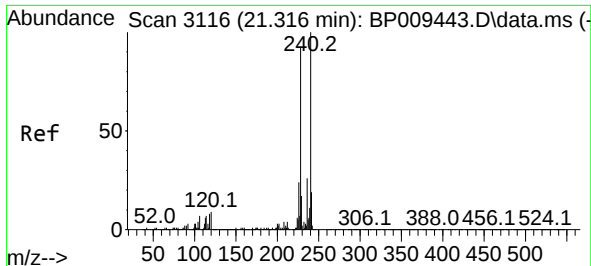

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.316 min Scan# 3116
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22




Instrument :
BNA_P
ClientSampleId :
PILE


Tgt Ion:240 Resp: 1804748
Ion Ratio Lower Upper
240 100
120 9.6 9.0 13.4
236 26.5 20.6 30.8

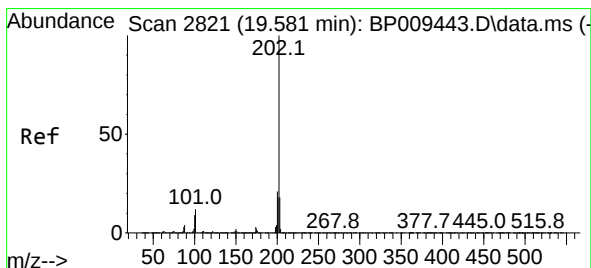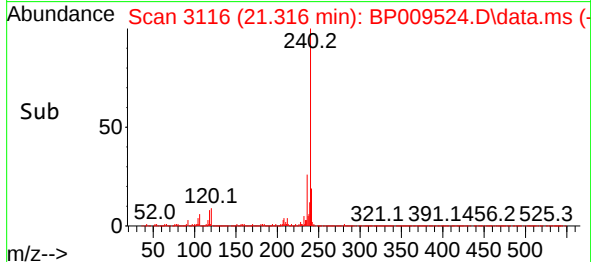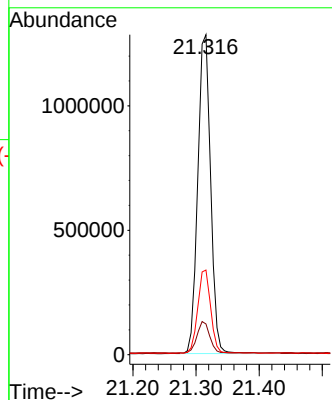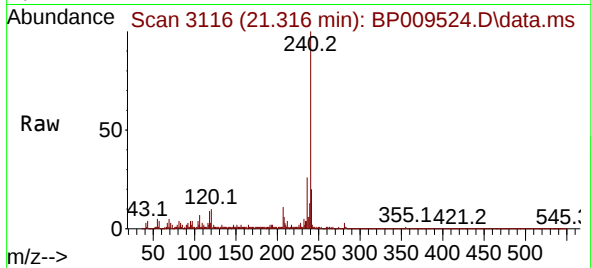

#78
Pyrene
Concen: 2.532 ng
RT: 19.574 min Scan# 2820
Delta R.T. 0.000 min
Lab File: BP009524.D
Acq: 24 Mar 2022 01:22

Tgt Ion:202 Resp: 301110
Ion Ratio Lower Upper
202 100
200 20.4 16.8 25.2
203 19.9 14.2 21.4


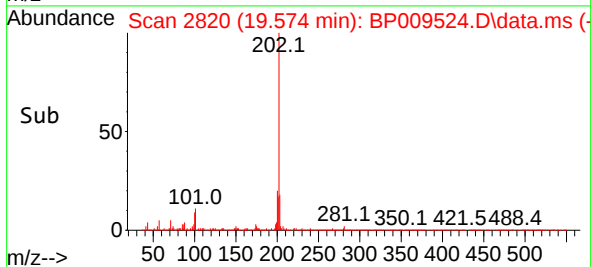
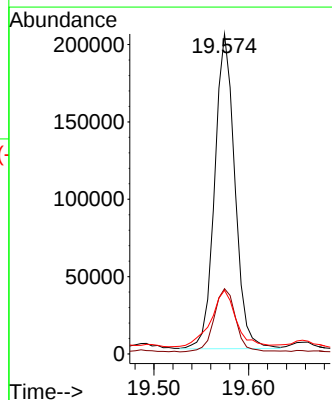
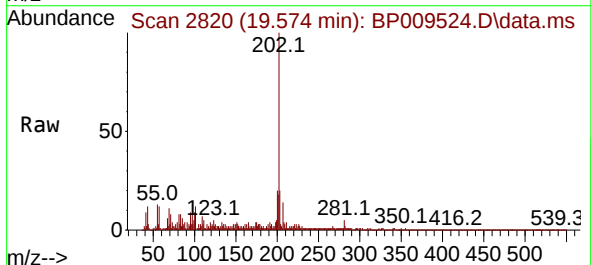


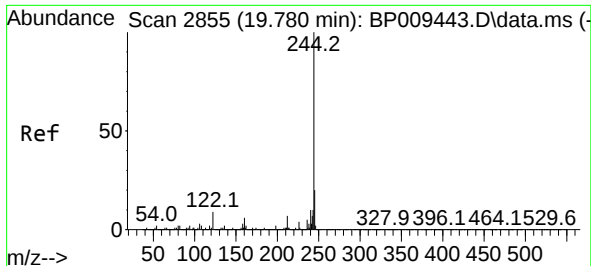

#79
 Terphenyl-d14
 Concen: 6.767 ng
 RT: 19.774 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP009524.D
 Acq: 24 Mar 2022 01:22

Instrument :
 BNA_P
 ClientSampleId :
 PILE

Tgt Ion:244 Resp: 680431
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 9.7 8.3 12.5

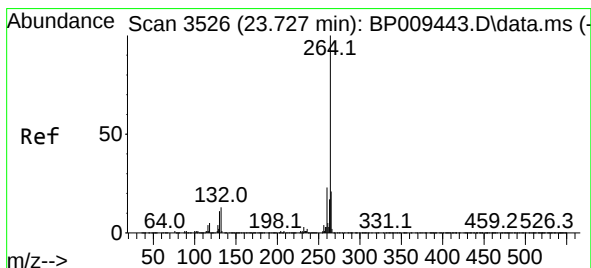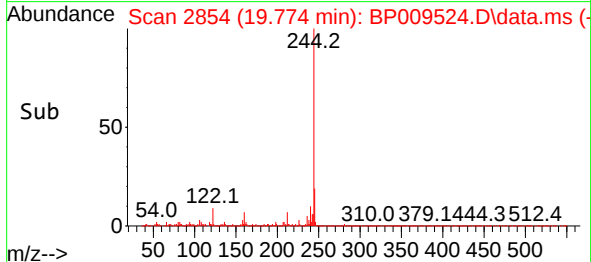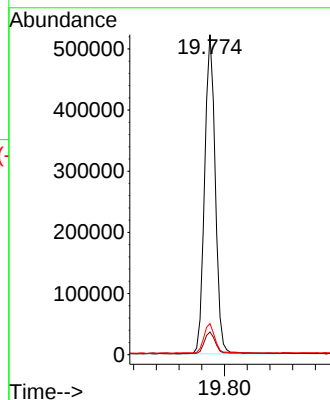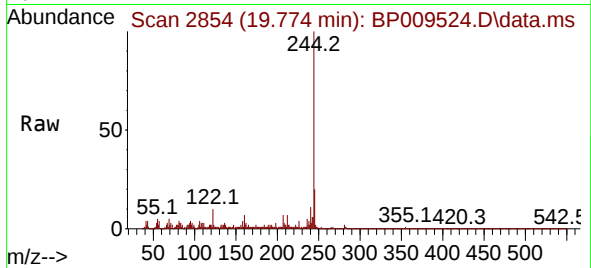

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.721 min Scan# 3525
 Delta R.T. 0.006 min
 Lab File: BP009524.D
 Acq: 24 Mar 2022 01:22

Tgt Ion:264 Resp: 1904069
 Ion Ratio Lower Upper
 264 100
 260 24.6 19.4 29.0
 265 22.5 17.2 25.8

