

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032322\  
 Data File : BP009502.D  
 Acq On : 23 Mar 2022 12:08  
 Operator : CG/JU  
 Sample : PB143208BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB143208BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009502.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.399       | 403           | 410         | 436          | rBV      | 8257645        | 14003800      | 49.19%          | 10.188%       |
| 2         | 6.981       | 671           | 679         | 707          | rBV      | 7595178        | 14235329      | 50.01%          | 10.356%       |
| 3         | 7.793       | 808           | 817         | 828          | rBV      | 1642062        | 2953993       | 10.38%          | 2.149%        |
| 4         | 8.952       | 1005          | 1014        | 1038         | rBV      | 4990654        | 9533614       | 33.49%          | 6.936%        |
| 5         | 10.587      | 1282          | 1292        | 1314         | rBV      | 1967717        | 4140416       | 14.54%          | 3.012%        |
| 6         | 13.057      | 1703          | 1712        | 1746         | rBV      | 14157973       | 23634440      | 83.02%          | 17.194%       |
| 7         | 14.434      | 1937          | 1946        | 1965         | rBV      | 3255594        | 5738202       | 20.16%          | 4.175%        |
| 8         | 15.934      | 2192          | 2201        | 2234         | rBV      | 10376640       | 17864279      | 62.75%          | 12.996%       |
| 9         | 17.198      | 2408          | 2416        | 2433         | rBV      | 3715554        | 6468114       | 22.72%          | 4.706%        |
| 10        | 19.780      | 2848          | 2855        | 2870         | rBV      | 21111642       | 28467329      | 100.00%         | 20.710%       |
| 11        | 21.316      | 3111          | 3116        | 3130         | rBV      | 3531371        | 5451312       | 19.15%          | 3.966%        |
| 12        | 23.715      | 3518          | 3524        | 3539         | rVB2     | 2049678        | 4965104       | 17.44%          | 3.612%        |




Sum of corrected areas: 137455932

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032322\  
Data File : BP009502.D  
Acq On : 23 Mar 2022 12:08  
Operator : CG/JU  
Sample : PB143208BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

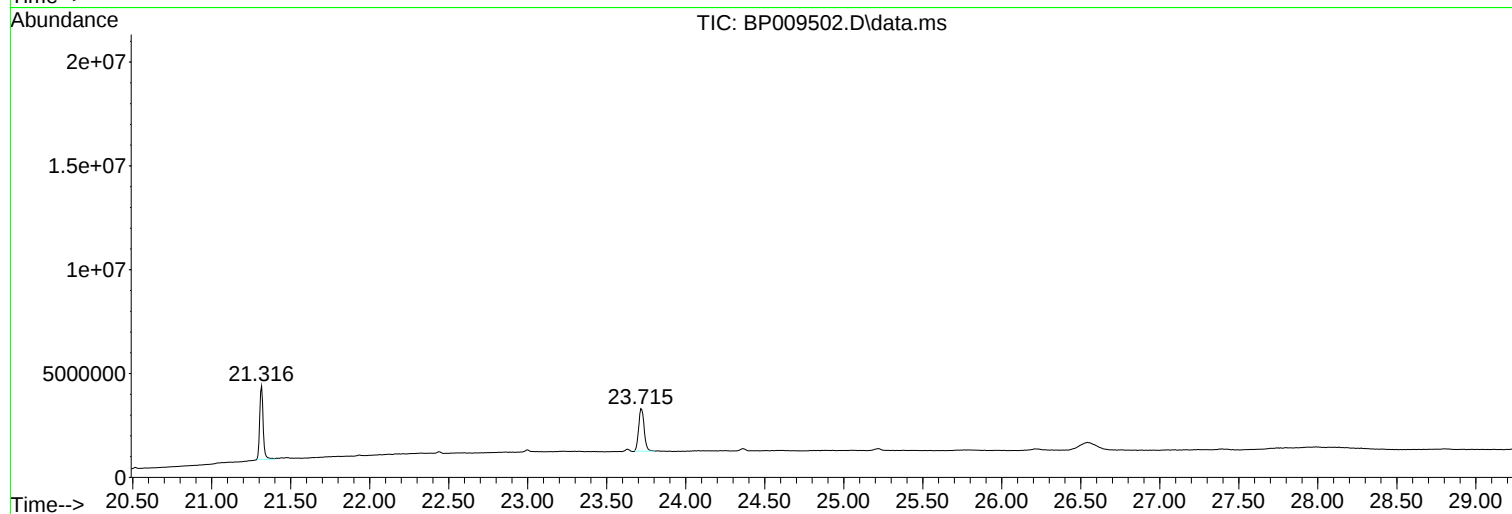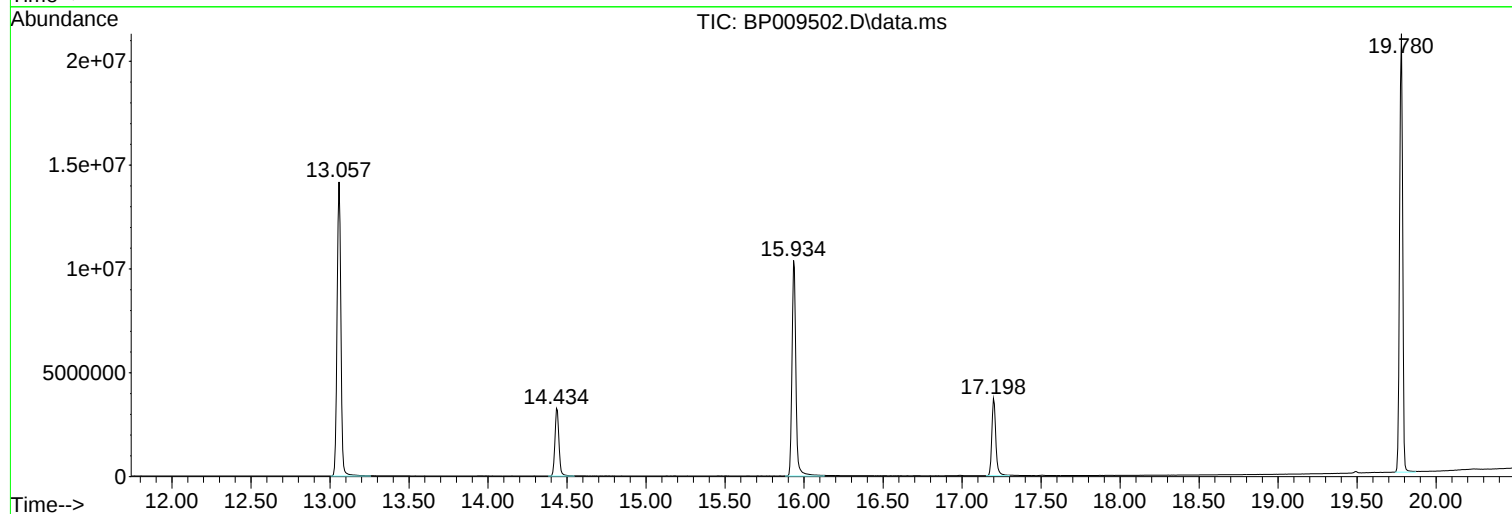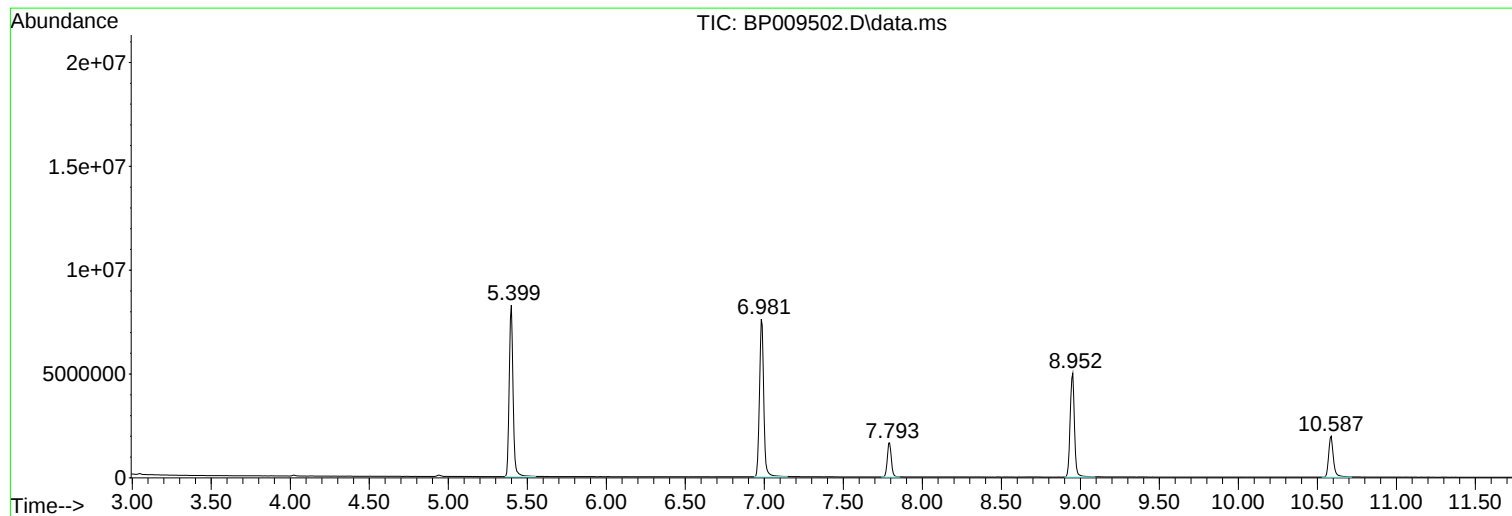

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032322\  
Data File : BP009502.D  
Acq On : 23 Mar 2022 12:08  
Operator : CG/JU  
Sample : PB143208BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP032322\  
Data File : BP009502.D  
Acq On : 23 Mar 2022 12:08  
Operator : CG/JU  
Sample : PB143208BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP031722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|