

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009505.D
 Acq On : 23 Mar 2022 13:49
 Operator : CG/JU
 Sample : PB143209BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143209BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	403	409	439	rBV	6103461	10760118	50.04%	10.595%
2	6.981	671	679	715	rBV	5725508	10763338	50.05%	10.598%
3	7.793	809	817	832	rBV	1256933	2245487	10.44%	2.211%
4	8.946	1005	1013	1048	rBV	3737062	7142656	33.21%	7.033%
5	10.587	1283	1292	1316	rBV	1397261	3027180	14.08%	2.981%
6	13.057	1703	1712	1737	rBV	9835658	16957792	78.85%	16.697%
7	14.434	1939	1946	1967	rBV	2192902	3990624	18.56%	3.929%
8	15.933	2191	2201	2232	rBV	6931773	12076232	56.16%	11.890%
9	17.198	2409	2416	2434	rBV	2531198	4492104	20.89%	4.423%
10	19.780	2848	2855	2868	rBV	15499019	21505113	100.00%	21.174%
11	21.316	3111	3116	3128	rBV	2772845	4348005	20.22%	4.281%
12	23.721	3518	3525	3541	rVB2	1802902	4253534	19.78%	4.188%




Sum of corrected areas: 101562183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009505.D
Acq On : 23 Mar 2022 13:49
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

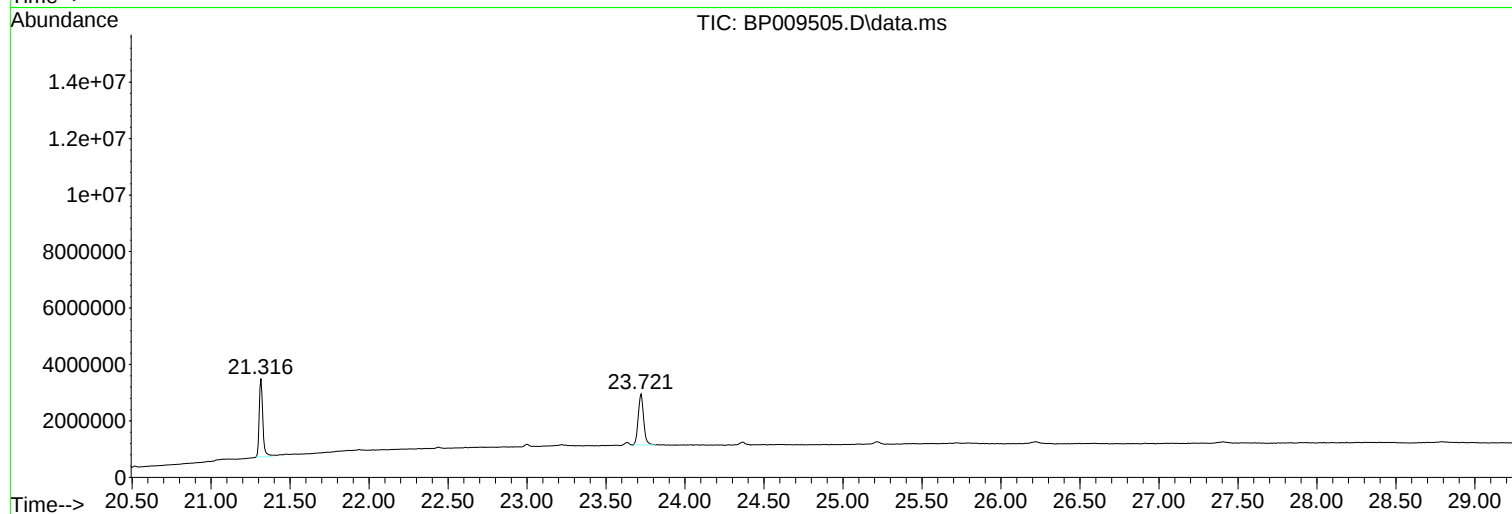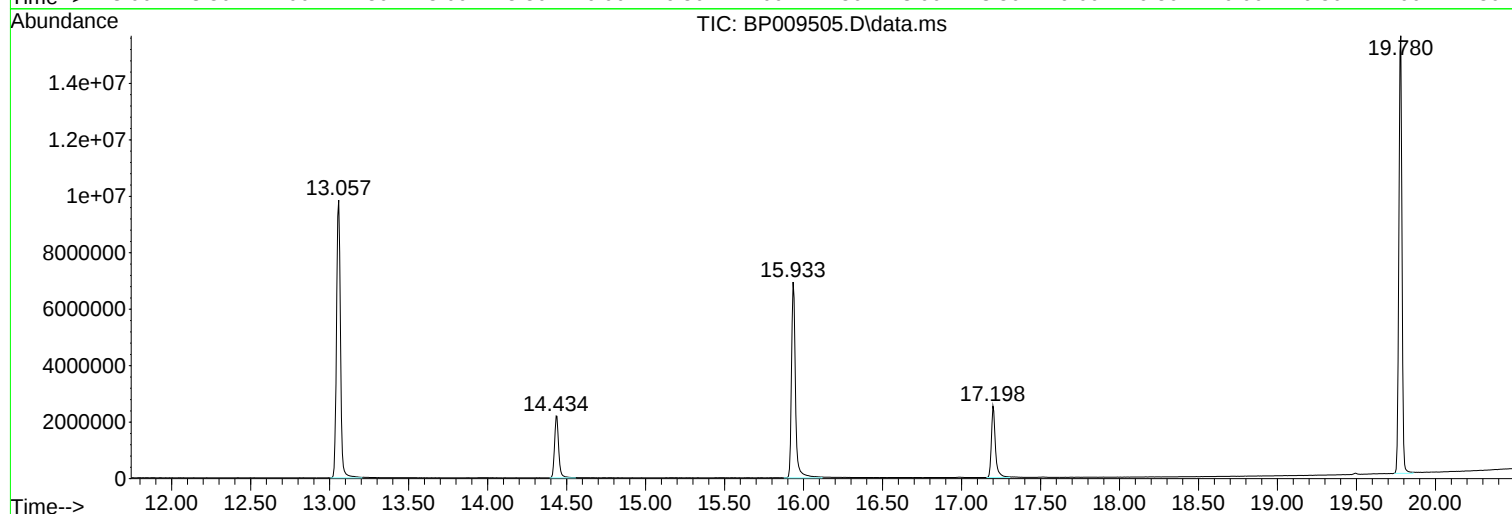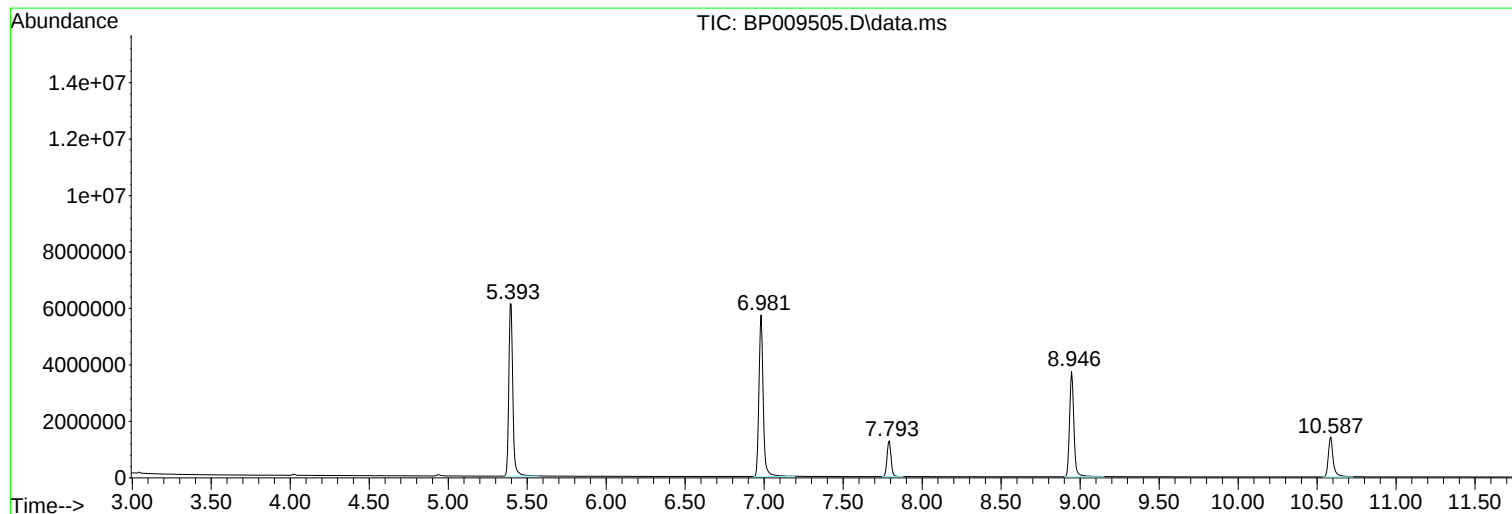

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009505.D
Acq On : 23 Mar 2022 13:49
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009505.D
Acq On : 23 Mar 2022 13:49
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------