

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009522.D
 Acq On : 24 Mar 2022 00:15
 Operator : CG/JU
 Sample : N2031-02 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CMP-B1-031822-0-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	14	rVB	153554	194446	3.83%	0.491%
2	4.017	172	175	183	rVB	31374	54092	1.07%	0.136%
3	5.393	403	409	424	rBV	1029181	1827005	36.02%	4.609%
4	6.975	669	678	701	rBV	890420	1964674	38.73%	4.957%
5	7.787	808	816	829	rBV	1725139	3051532	60.16%	7.699%
6	8.946	1006	1013	1037	rBV	562522	1237556	24.40%	3.122%
7	10.581	1281	1291	1311	rBV	2165379	4201671	82.83%	10.600%
8	13.051	1704	1711	1727	rBV	1647930	2905266	57.27%	7.330%
9	13.269	1743	1748	1755	rVB	33612	54014	1.06%	0.136%
10	14.434	1938	1946	1954	rBV	2891804	4792112	94.47%	12.090%
11	15.934	2195	2201	2222	rBV	782148	1491350	29.40%	3.763%
12	16.169	2238	2241	2244	rBV2	44730	64543	1.27%	0.163%
13	17.198	2409	2416	2421	rBV	2731251	4364032	86.03%	11.010%
14	19.222	2756	2760	2765	rBV	310960	448726	8.85%	1.132%
15	19.569	2817	2819	2823	rVB	203421	239097	4.71%	0.603%
16	19.775	2849	2854	2861	rVB	2015729	2723709	53.69%	6.872%
17	21.310	3110	3115	3120	rBV	3469476	5072611	100.00%	12.798%
18	23.716	3519	3524	3532	rVB2	2294489	4950125	97.59%	12.489%




Sum of corrected areas: 39636561

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009522.D
Acq On : 24 Mar 2022 00:15
Operator : CG/JU
Sample : N2031-02 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

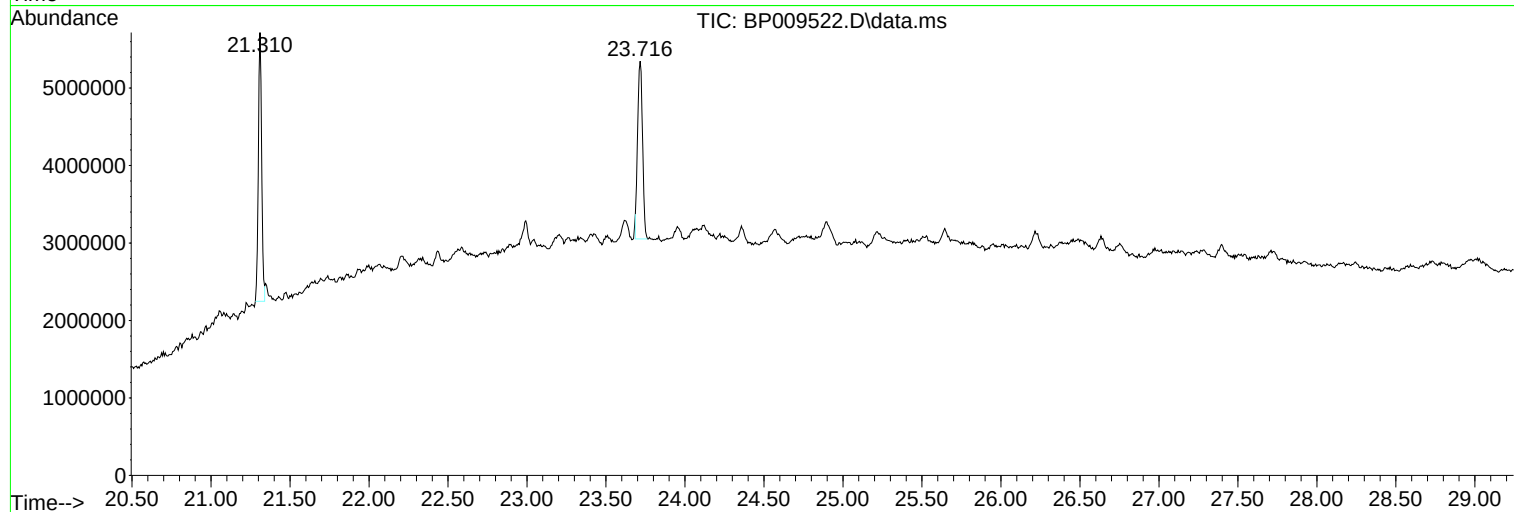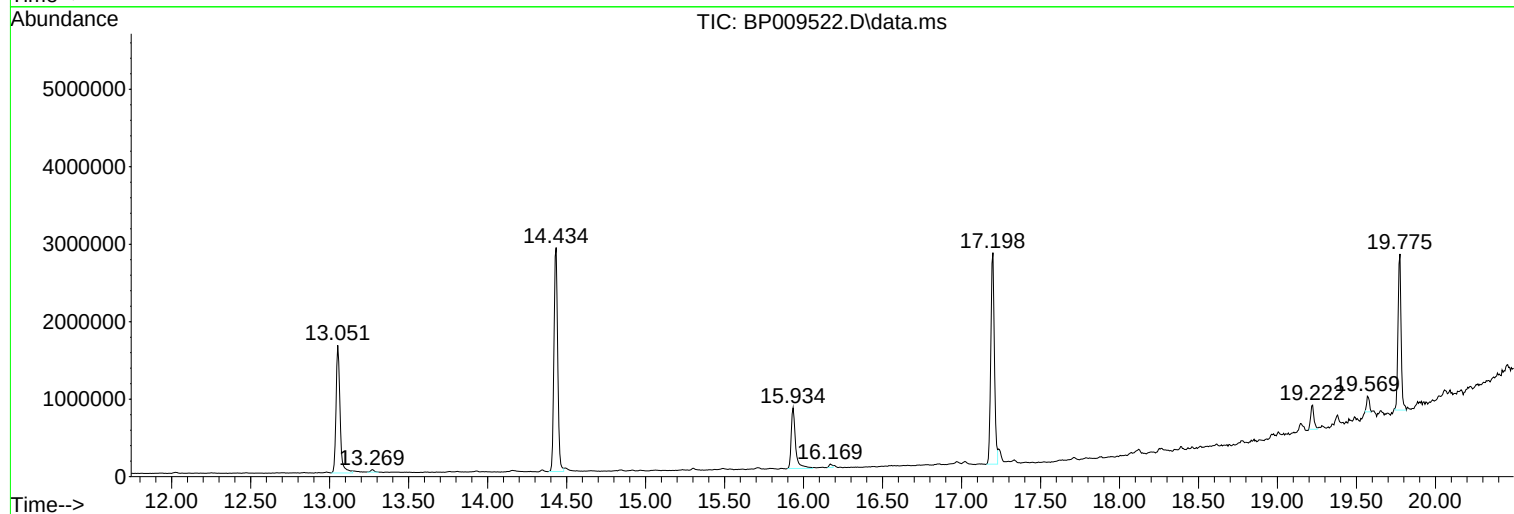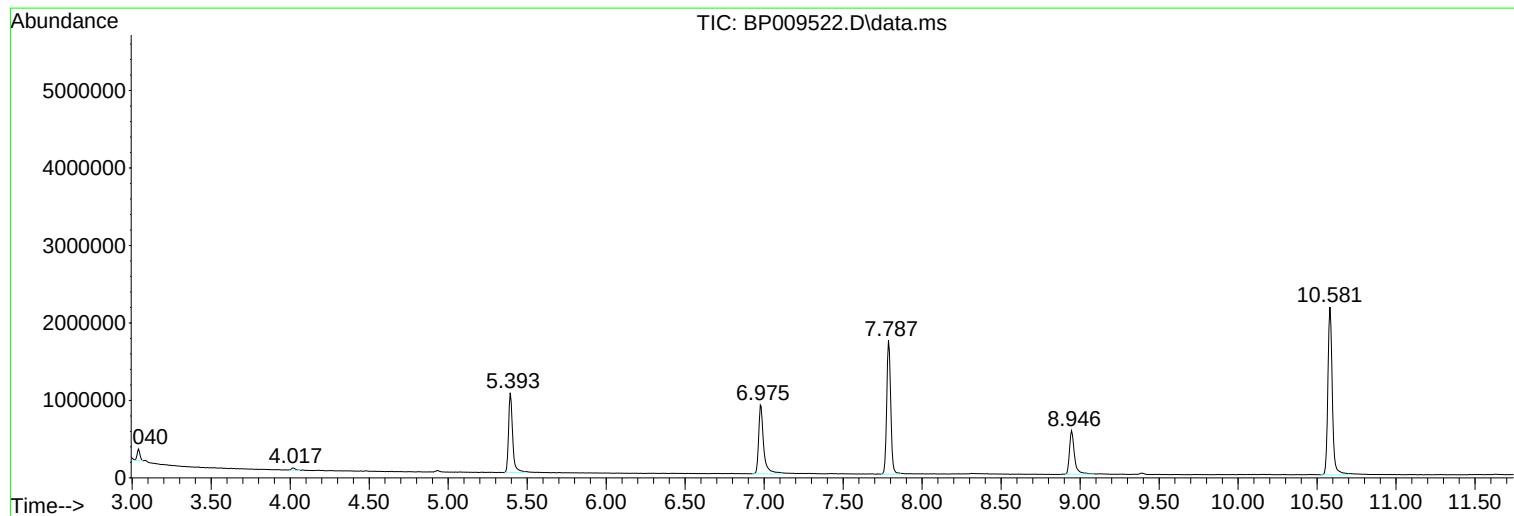

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009522.D
Acq On : 24 Mar 2022 00:15
Operator : CG/JU
Sample : N2031-02 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009522.D
Acq On : 24 Mar 2022 00:15
Operator : CG/JU
Sample : N2031-02 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------