

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009523.D
 Acq On : 24 Mar 2022 00:49
 Operator : CG/JU
 Sample : N2031-06 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CMP-B1-031822-0-2-BD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	5	9	13	rVB	133912	176984	3.28%	0.410%
2	5.393	403	409	429	rBV	1209195	2176059	40.27%	5.037%
3	6.975	671	678	695	rBV	1055293	2240594	41.47%	5.187%
4	7.787	809	816	833	rBV	1781935	3192913	59.09%	7.391%
5	8.946	1004	1013	1035	rBV	684835	1499110	27.75%	3.470%
6	10.581	1280	1291	1317	rBV	2289927	4500348	83.29%	10.418%
7	13.051	1704	1711	1728	rBV	2009800	3499612	64.77%	8.101%
8	14.434	1938	1946	1963	rBV	3282540	5403027	100.00%	12.508%
9	15.934	2194	2201	2219	rBV	1022875	1934044	35.80%	4.477%
10	16.169	2238	2241	2250	rBV3	40833	89348	1.65%	0.207%
11	17.198	2409	2416	2430	rBV	2957386	4929560	91.24%	11.411%
12	18.110	2567	2571	2577	rBV6	81522	164190	3.04%	0.380%
13	19.775	2849	2854	2859	rBV	2444735	3039992	56.26%	7.037%
14	21.310	3111	3115	3125	rVB	3492168	4974887	92.08%	11.516%
15	23.716	3519	3524	3534	rVB2	2513575	5377593	99.53%	12.449%




Sum of corrected areas: 43198261

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009523.D
Acq On : 24 Mar 2022 00:49
Operator : CG/JU
Sample : N2031-06 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

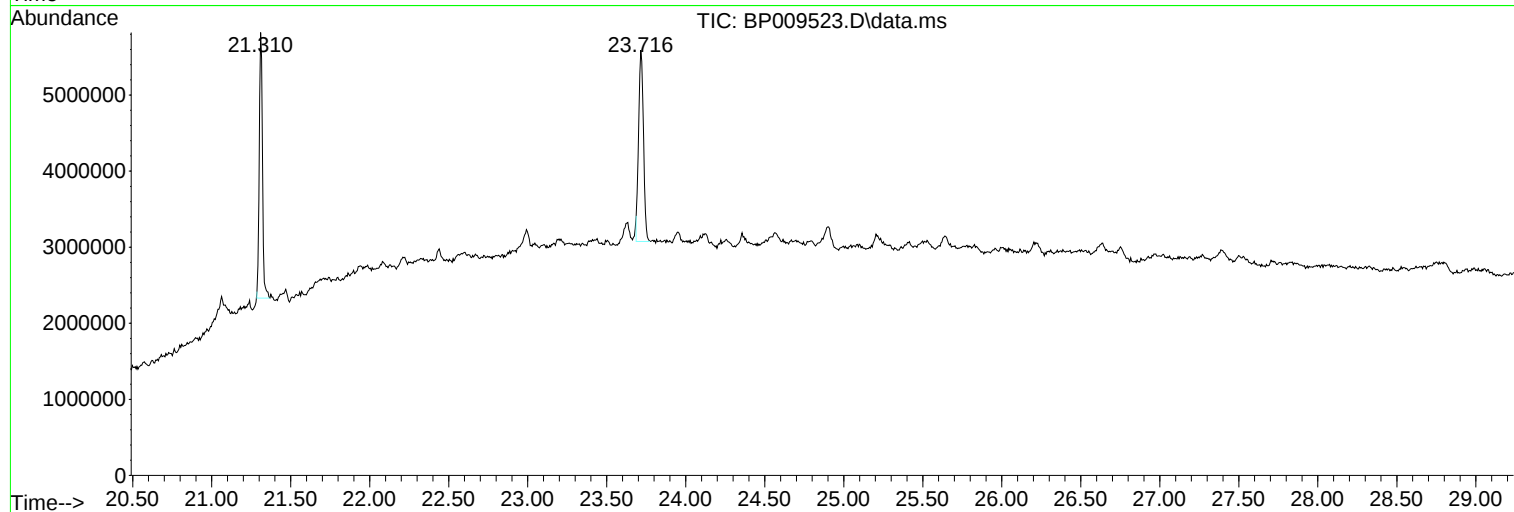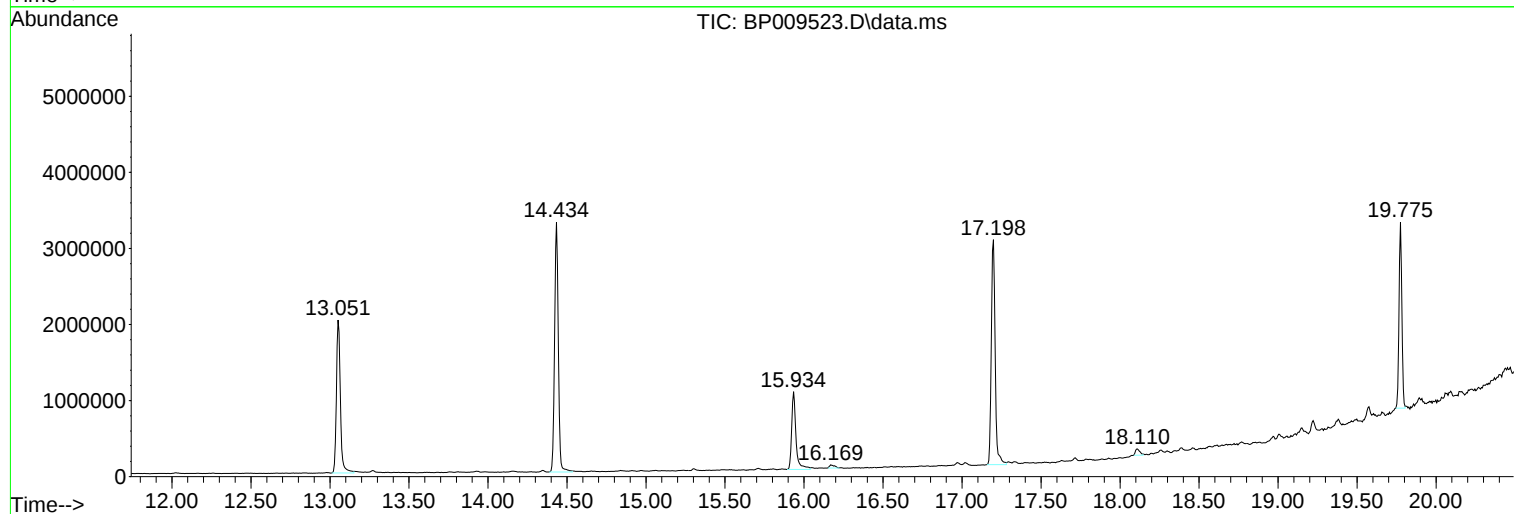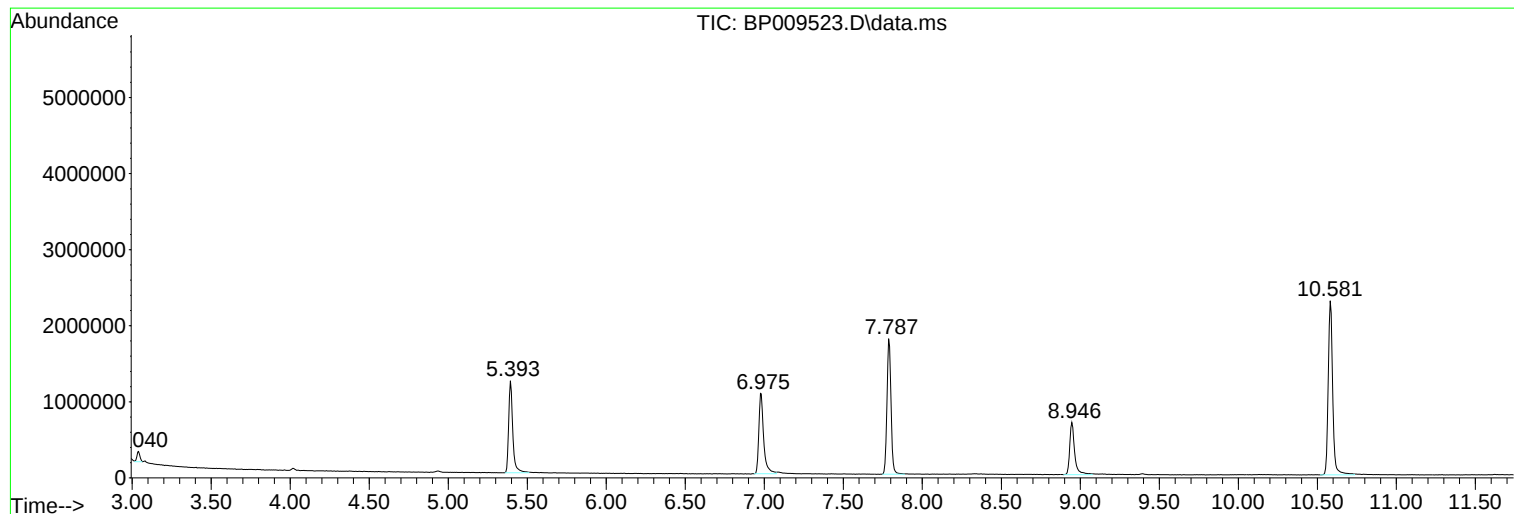

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009523.D
Acq On : 24 Mar 2022 00:49
Operator : CG/JU
Sample : N2031-06 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009523.D
Acq On : 24 Mar 2022 00:49
Operator : CG/JU
Sample : N2031-06 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CMP-B1-031822-0-2-BD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------