

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009524.D
 Acq On : 24 Mar 2022 01:22
 Operator : CG/JU
 Sample : N2071-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FILE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	403	410	425	rBV	335222	714943	11.85%	1.776%
2	6.981	667	679	695	rBV	326218	810228	13.43%	2.012%
3	7.787	809	816	827	rBV	1395148	2495613	41.37%	6.198%
4	8.040	852	859	884	rBV	396553	1433670	23.77%	3.561%
5	8.334	905	909	922	rVB3	38577	91572	1.52%	0.227%
6	8.951	1007	1014	1024	rBV	210140	470679	7.80%	1.169%
7	10.581	1283	1291	1309	rBV	1865908	3653602	60.57%	9.074%
8	13.051	1704	1711	1720	rBV	761356	1309761	21.71%	3.253%
9	13.492	1781	1786	1797	rVB4	30784	74883	1.24%	0.186%
10	13.698	1814	1821	1828	rBV5	129719	284091	4.71%	0.706%
11	13.898	1850	1855	1863	rBV2	113282	200171	3.32%	0.497%
12	14.169	1887	1901	1914	rVB6	94227	316800	5.25%	0.787%
13	14.434	1939	1946	1953	rBV	3140017	5113551	84.77%	12.700%
14	14.492	1953	1956	1966	rVB4	87409	182312	3.02%	0.453%
15	15.381	2103	2107	2111	rBV	61774	94672	1.57%	0.235%
16	15.545	2129	2135	2141	rBV	595953	913556	15.15%	2.269%
17	15.792	2172	2177	2185	rVB2	74689	130789	2.17%	0.325%
18	15.933	2196	2201	2211	rBV2	549855	913478	15.14%	2.269%
19	16.175	2238	2242	2243	rBV3	48712	65045	1.08%	0.162%
20	16.492	2292	2296	2303	rBV	108217	200179	3.32%	0.497%
21	16.610	2312	2316	2324	rBV7	84610	143272	2.38%	0.356%
22	16.851	2354	2357	2360	rBV3	45508	68525	1.14%	0.170%
23	17.139	2403	2406	2409	rBV4	86815	130675	2.17%	0.325%
24	17.198	2409	2416	2421	rVV	3753719	6031933	100.00%	14.981%
25	17.239	2421	2423	2429	rVB	292866	371518	6.16%	0.923%
26	17.333	2435	2439	2442	rBV	108221	134779	2.23%	0.335%
27	17.551	2473	2476	2479	rBV3	56052	68562	1.14%	0.170%
28	17.710	2499	2503	2506	rBV3	192936	323297	5.36%	0.803%
29	17.916	2534	2538	2545	rBV4	197358	330556	5.48%	0.821%
30	18.116	2568	2572	2579	rVB3	146916	237667	3.94%	0.590%
31	19.222	2756	2760	2768	rBV	542237	924324	15.32%	2.296%
32	19.574	2817	2820	2823	rBV	363155	448615	7.44%	1.114%
33	19.774	2850	2854	2858	rBV	1280763	1601876	26.56%	3.978%
34	21.316	3111	3116	3126	rVB	3283279	5337023	88.48%	13.255%
35	23.721	3521	3525	3533	rVB2	2345801	4641958	76.96%	11.529%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009524.D
Acq On : 24 Mar 2022 01:22
Operator : CG/JU
Sample : N2071-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PILE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 40264175

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009524.D
Acq On : 24 Mar 2022 01:22
Operator : CG/JU
Sample : N2071-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PILE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

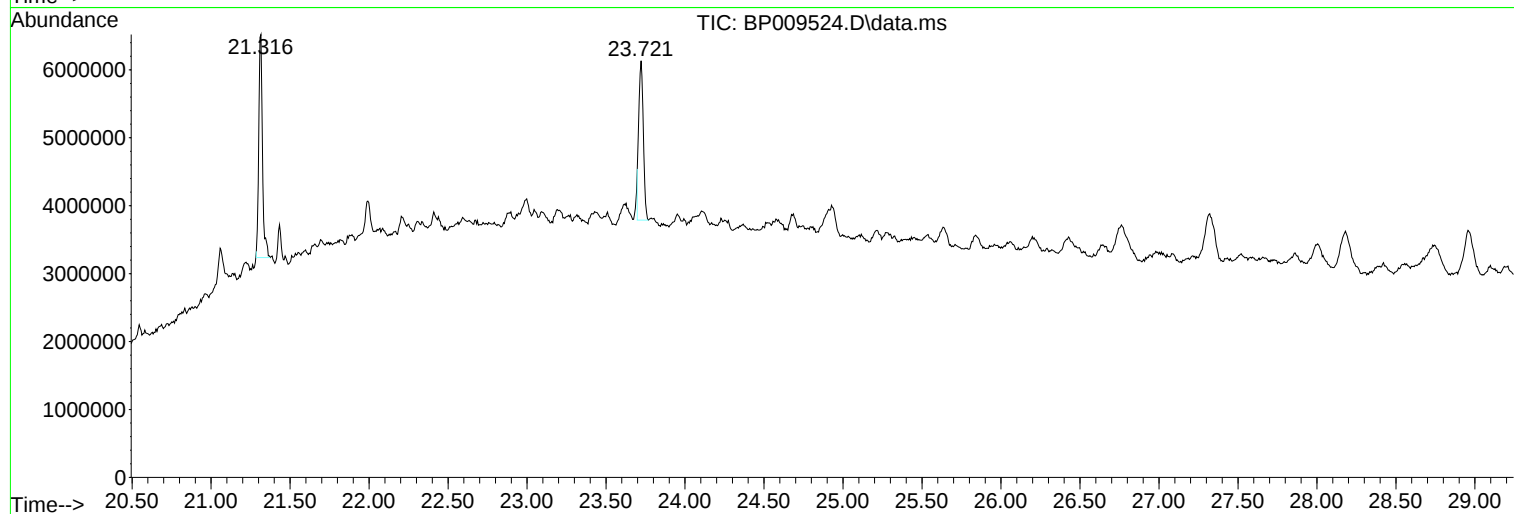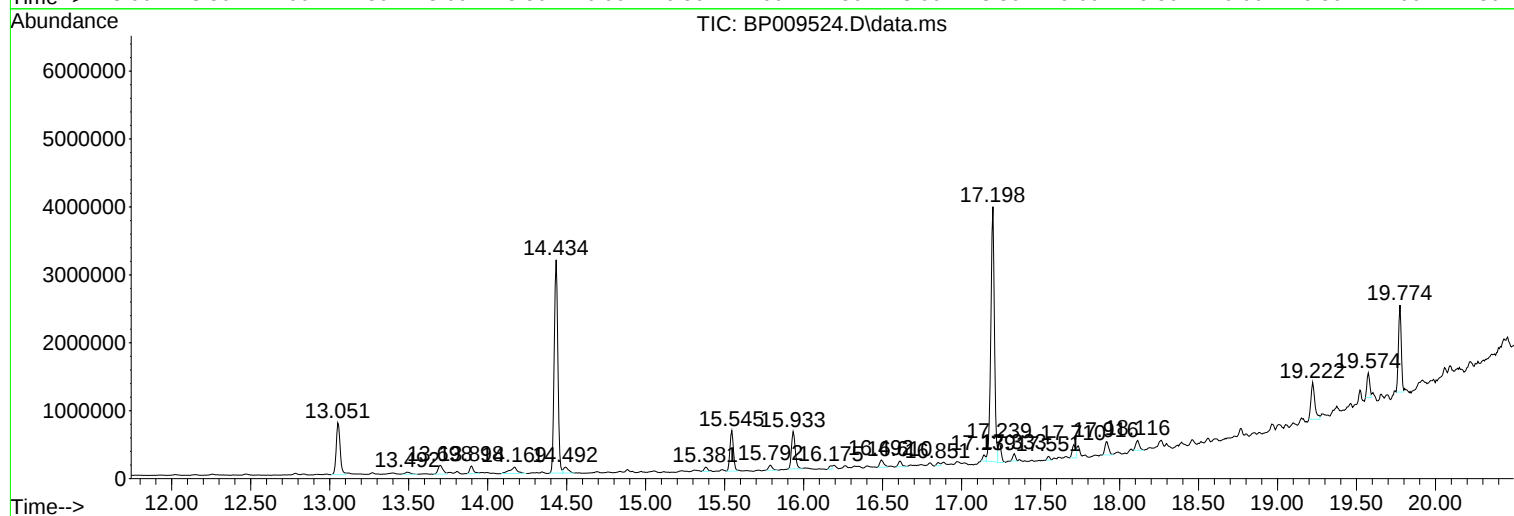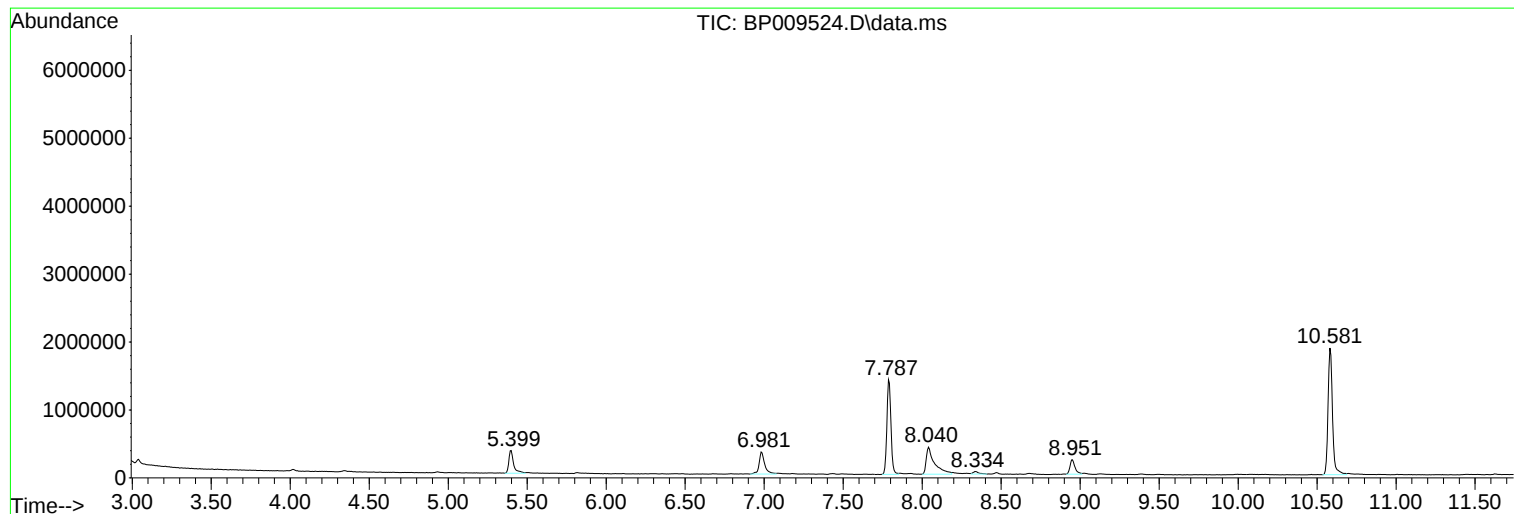

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009524.D
Acq On : 24 Mar 2022 01:22
Operator : CG/JU
Sample : N2071-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PILE










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1H-Cycloprop[e]azulen-4-ol,... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.545	3.57 ng	913556	Acenaphthene-d10	14.434

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Cycloprop[e]azulen-4-ol, deca...	222	C15H26O	000552-02-3	91
2			Azulene, 1,2,3,3a,4,5,6,7-octahy...	204	C15H24	022567-17-5	90
3			Azulene, 1,2,3,5,6,7,8,8a-octahy...	204	C15H24	003691-11-0	83
4			Guaia-9,11-diene	204	C15H24	1000374-19-8	55
5			Naphthalene, decahydro-4a-methyl...	204	C15H24	017066-67-0	50

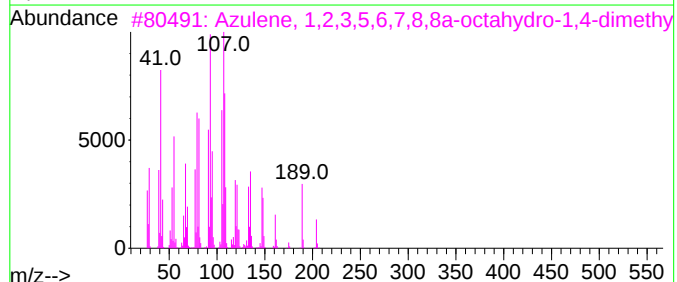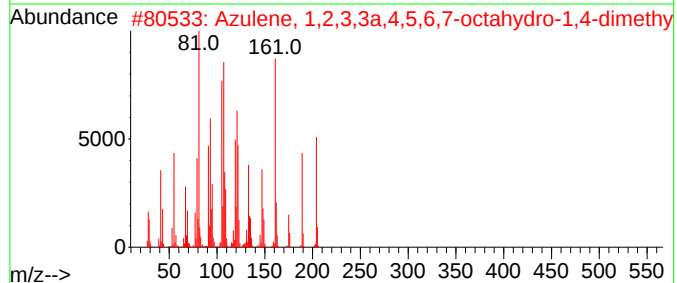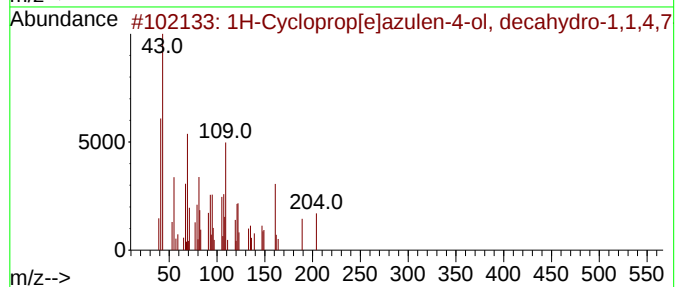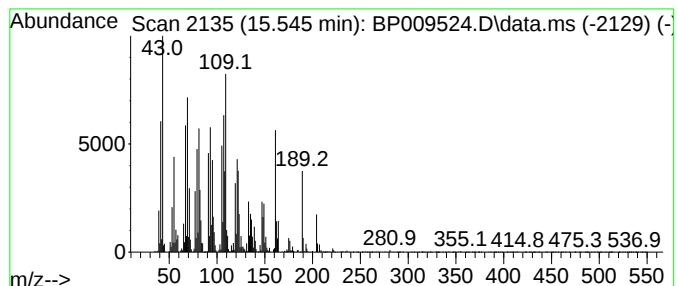

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009524.D
Acq On : 24 Mar 2022 01:22
Operator : CG/JU
Sample : N2071-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PILE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Cycloprop[e]...	15.545	3.6	ng	913556	3	14.434	5113550	20.0