


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009500.D
 Acq On : 23 Mar 2022 10:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 01:19:11 2022

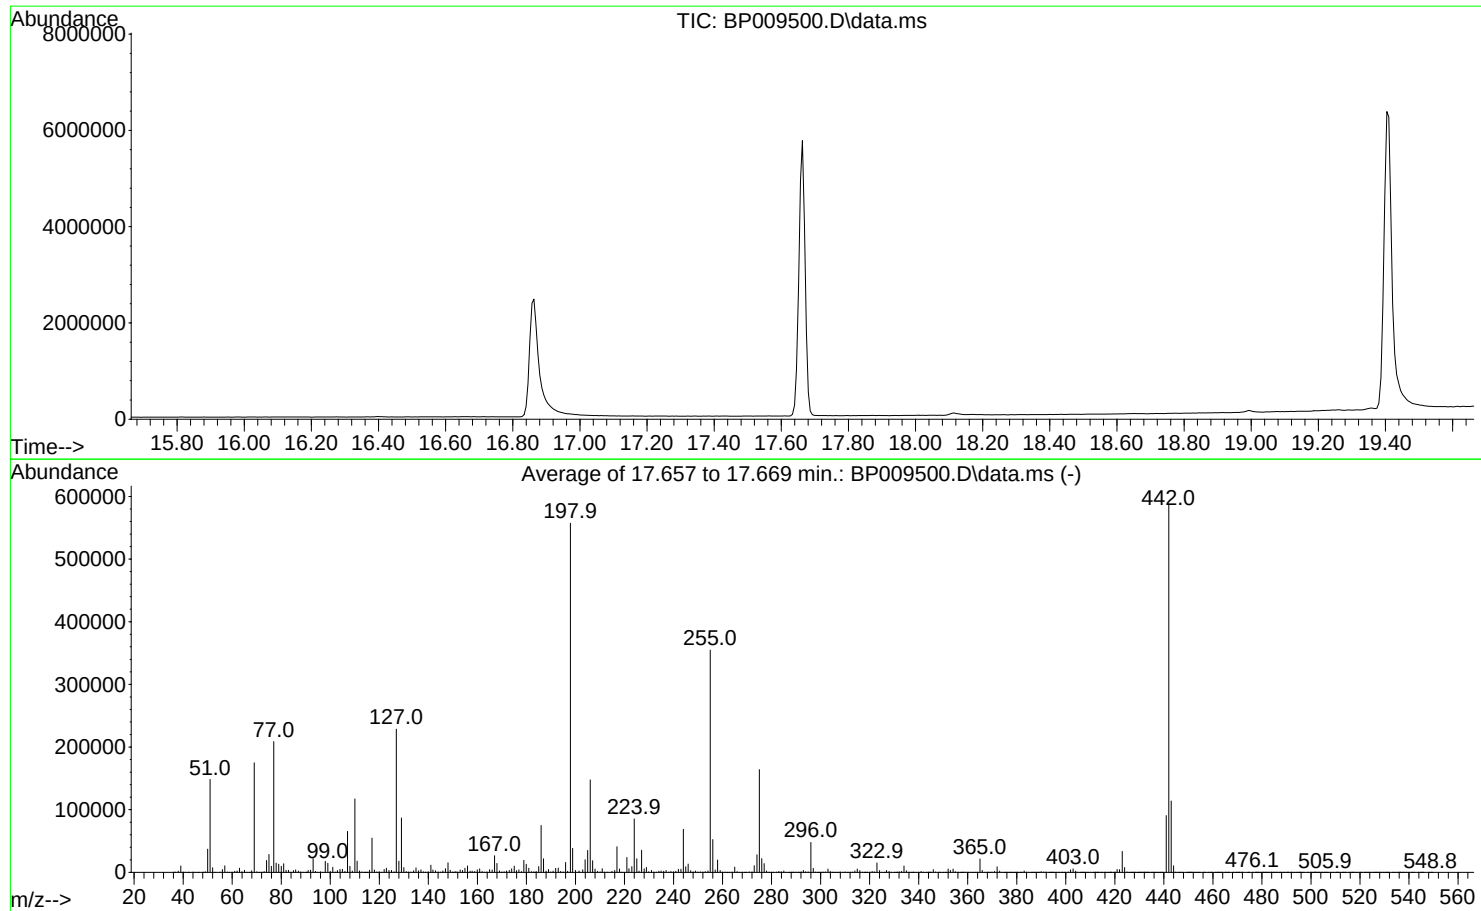




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	148308	PASS
68	69	0.00	2	1.5	2706	PASS
69	198	0.00	100	31.4	175048	PASS
70	69	0.00	2	0.6	1130	PASS
127	198	10	80	41.0	228676	PASS
197	198	0.00	2	0.3	1735	PASS
198	198	100	100	100.0	557291	PASS
199	198	5	9	6.9	38304	PASS
275	198	10	60	29.4	164011	PASS
365	198	1	100	3.9	21504	PASS
441	198	0.01	100	16.3	90610	PASS
442	442	100	100	100.0	587136	PASS
443	442	15	24	19.4	113973	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009500.D
Acq On : 23 Mar 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 23 13:02:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

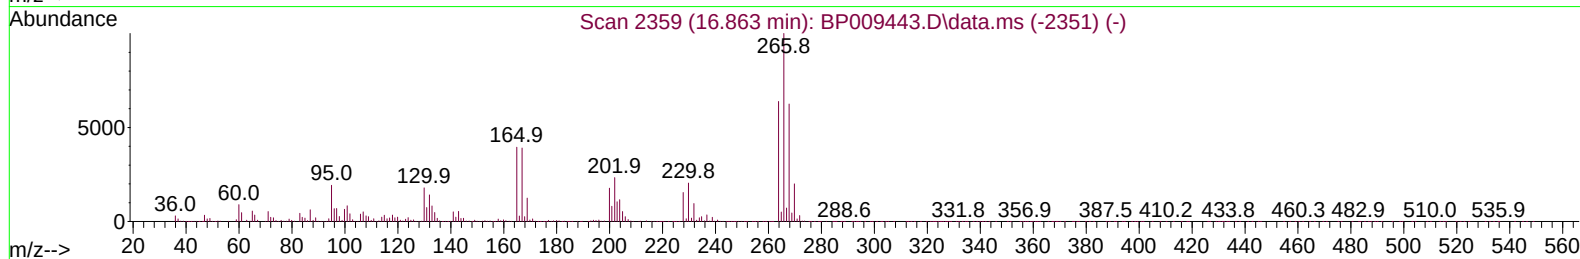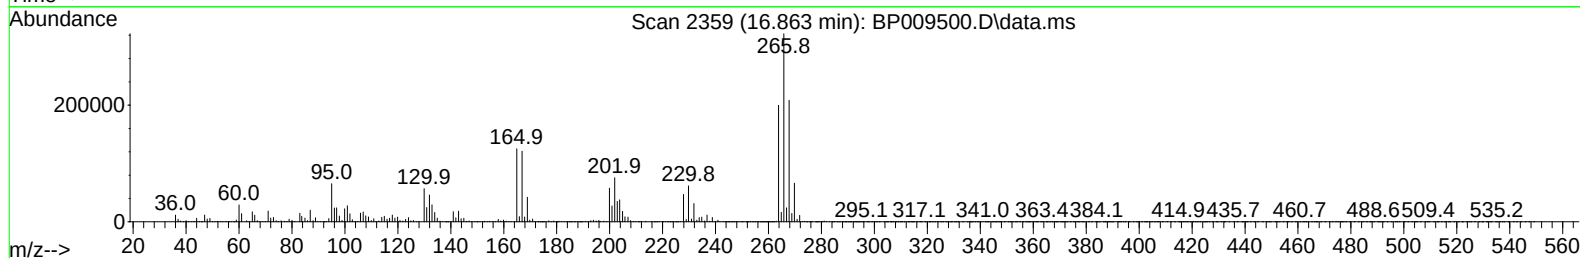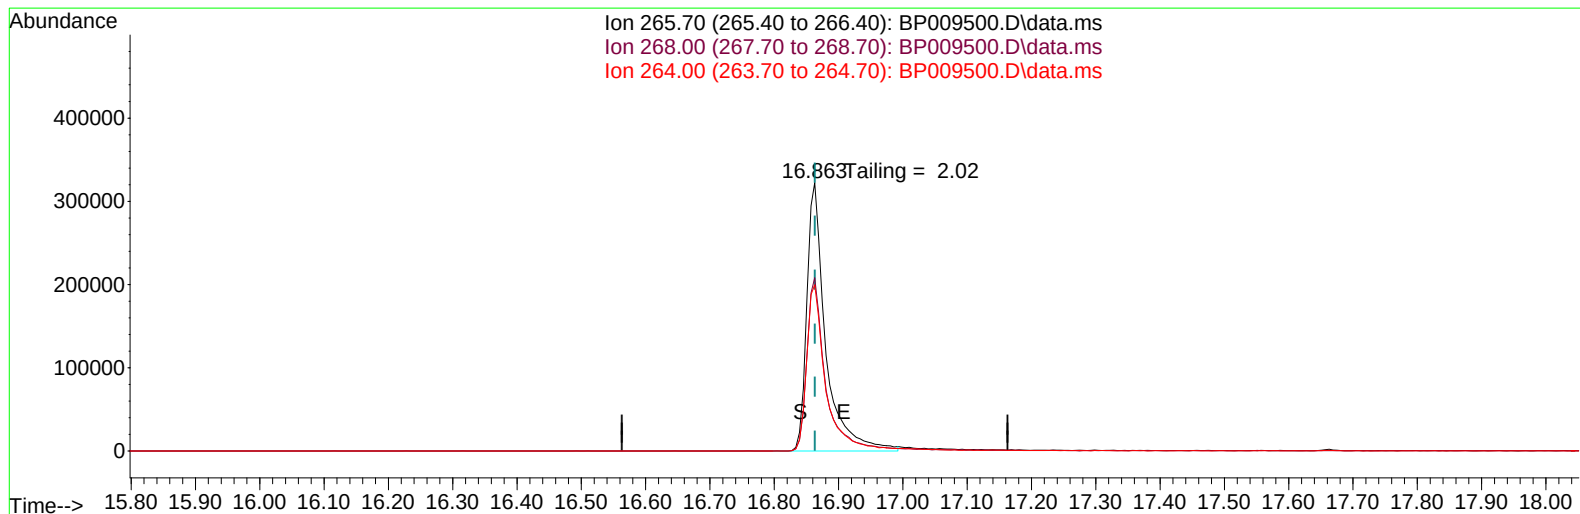

TIC: BP009500.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.000) 611034.74 ng




response 671601

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.60
264.00	63.60	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009500.D
Acq On : 23 Mar 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 23 13:02:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

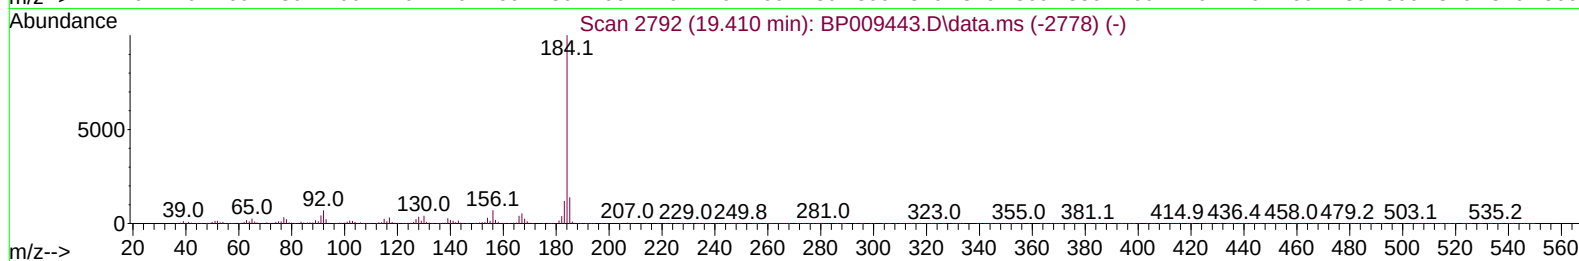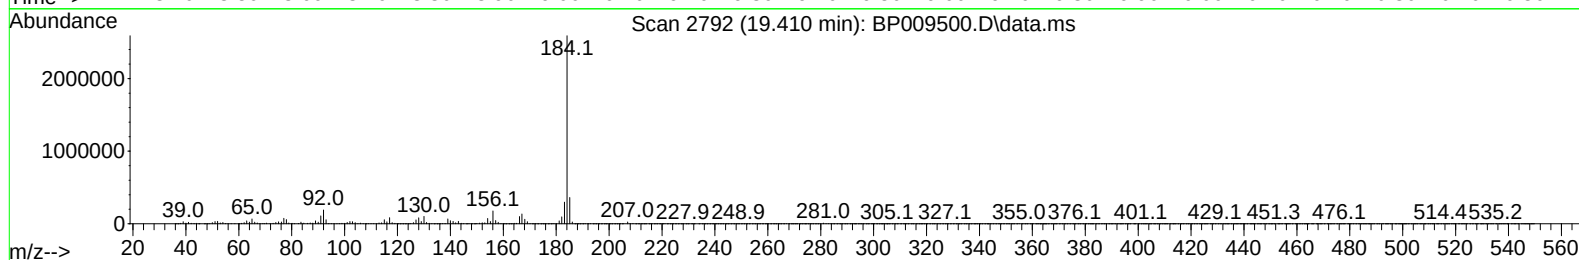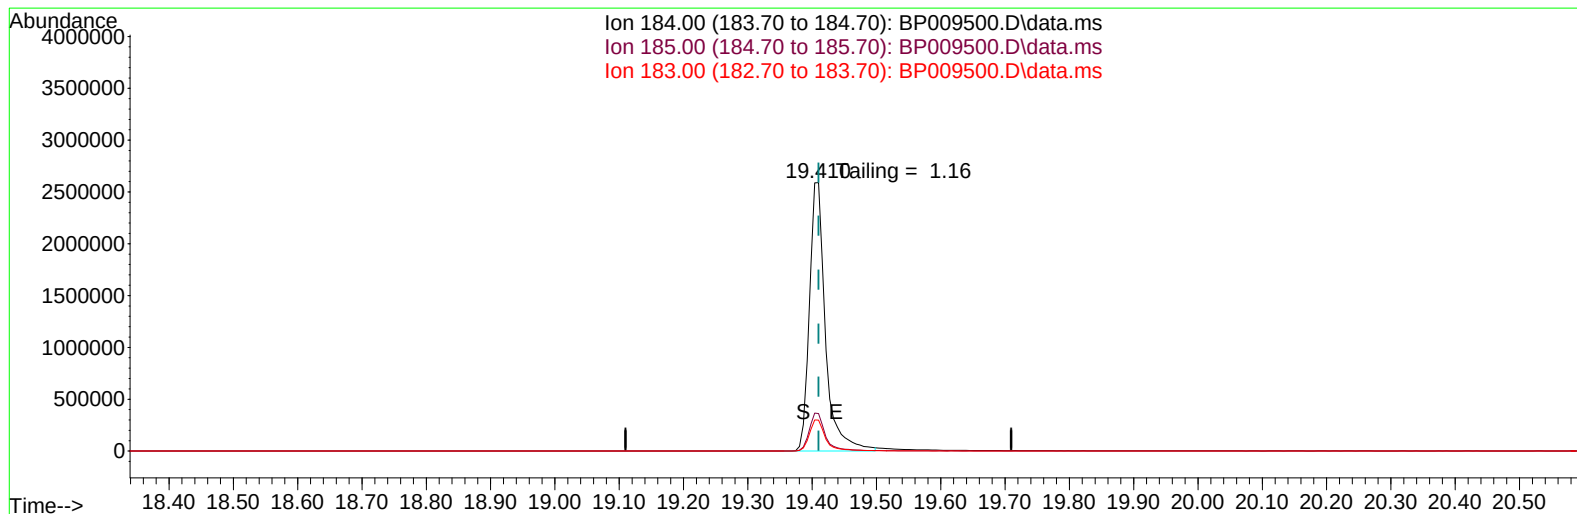

TIC: BP009500.D\data.ms

(77) Benzidine

19.410min (-0.000) 655631.42 ng

response 4596132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	11.70	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2022	BNA_P	<u>BP009500.D</u>
Compound Name	Response	Retention Time
DDT	2019078	20.62
DDD	24257	20.19
DDE	2534	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26791	2045869	1.31

Instrument :
BNA_P
ClientSampleId :
DFTPP