
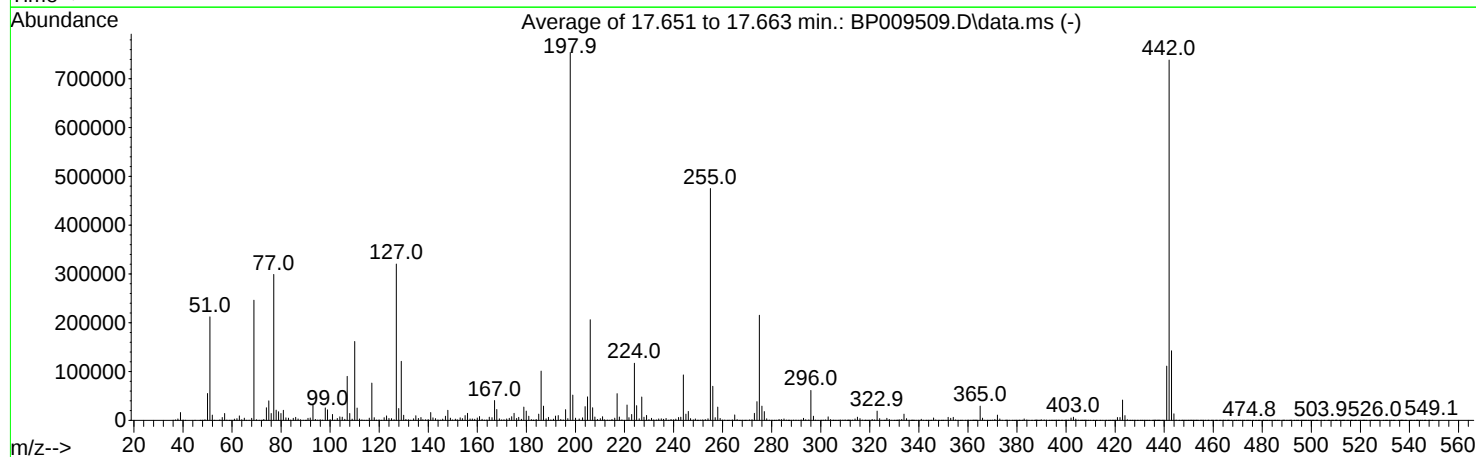


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
 Data File : BP009509.D
 Acq On : 23 Mar 2022 16:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 01:19:11 2022

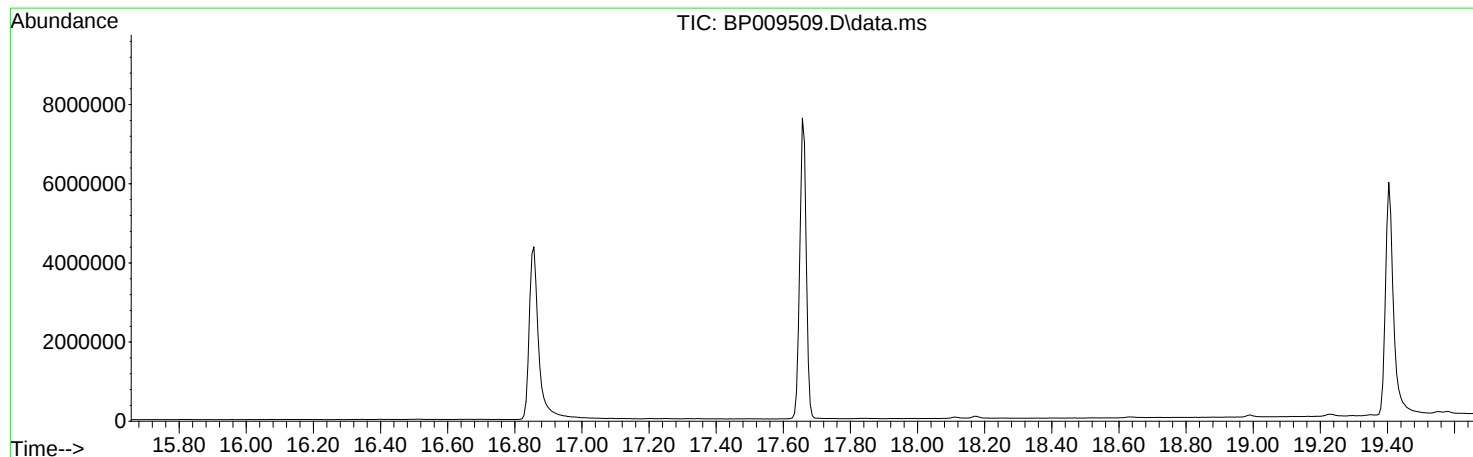




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	212233	PASS
68	69	0.00	2	1.7	4130	PASS
69	198	0.00	100	32.7	246405	PASS
70	69	0.00	2	0.5	1286	PASS
127	198	10	80	42.5	320312	PASS
197	198	0.00	2	0.5	3716	PASS
198	198	100	100	100.0	753964	PASS
199	198	5	9	6.9	51770	PASS
275	198	10	60	28.6	215616	PASS
365	198	1	100	3.9	29104	PASS
441	198	0.01	100	14.8	111309	PASS
442	442	100	100	100.0	738667	PASS
443	442	15	24	19.3	142554	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009509.D
Acq On : 23 Mar 2022 16:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 24 06:07:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 01:19:11 2022
Response via : Initial Calibration

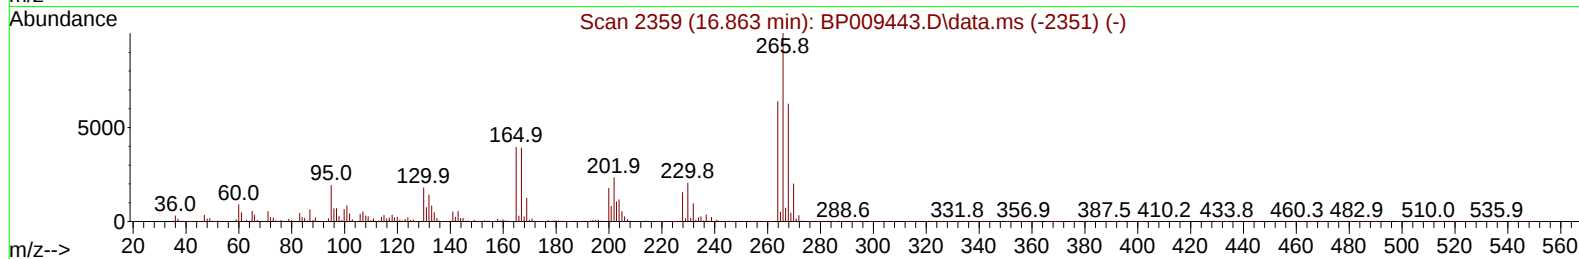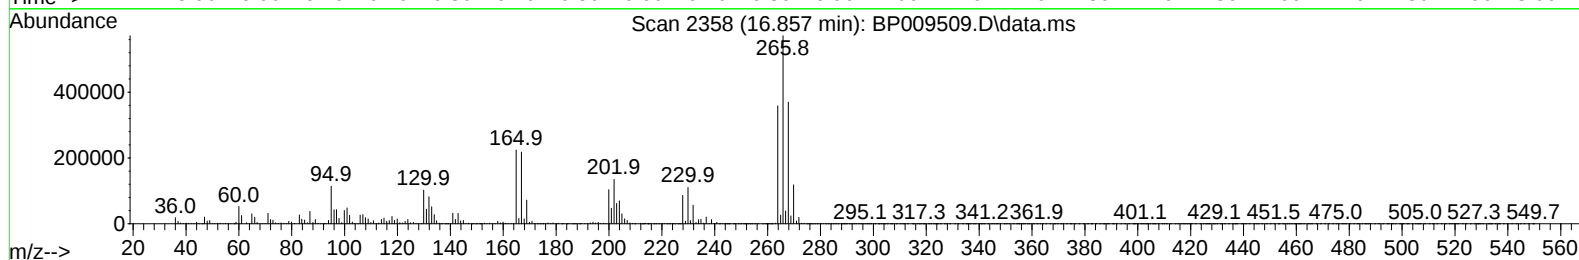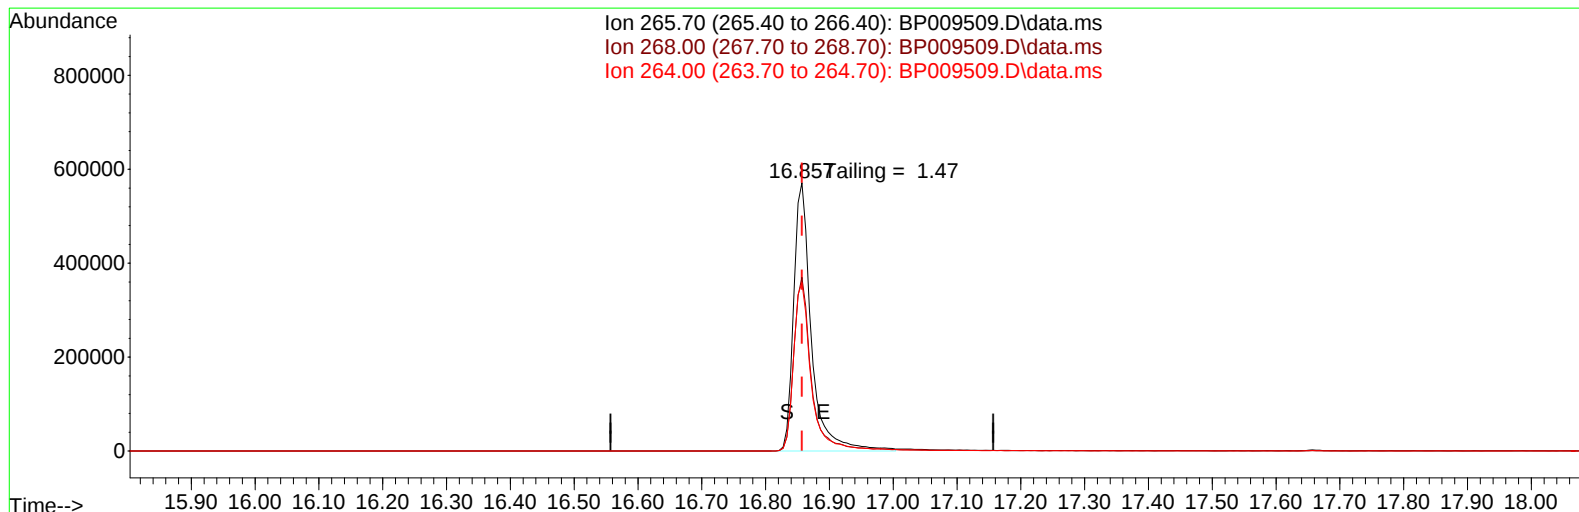

TIC: BP009509.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.000) 20483.74 ng




response 1115682

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.67
264.00	63.60	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032322\
Data File : BP009509.D
Acq On : 23 Mar 2022 16:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 24 06:07:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 01:19:11 2022
Response via : Initial Calibration

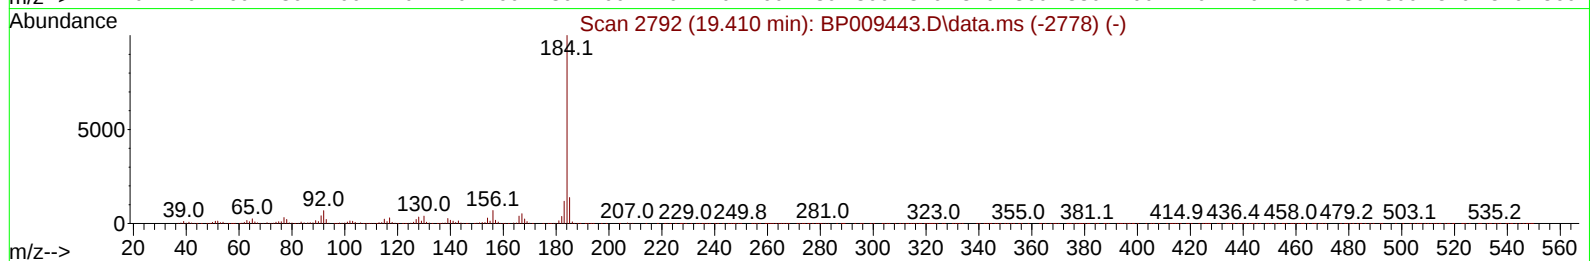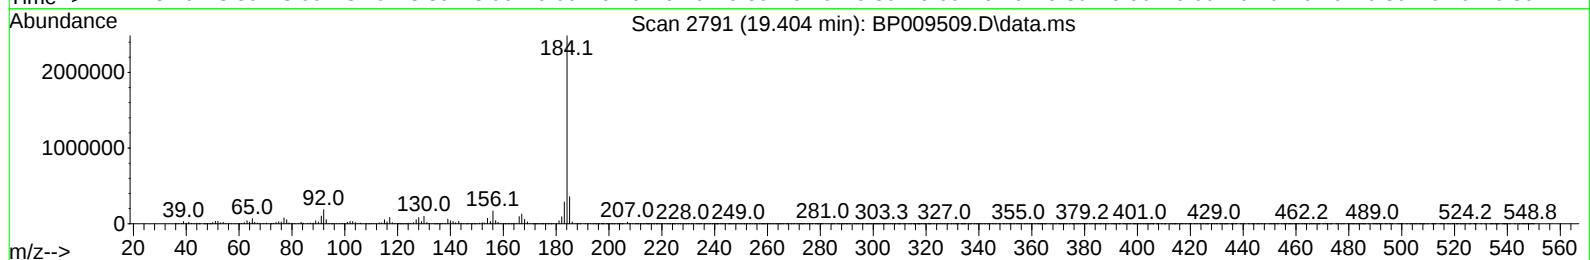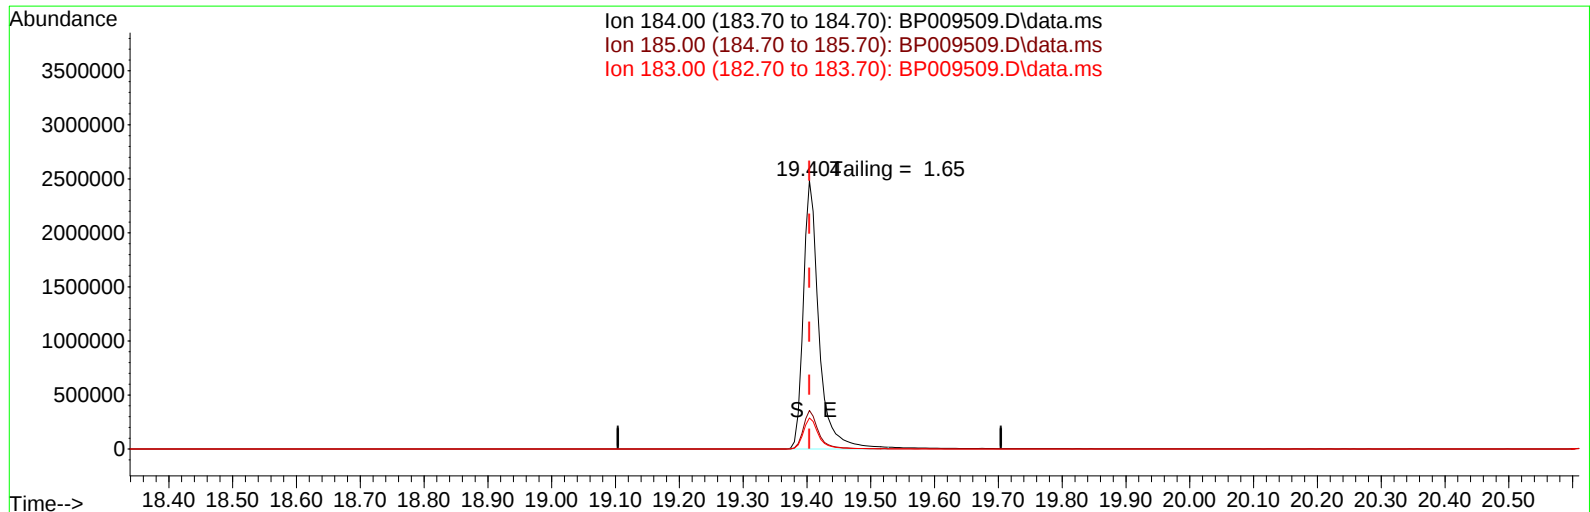

TIC: BP009509.D\data.ms

(77) Benzidine

19.404min (+ 0.000) 1680.34 ng

response 4295068

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.37
183.00	11.70	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2022	BNA_P	<u>BP009509.D</u>
Compound Name	Response	Retention Time
DDT	2364824	20.616
DDD	59912	20.186
DDE	4783	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
64695	2429519	2.66

Instrument :
BNA_P
ClientSampleId :
DFTPP