
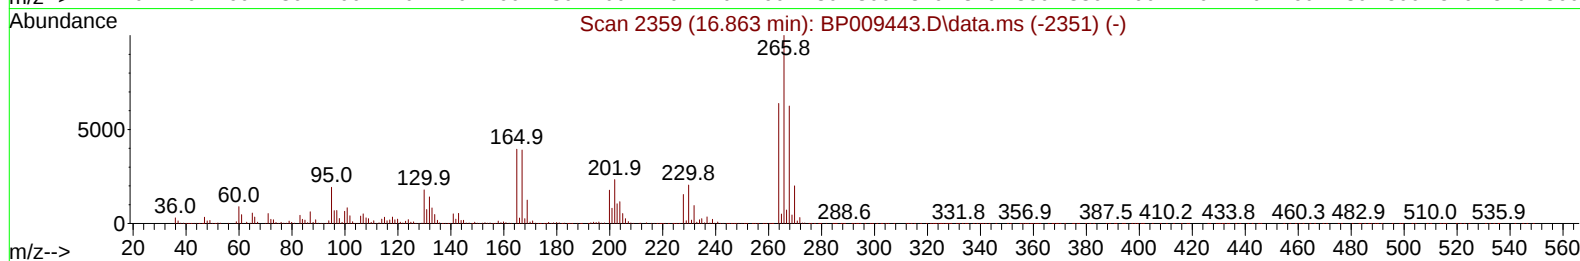
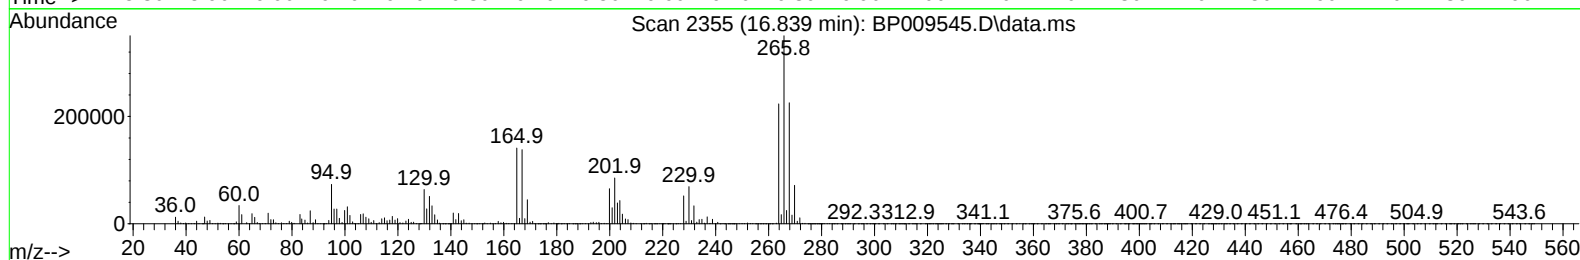


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009545.D
Acq On : 25 Mar 2022 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:49:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration

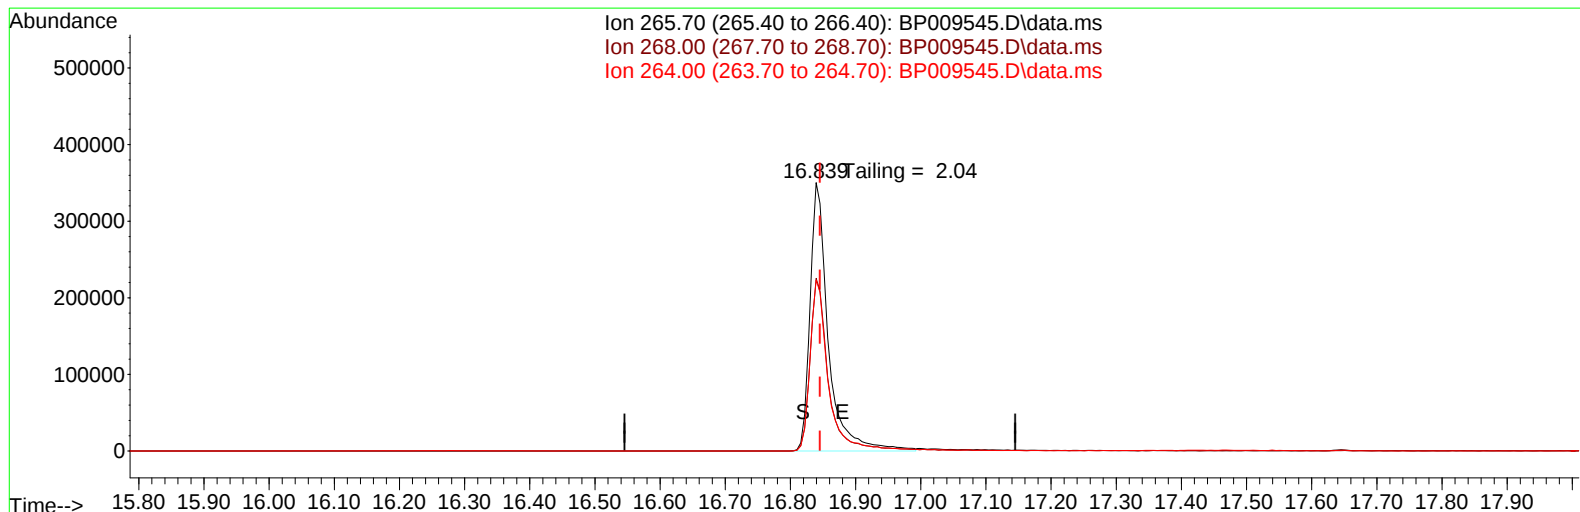

TIC: BP009545.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.006) 712801.89 ng

response 686865

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.33
264.00	63.60	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
 Data File : BP009545.D
 Acq On : 25 Mar 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:49:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

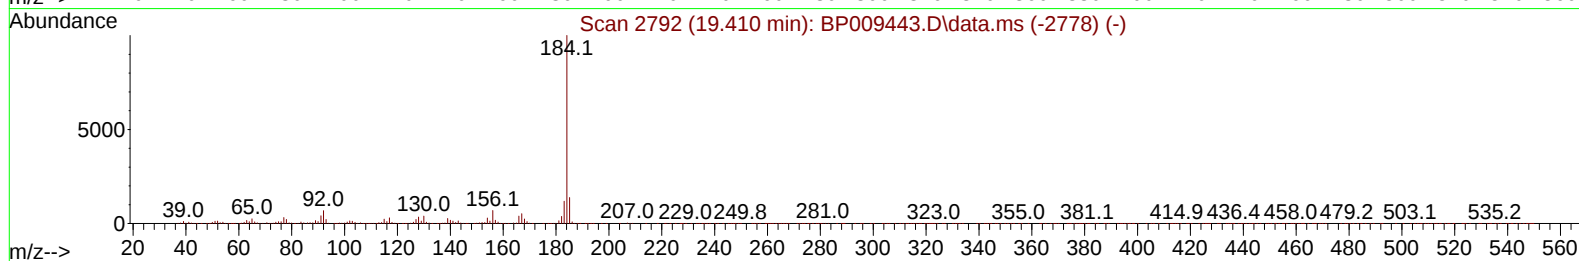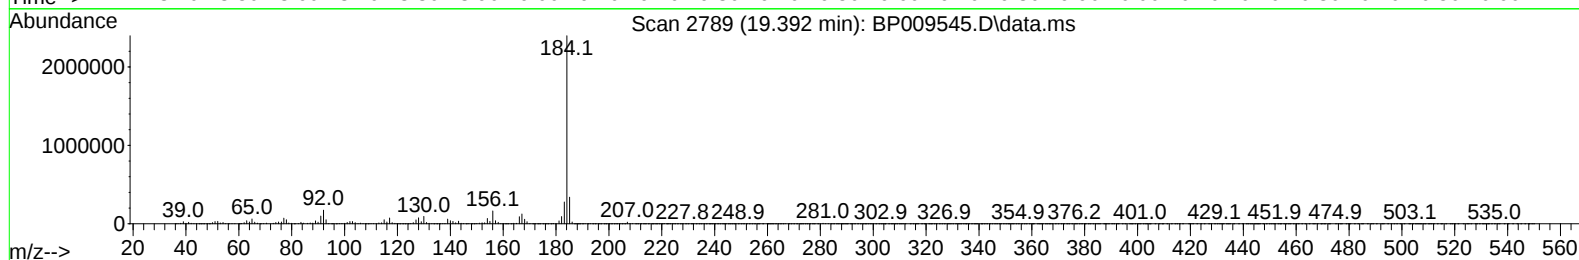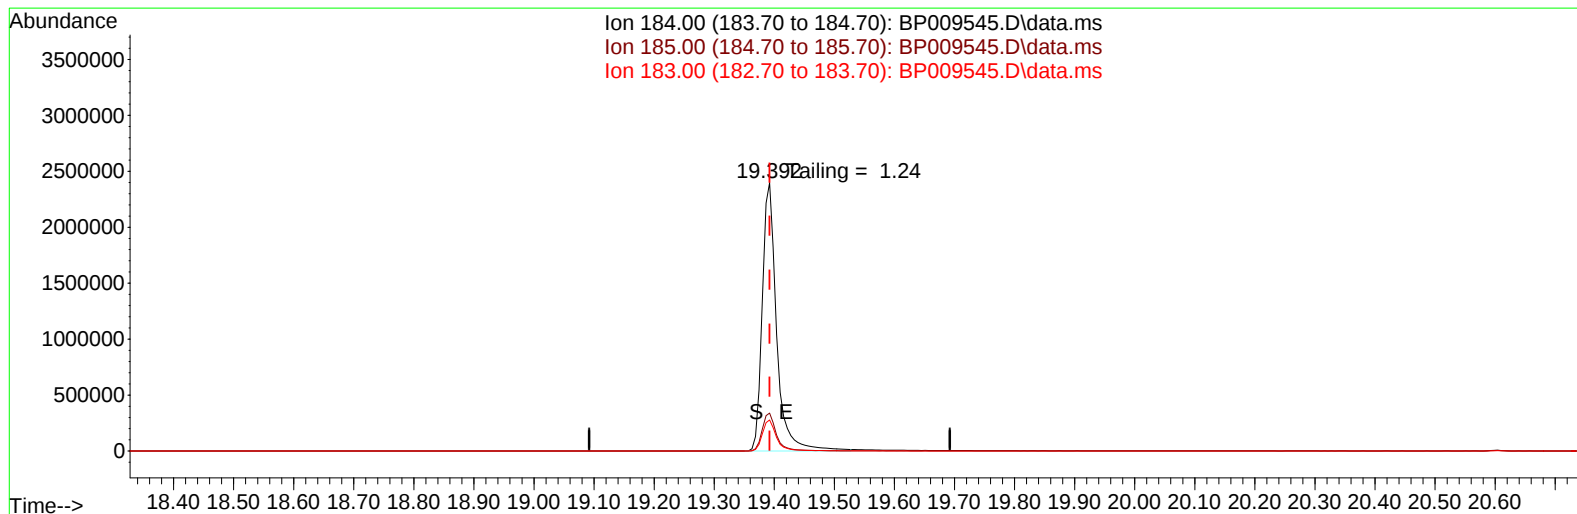

TIC: BP009545.D\data.ms

(77) Benzidine**19.392min (-0.000) 1263795.16 ng****response 4089002**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	11.70	11.59
0.00	0.00	0.00