

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
 Data File : BP009547.D
 Acq On : 25 Mar 2022 11:10
 Operator : CG/JU
 Sample : PB143517BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143517BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	399	406	429	rBV	4835246	8352934	34.87%	8.758%
2	6.958	667	675	695	rBV	4733175	8794287	36.71%	9.221%
3	7.769	806	813	829	rBV	879479	1566347	6.54%	1.642%
4	8.928	1001	1010	1037	rBV	2869771	5603332	23.39%	5.875%
5	10.563	1279	1288	1310	rBV	1121755	2306007	9.63%	2.418%
6	13.034	1700	1708	1735	rBV	8555480	14320652	59.78%	15.015%
7	14.416	1933	1943	1962	rBV	1994945	3399008	14.19%	3.564%
8	15.916	2190	2198	2229	rBV	7083024	11837564	49.41%	12.412%
9	17.181	2405	2413	2431	rBV	2531695	4341221	18.12%	4.552%
10	19.763	2845	2852	2864	rBV	17580504	23957448	100.00%	25.119%
11	21.292	3107	3112	3125	rBV	3721829	5353038	22.34%	5.613%
12	23.686	3512	3519	3533	rVB2	2406396	5543727	23.14%	5.813%




Sum of corrected areas: 95375565

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009547.D
Acq On : 25 Mar 2022 11:10
Operator : CG/JU
Sample : PB143517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143517BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

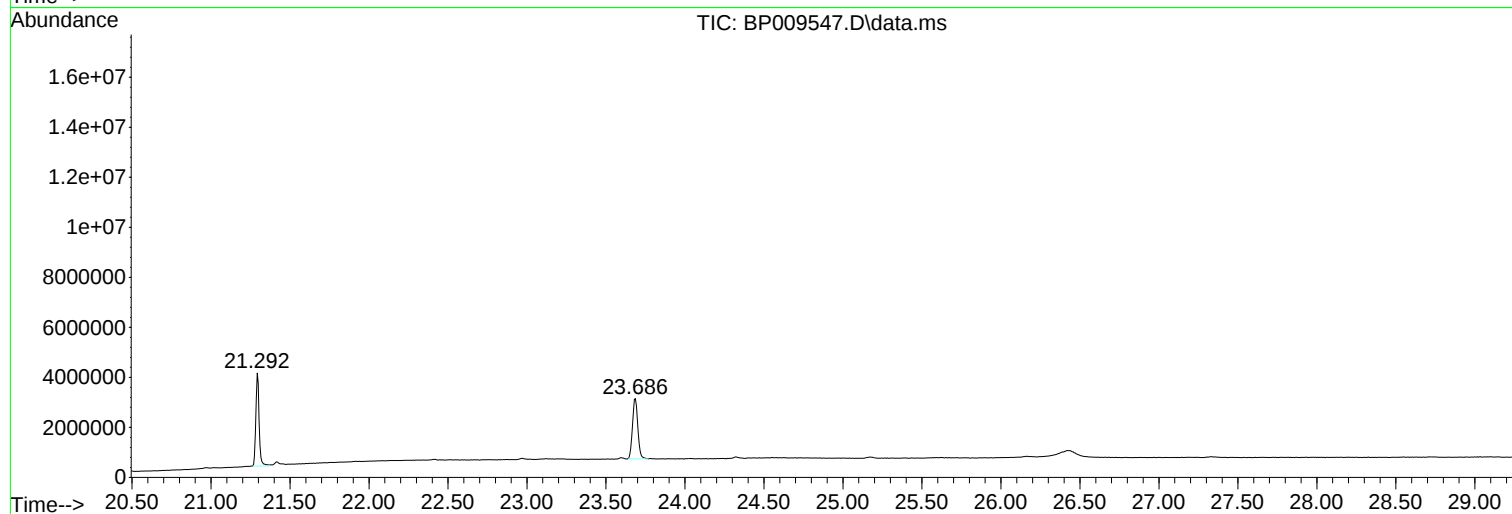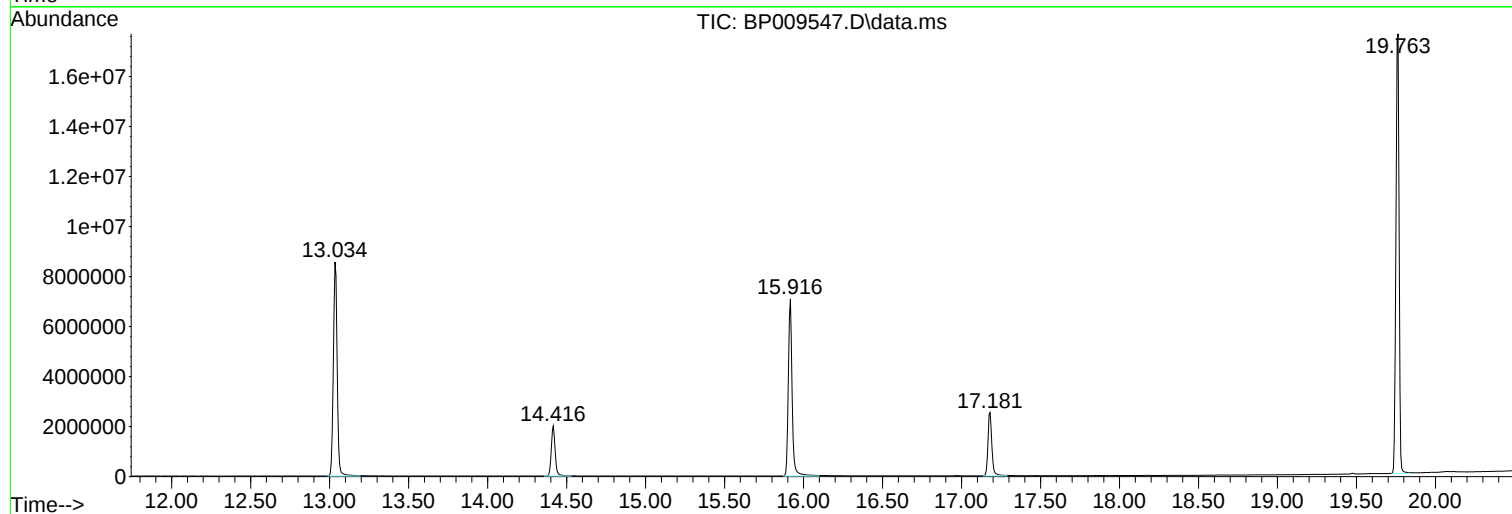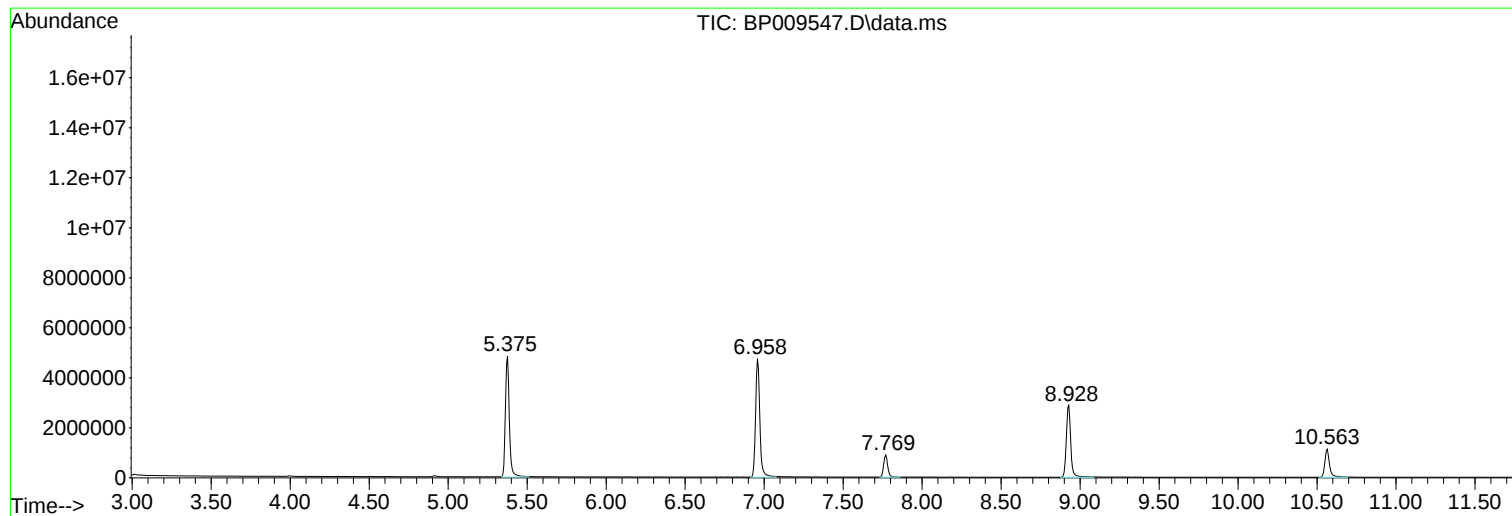

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009547.D
Acq On : 25 Mar 2022 11:10
Operator : CG/JU
Sample : PB143517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143517BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009547.D
Acq On : 25 Mar 2022 11:10
Operator : CG/JU
Sample : PB143517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143517BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------