

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
 Data File : BP009548.D
 Acq On : 25 Mar 2022 11:58
 Operator : CG/JU
 Sample : PB143570BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143570BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	399	406	427	rBV	5585082	9581708	37.28%	9.207%
2	6.964	668	676	703	rBV	5493805	9907940	38.54%	9.520%
3	7.775	806	814	831	rBV	1002407	1833609	7.13%	1.762%
4	8.934	1002	1011	1034	rBV	3214220	6331264	24.63%	6.084%
5	10.569	1280	1289	1306	rBV	1273094	2603138	10.13%	2.501%
6	13.040	1700	1709	1734	rBV	9583137	15795548	61.45%	15.178%
7	14.422	1937	1944	1962	rBV	2242226	3725678	14.49%	3.580%
8	15.922	2190	2199	2227	rBV	7683074	12837036	49.94%	12.335%
9	17.187	2407	2414	2429	rBV	2723262	4669745	18.17%	4.487%
10	19.769	2847	2853	2870	rBV	19381564	25705126	100.00%	24.700%
11	21.304	3109	3114	3128	rBV	3921621	5526106	21.50%	5.310%
12	23.704	3514	3522	3537	rVB2	2476405	5553169	21.60%	5.336%




Sum of corrected areas: 104070067

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009548.D
Acq On : 25 Mar 2022 11:58
Operator : CG/JU
Sample : PB143570BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143570BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

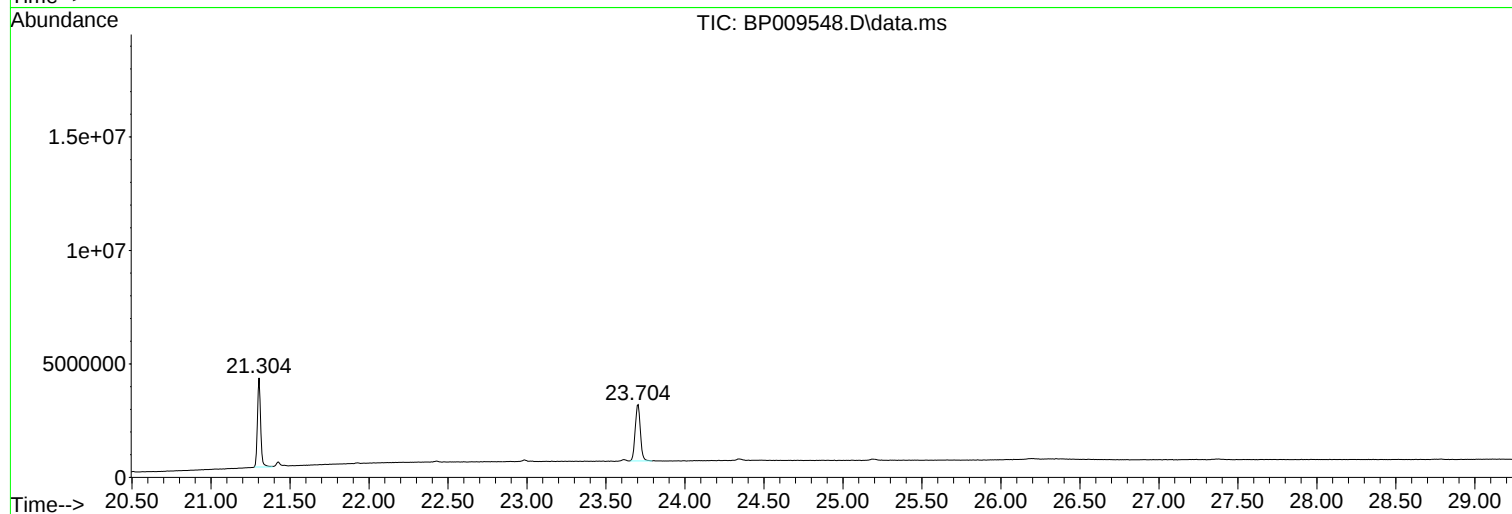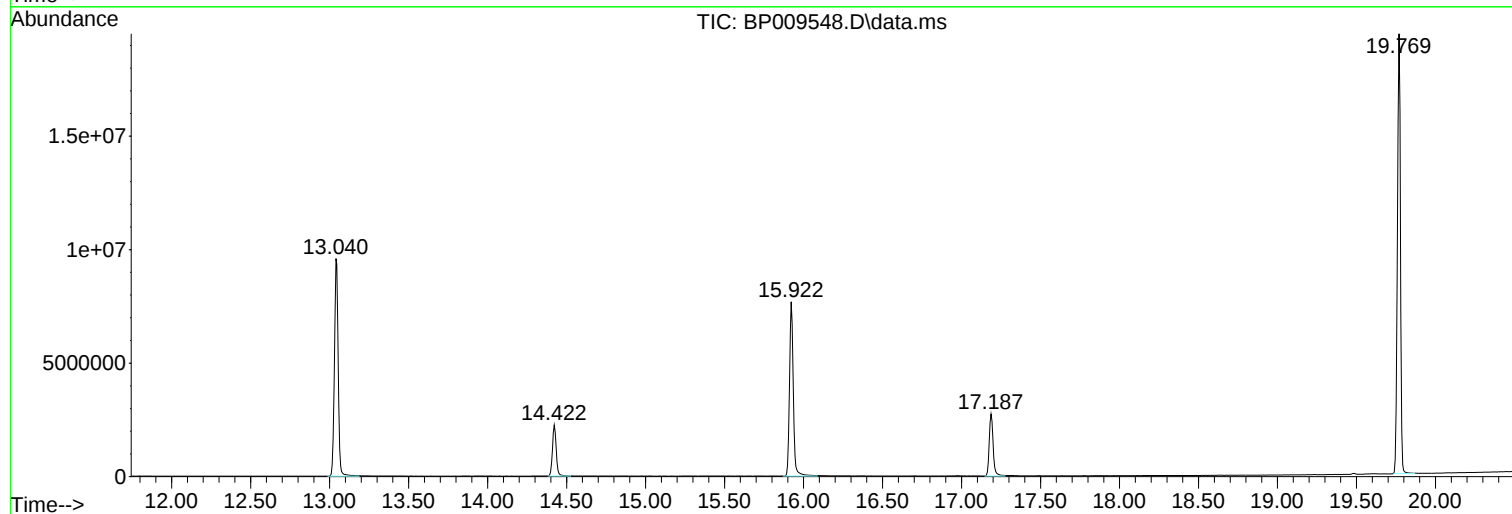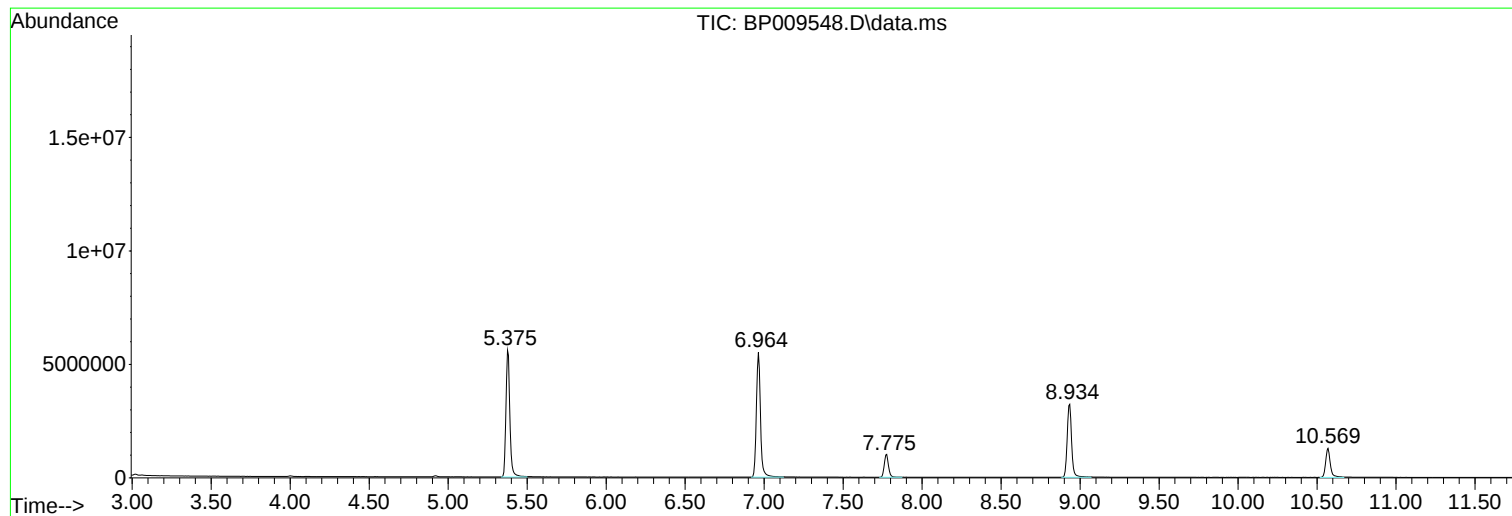

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009548.D
Acq On : 25 Mar 2022 11:58
Operator : CG/JU
Sample : PB143570BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143570BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009548.D
Acq On : 25 Mar 2022 11:58
Operator : CG/JU
Sample : PB143570BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143570BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------