
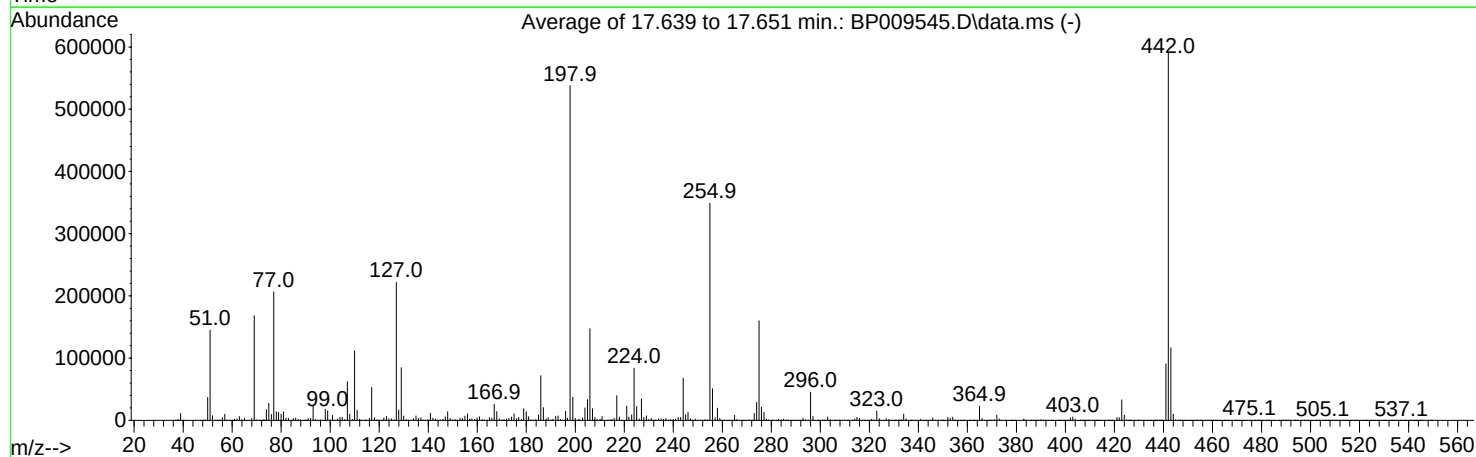


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
 Data File : BP009545.D
 Acq On : 25 Mar 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 06:34:38 2022

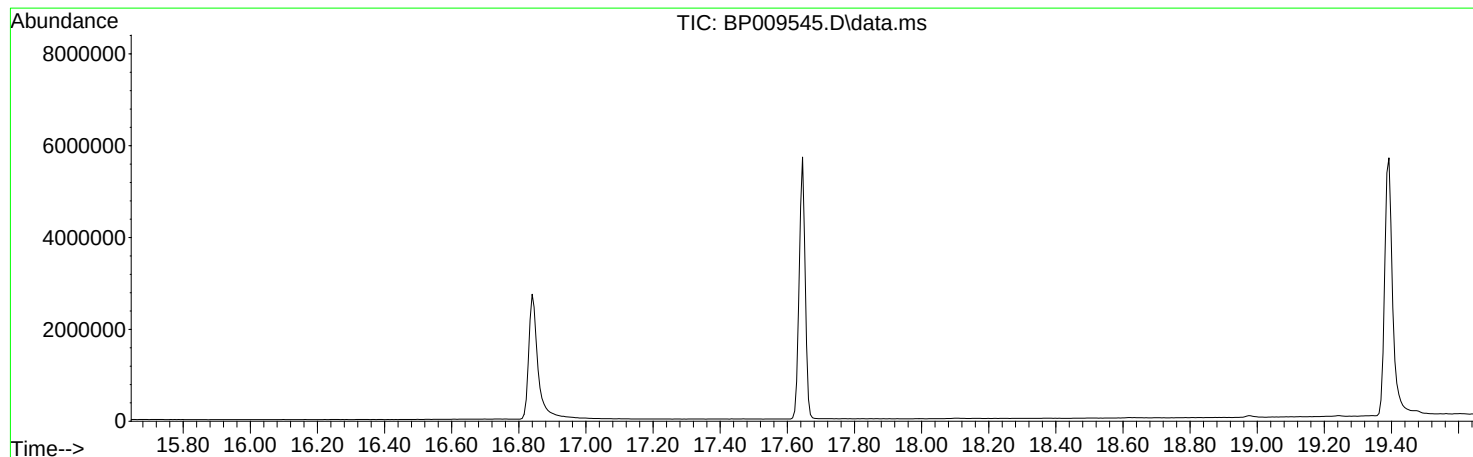


AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	144789	PASS
68	69	0.00	2	1.6	2748	PASS
69	198	0.00	100	31.3	168160	PASS
70	69	0.00	2	0.5	923	PASS
127	198	10	80	41.2	221728	PASS
197	198	0.00	2	0.7	3497	PASS
198	198	100	100	100.0	537797	PASS
199	198	5	9	6.9	37333	PASS
275	198	10	60	29.8	160034	PASS
365	198	1	100	4.2	22620	PASS
441	198	0.01	100	16.9	90661	PASS
442	442	100	100	100.0	591168	PASS
443	442	15	24	19.7	116507	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
 Data File : BP009545.D
 Acq On : 25 Mar 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 07:49:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

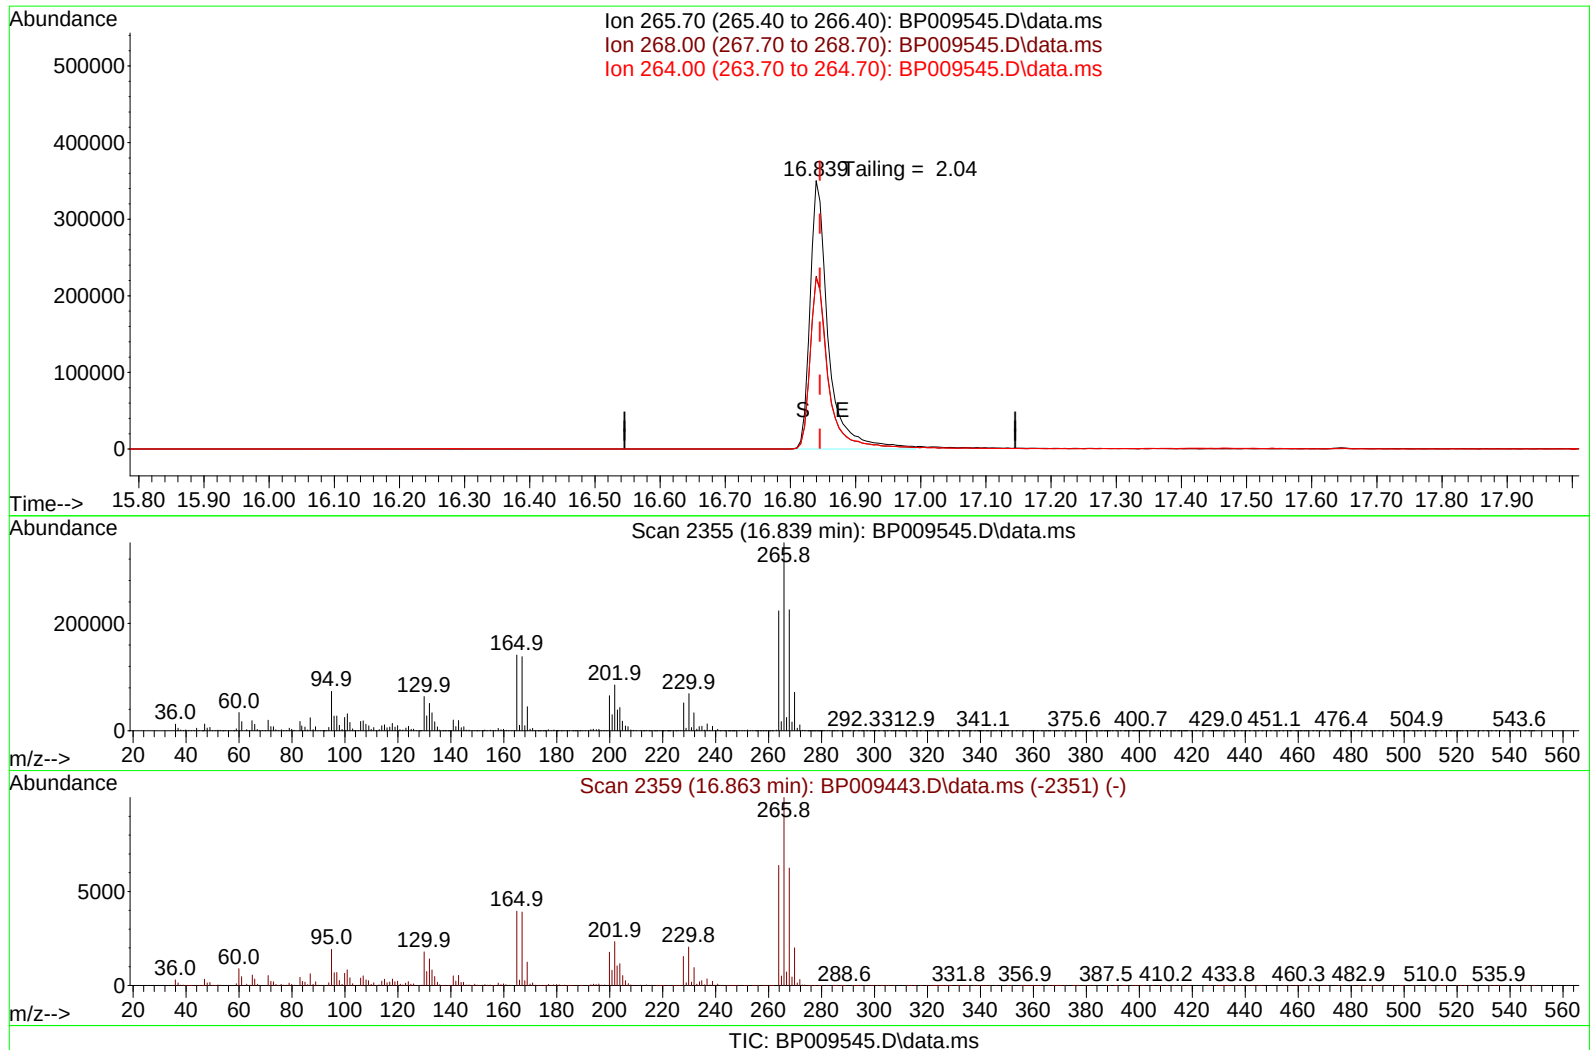

TIC: BP009545.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 712801.89 ng




response 686865

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.33
264.00	63.60	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032522\
Data File : BP009545.D
Acq On : 25 Mar 2022 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 26 07:49:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration

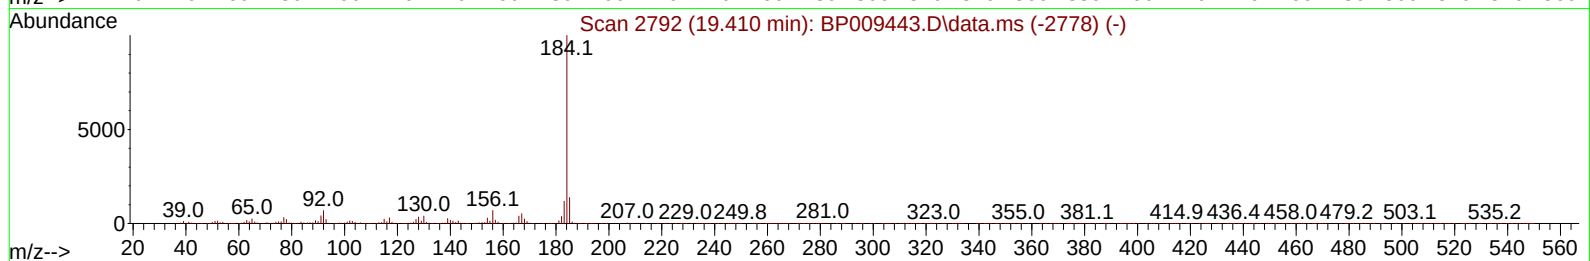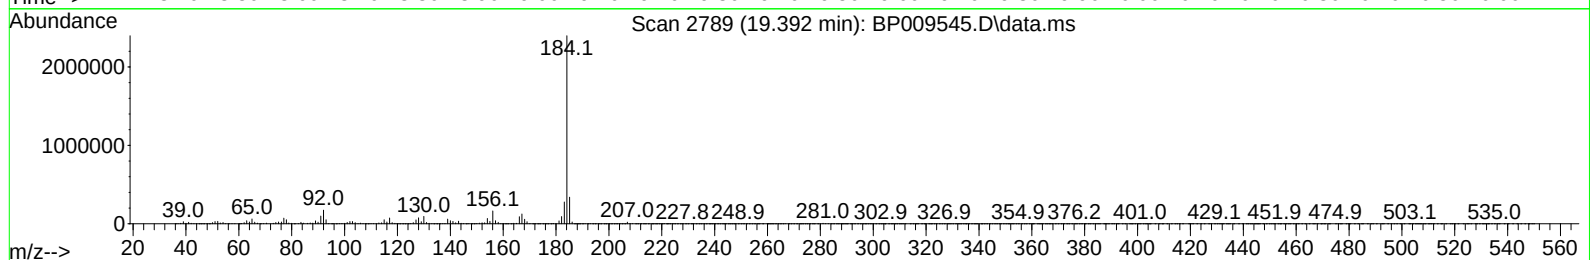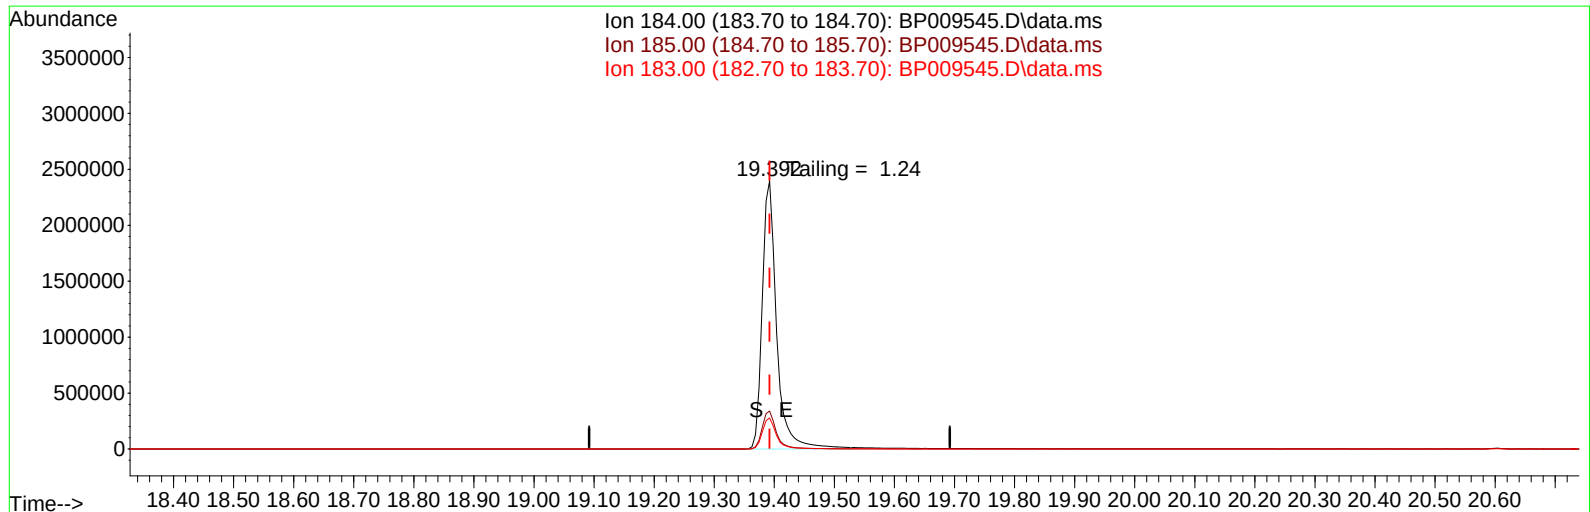

TIC: BP009545.D\data.ms

(77) Benzidine

19.392min (-0.000) 1263795.16 ng

response 4089002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	11.70	11.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2022	BNA_P	<u>BP009545.D</u>
Compound Name	Response	Retention Time
DDT	2071137	20.604
DDD	63888	20.175
DDE	4160	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68048	2139185	3.18

Instrument :
BNA_P
ClientSampleId :
DFTPP