


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005087.D
Acq On : 29 Mar 2021 22:28
Operator : CG/JU
Sample : M1818-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:10:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

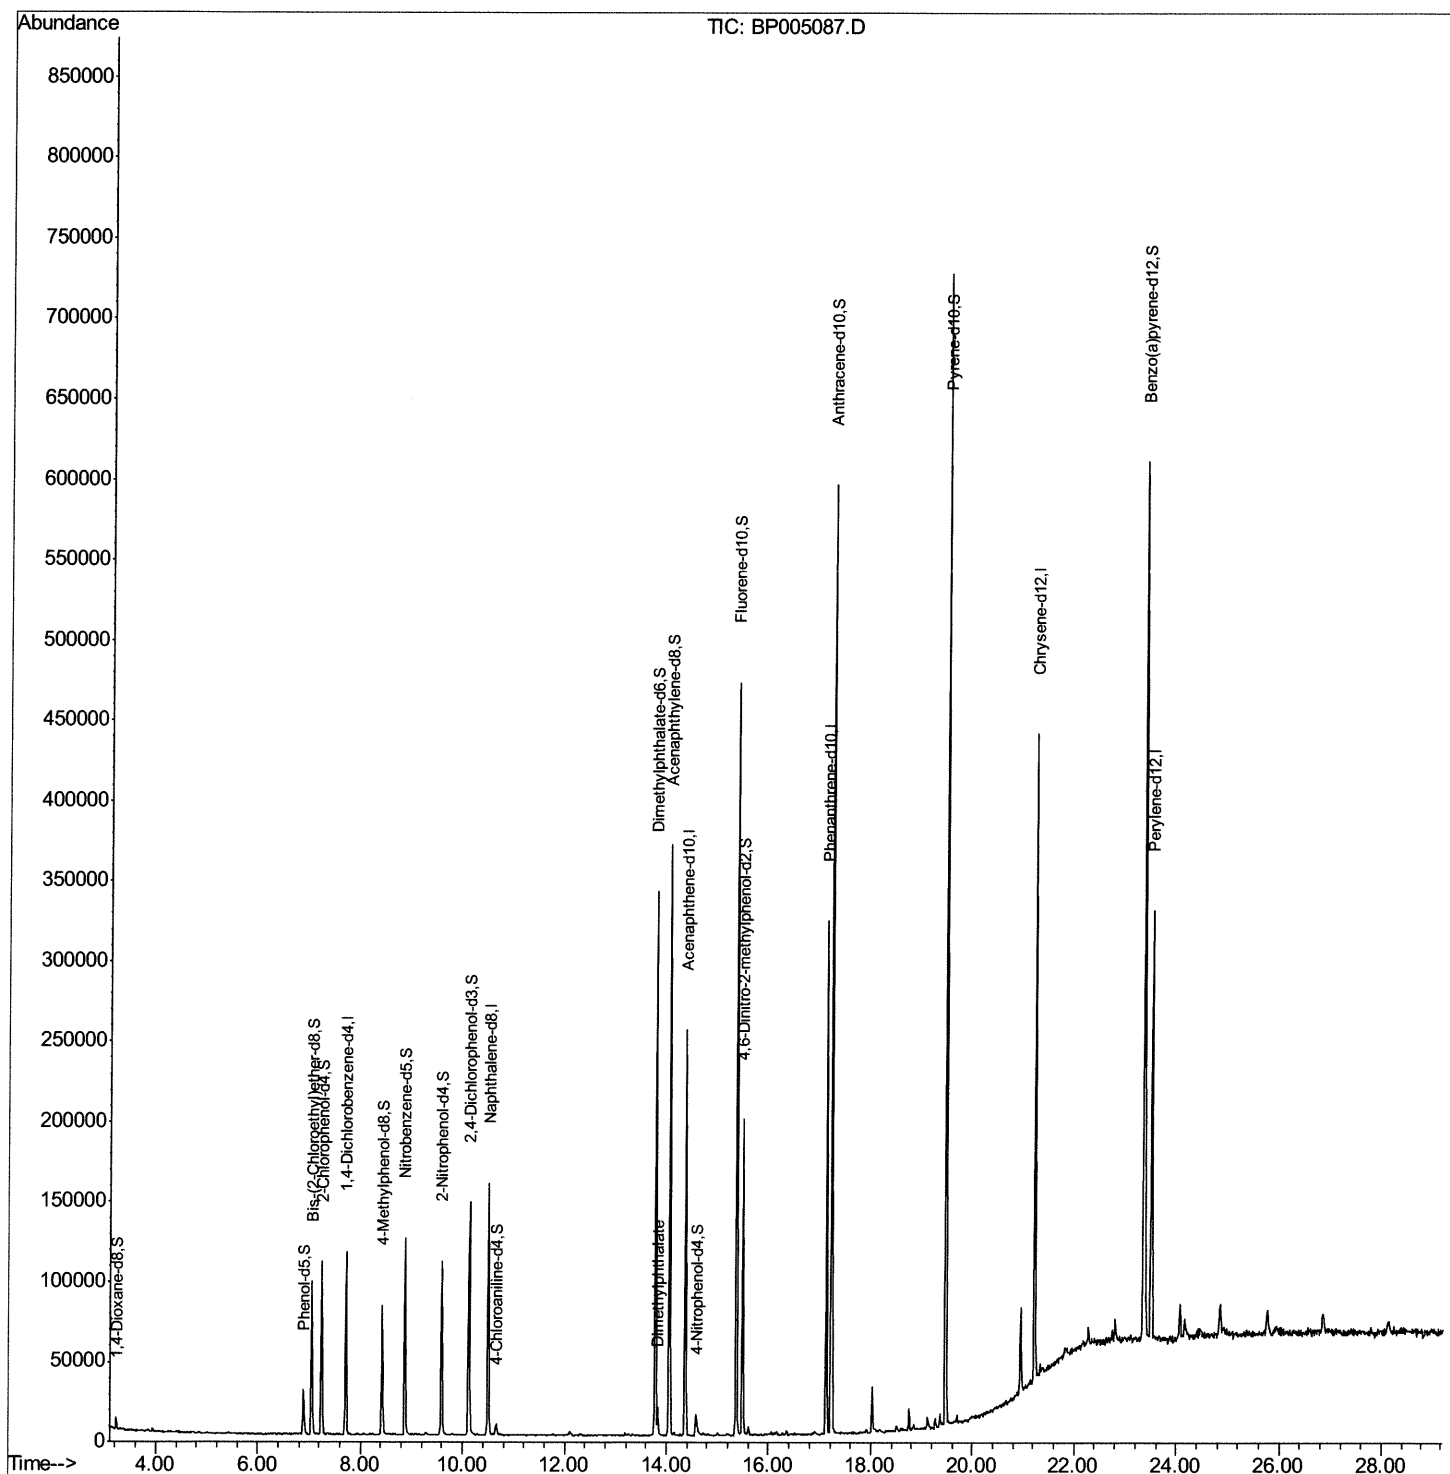

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005087.D
Acq On : 29 Mar 2021 22:28
Operator : CG/JU
Sample : M1818-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:07:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

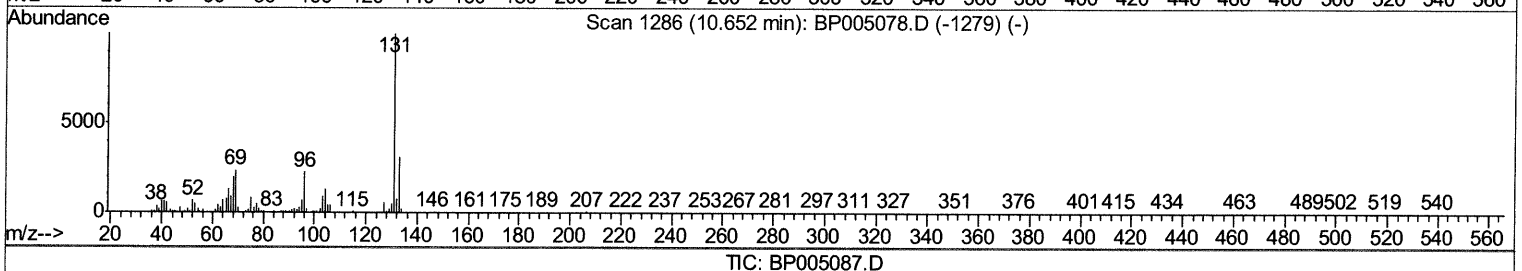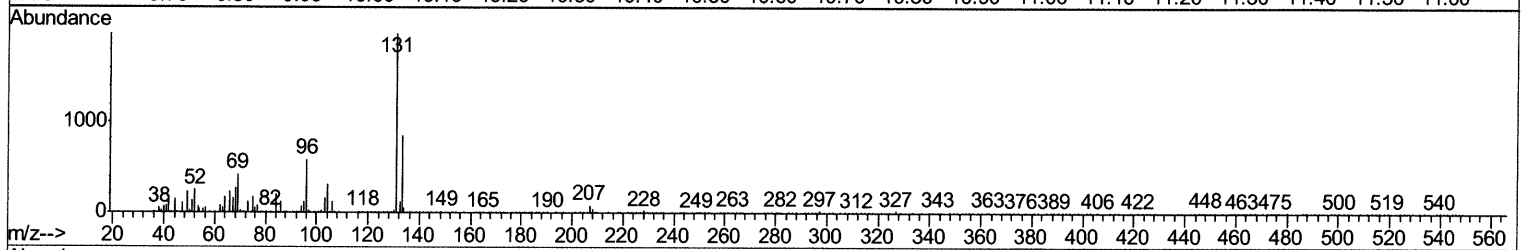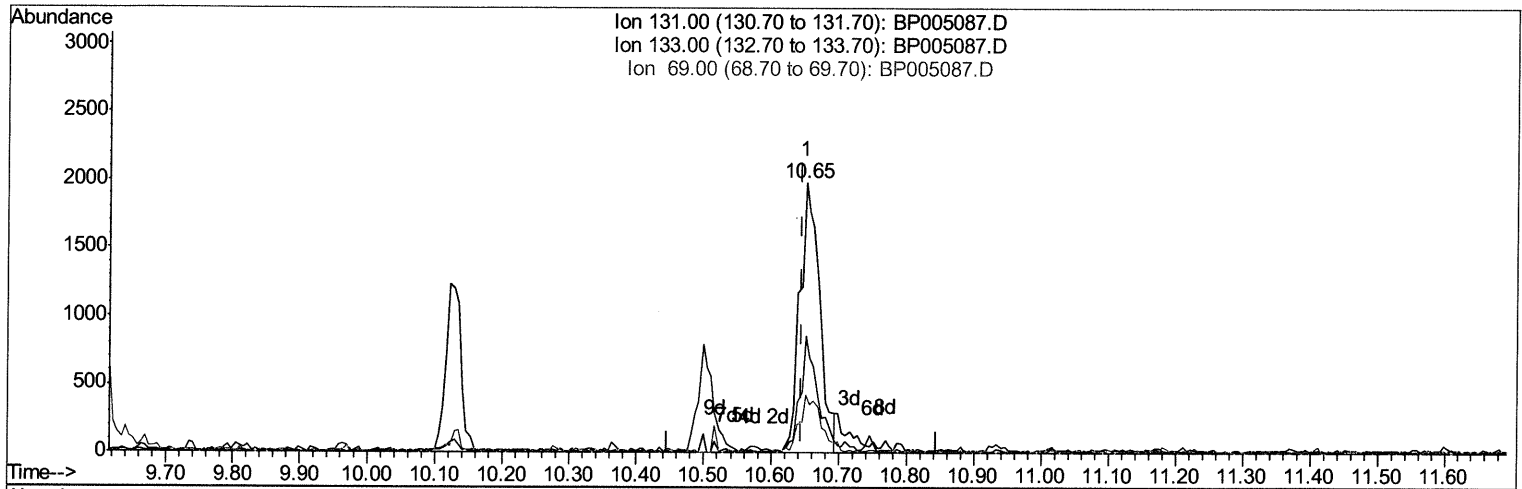

TIC: BP005087.D

(29) 4-Chloroaniline-d4 (S)

10.652min (+0.006) 1.86ng/ul

response 3989

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	43.06#
69.00	21.50	21.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005087.D
 Acq On : 29 Mar 2021 22:28
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:07:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

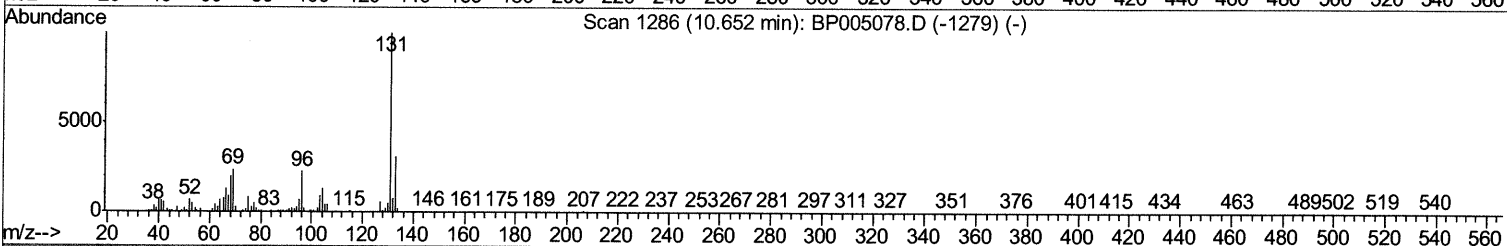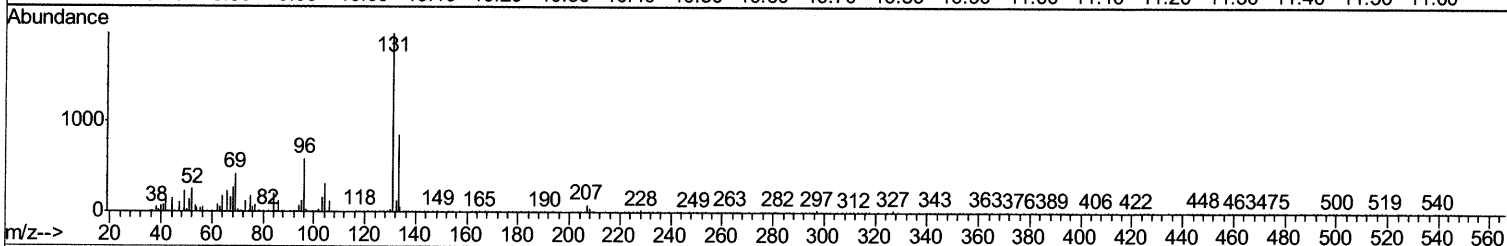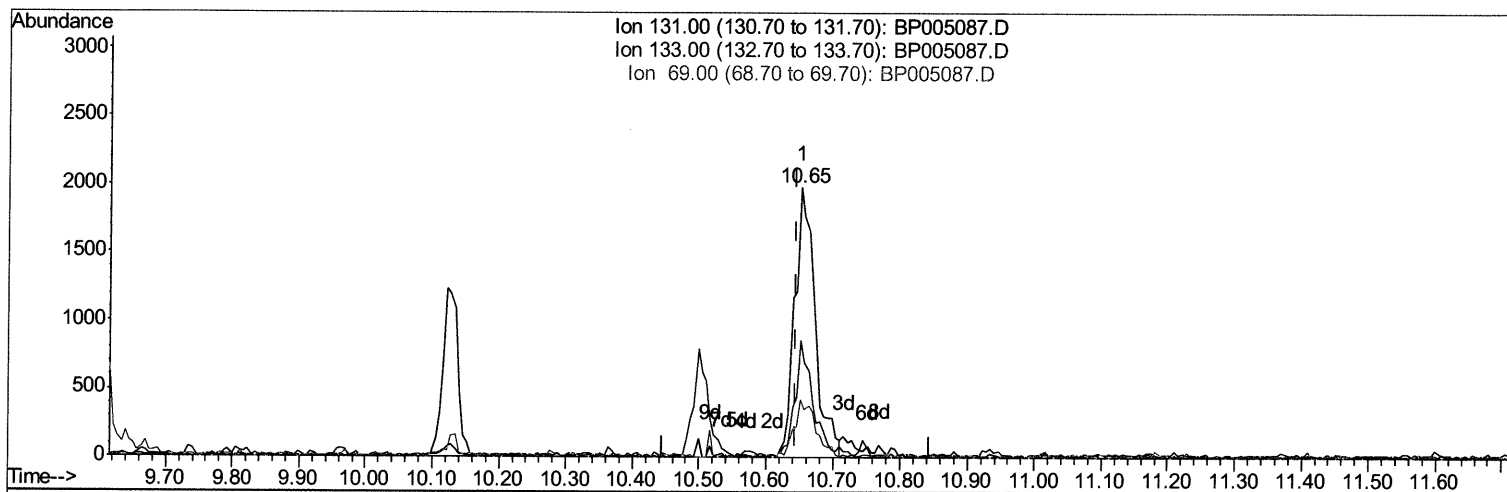

TIC: BP005087.D

(29) 4-Chloroaniline-d4 (S)

10.652min (+0.006) 1.95ng/ul m

04/01/21 JU

response 4184

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	43.06#
69.00	21.50	21.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005087.D
 Acq On : 29 Mar 2021 22:28
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampled :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:09:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

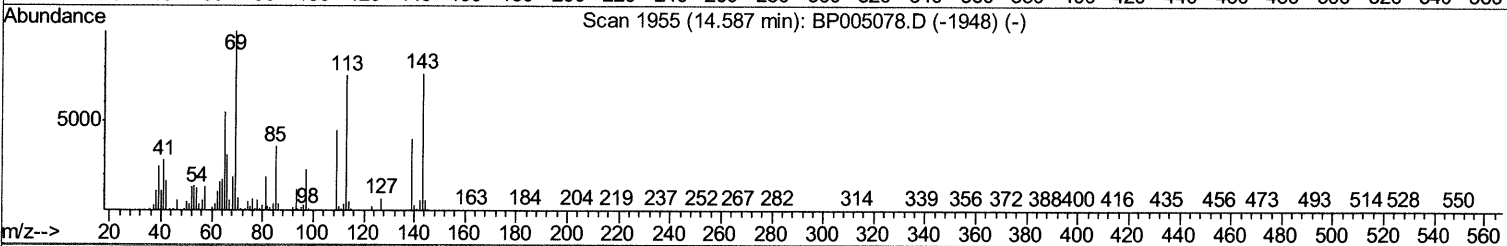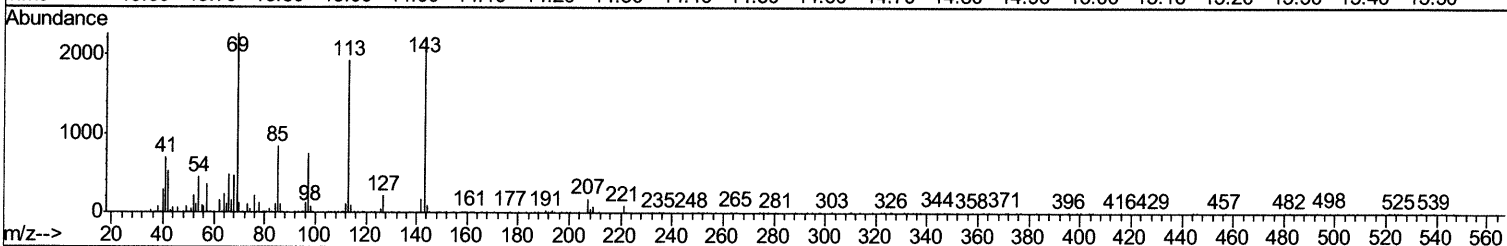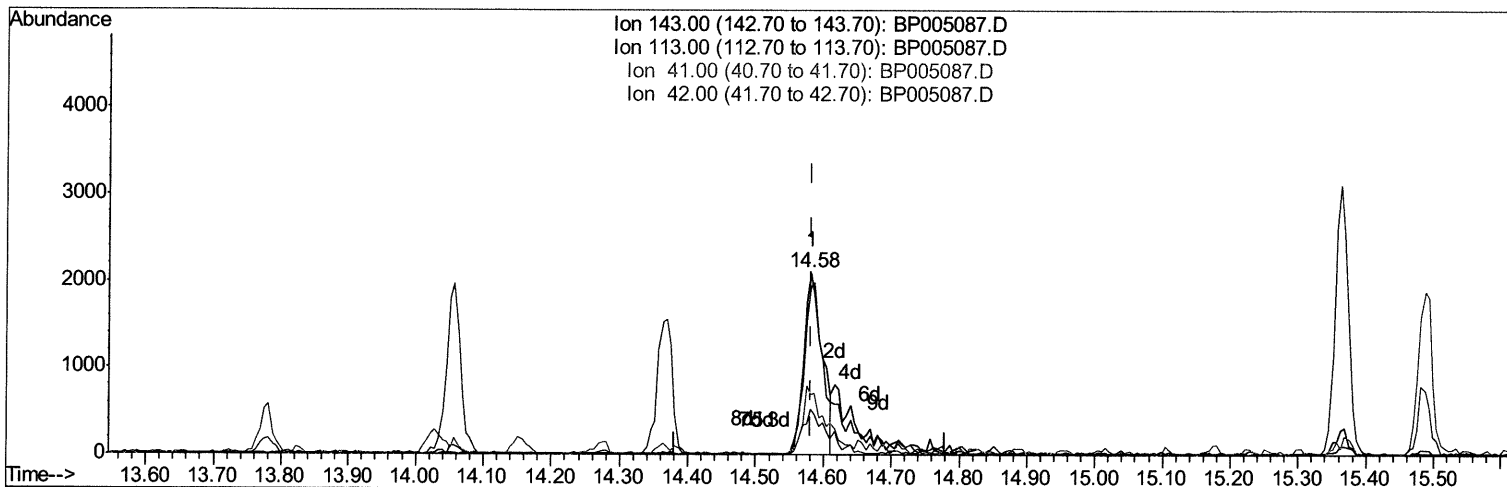

TIC: BP005087.D

(52) 4-Nitrophenol-d4 (S)
 14.581min (+0.000) 4.07ng/ul
 response 3982

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	91.79
41.00	27.10	33.16#
42.00	18.80	25.14#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005087.D
 Acq On : 29 Mar 2021 22:28
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampled :
 C0AA1

Manual Integrations
APPROVED

mohammad
 3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:09:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

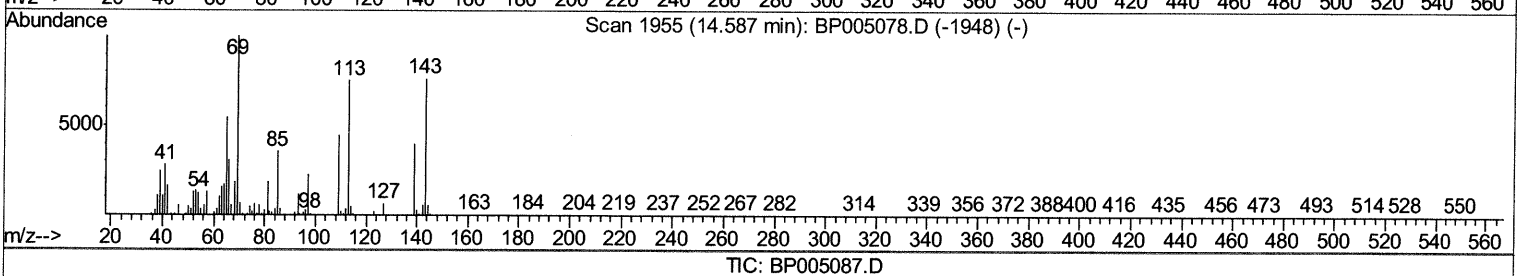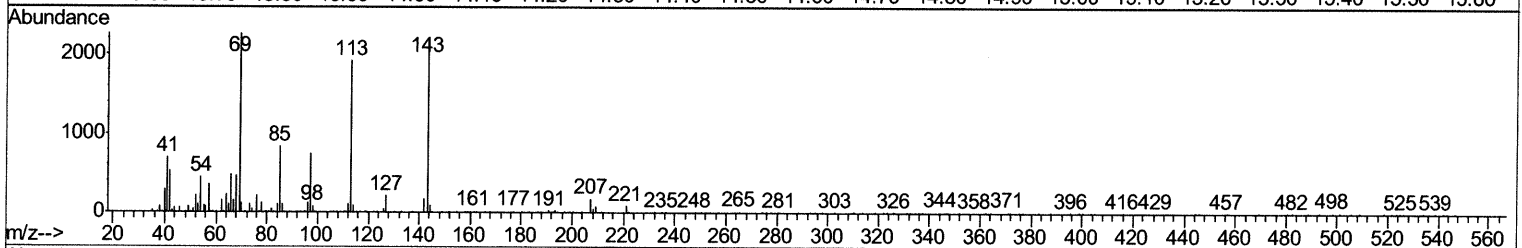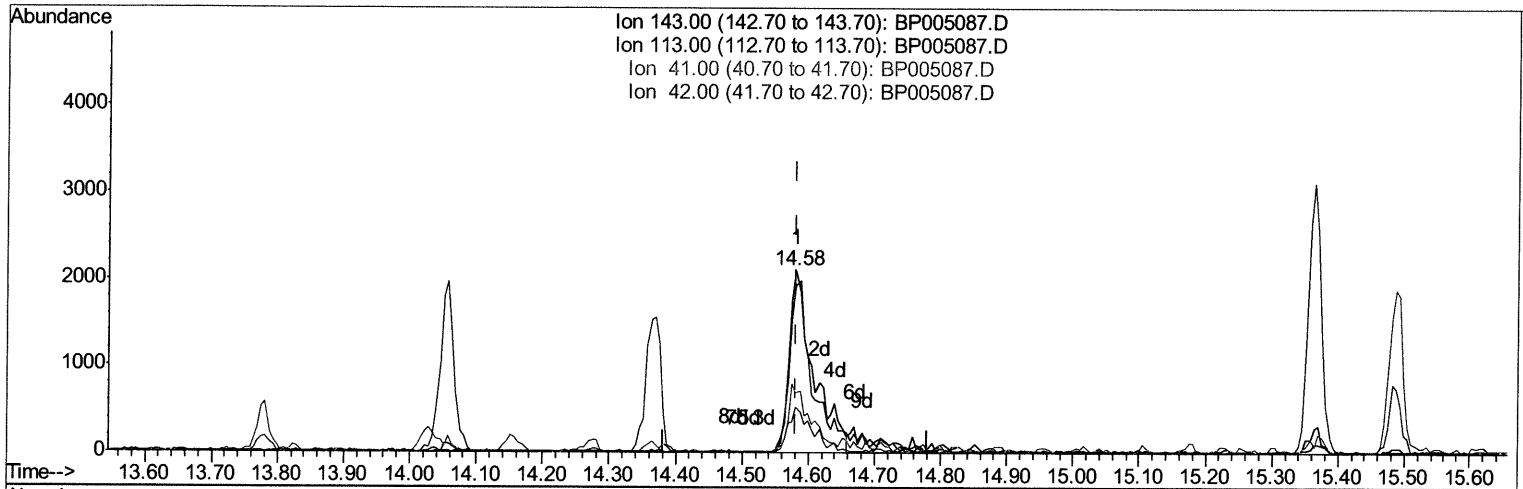

(52) 4-Nitrophenol-d4 (S)

14.581min (+0.000) 5.41ng/ul m 04/01/21 JU

response 5303

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	91.79
41.00	27.10	33.16#
42.00	18.80	25.14#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032921\
 Data File : BP005087.D
 Acq On : 29 Mar 2021 22:28
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:10:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	30106	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	122081	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	82591	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	185101	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	194416	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	197928	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3650	4.58	ng/uL	0.00
5) Phenol-d5	6.89	99	16040	6.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	40114	29.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	43626	23.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	29333	14.81	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	27341	30.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	31915	32.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	50605	26.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	4184m >	1.95	ng/ul >	0.00
44) Dimethylphthalate-d6	13.78	166	201344	33.57	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	236198	31.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	5303m >	5.41	ng/ul >	0.00
58) Fluorene-d10	15.36	176	177232	34.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	40471	33.10	ng/ul	0.00
71) Anthracene-d10	17.23	188	314461	37.74	ng/ul	0.00
79) Pyrene-d10	19.47	212	353941	38.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	392448	38.60	ng/ul	0.00

04/01/2021

04/01/2021

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.83	163	10248	1.671	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed