


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005091.D
Acq On : 30 Mar 2021 00:44
Operator : CG/JU
Sample : M1818-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:37 PM

Quant Time: Mar 30 02:53:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

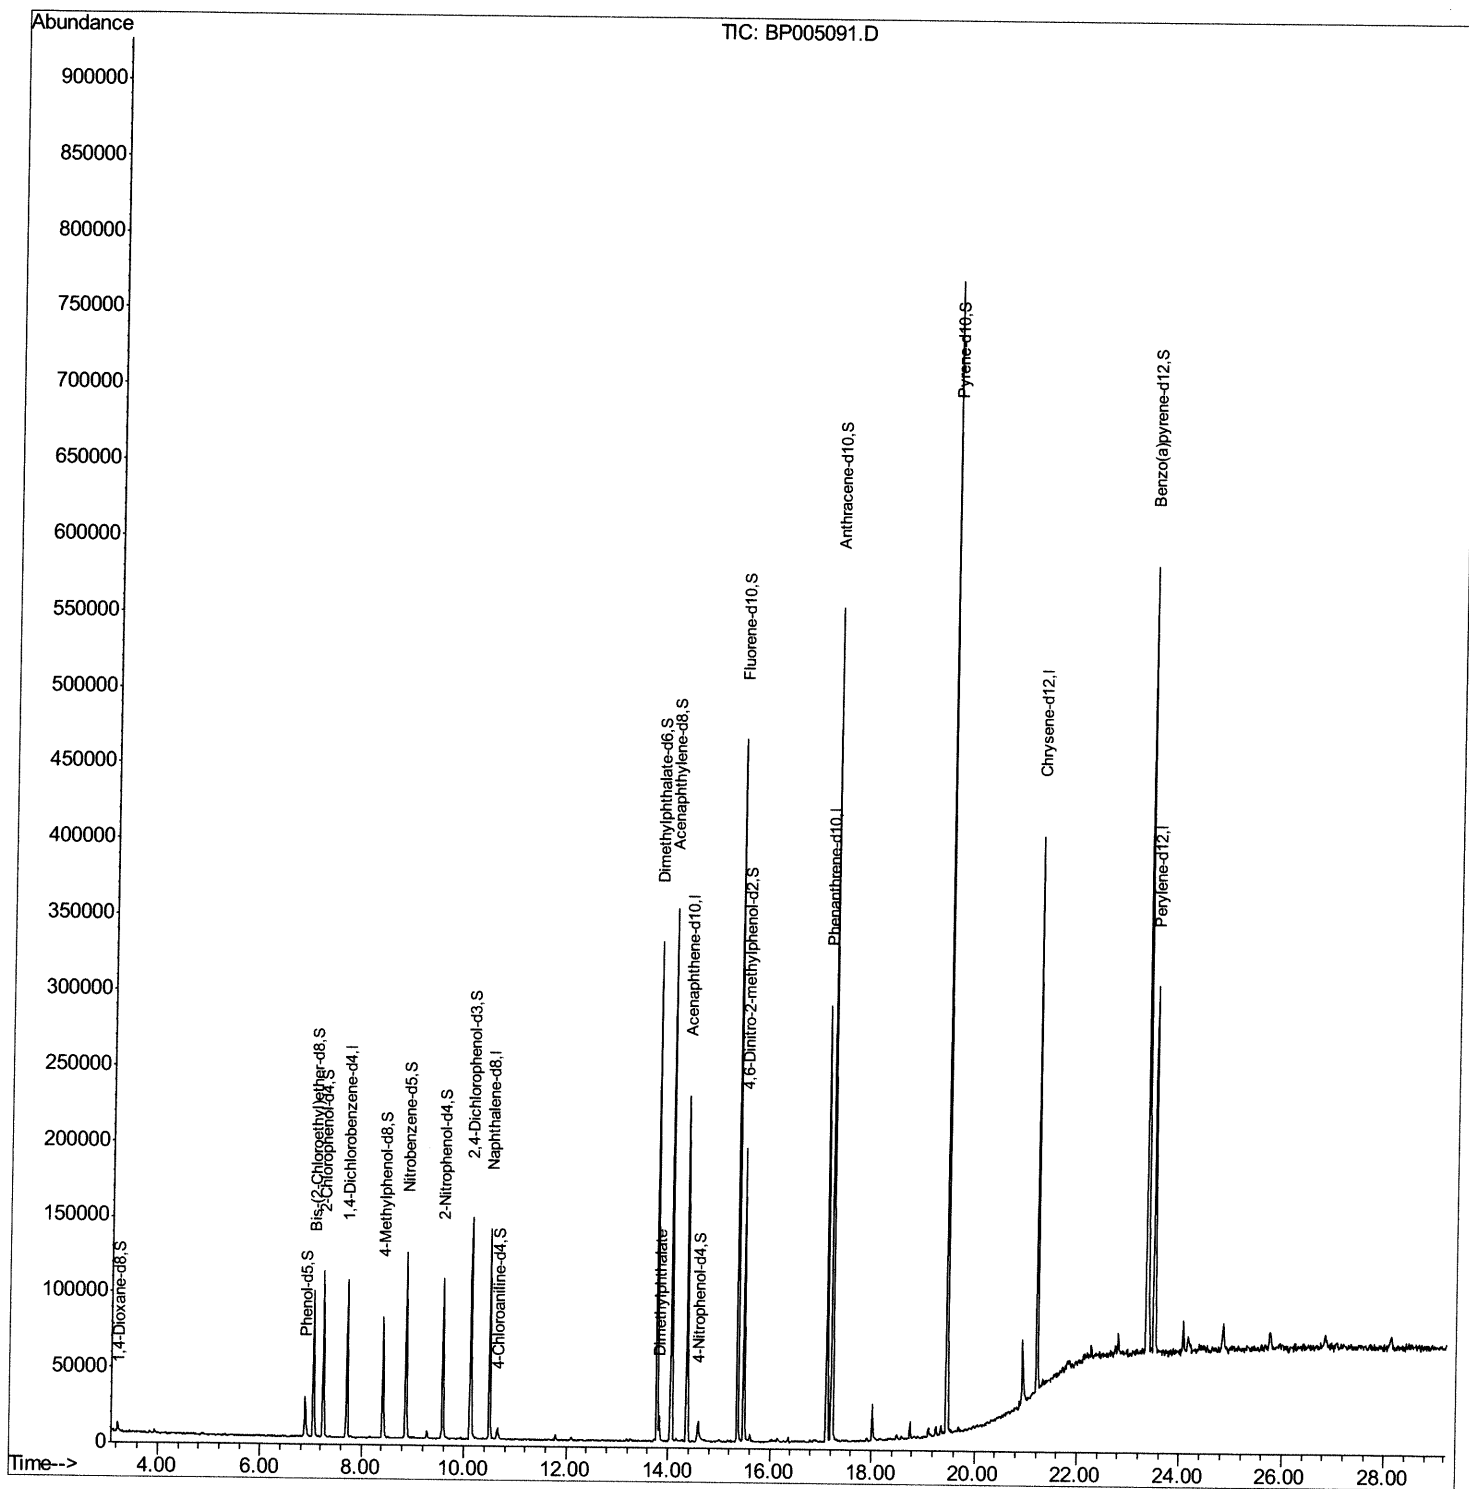


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005091.D
Acq On : 30 Mar 2021 00:44
Operator : CG/JU
Sample : M1818-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:37 PM

Quant Time: Mar 30 02:52:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

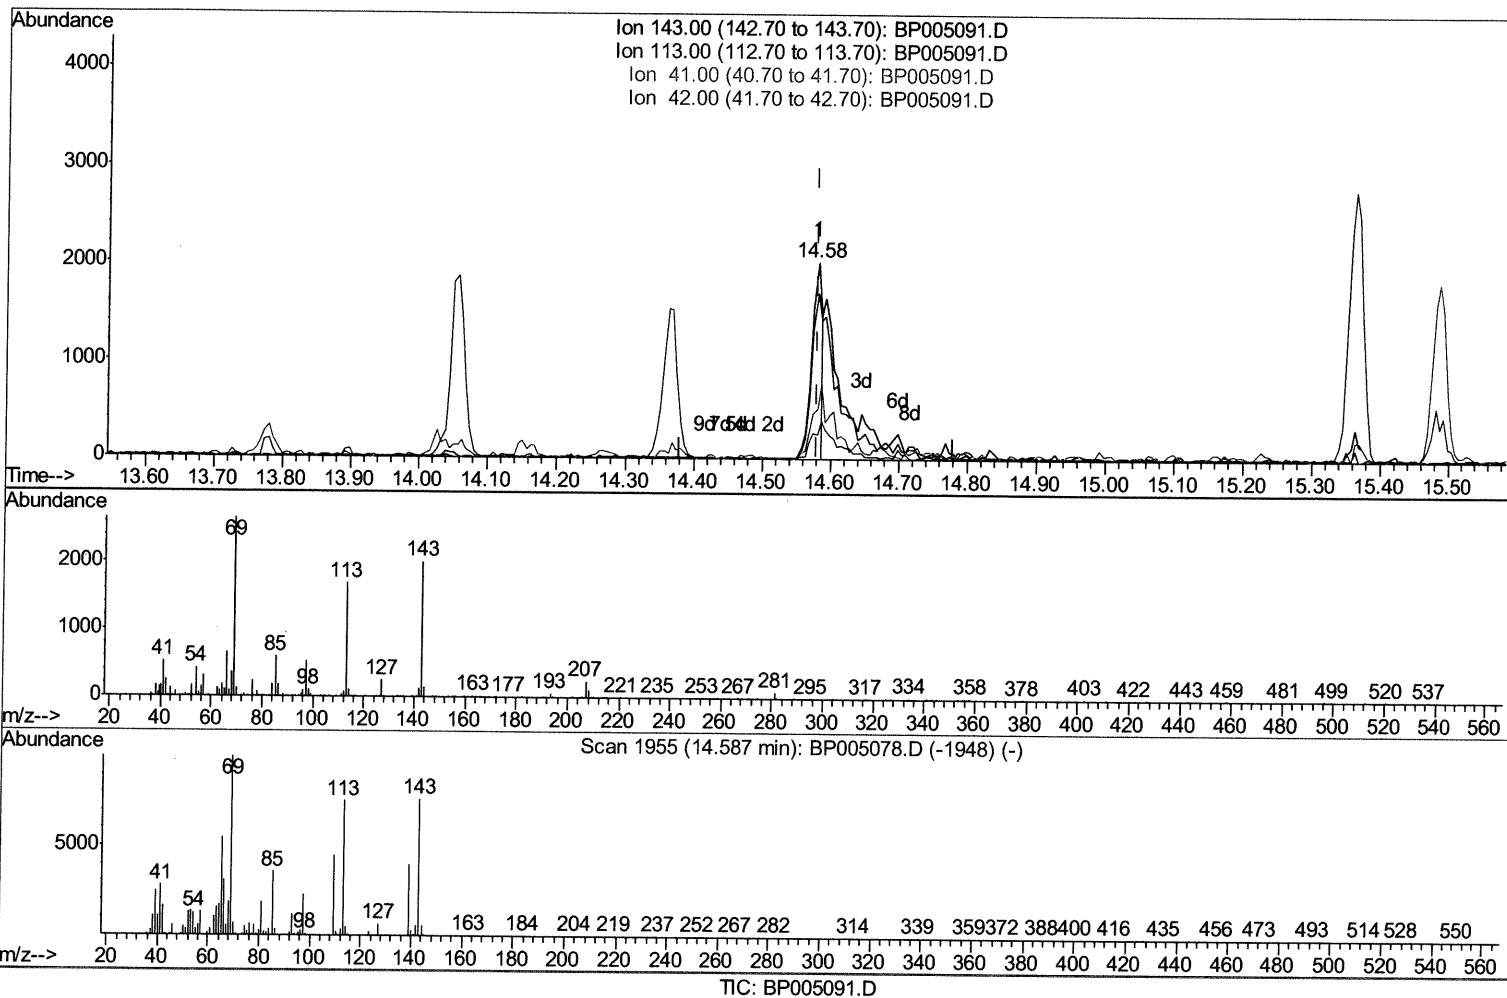

(52) 4-Nitrophenol-d4 (S)

14.581min (+0.000) 2.47ng/ul

response 2166

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	84.16
41.00	27.10	25.87
42.00	18.80	12.66#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005091.D
Acq On : 30 Mar 2021 00:44
Operator : CG/JU
Sample : M1818-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:37 PM

Quant Time: Mar 30 02:52:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

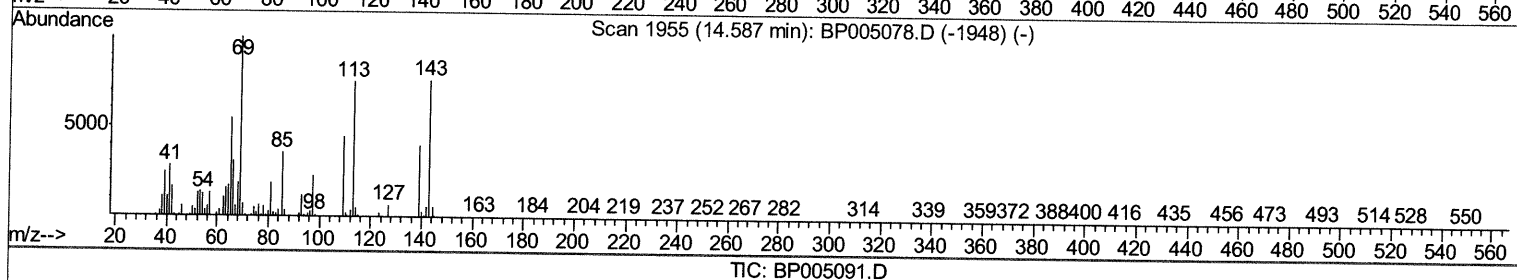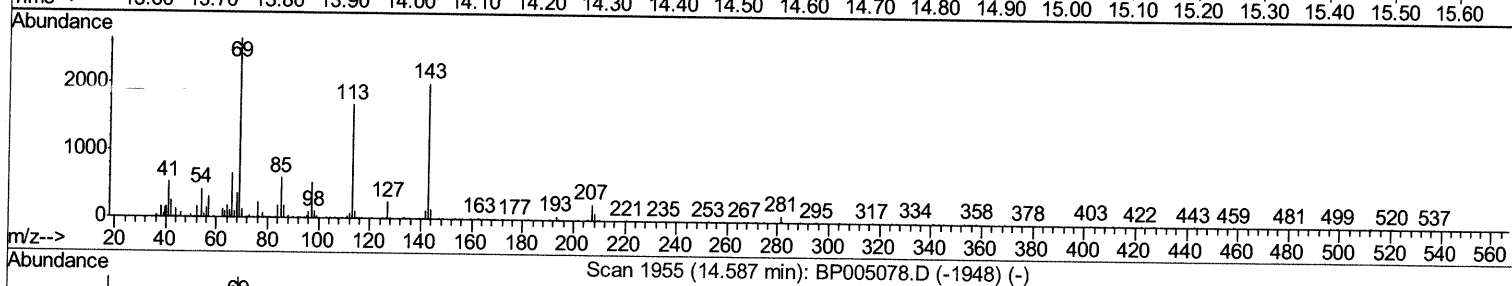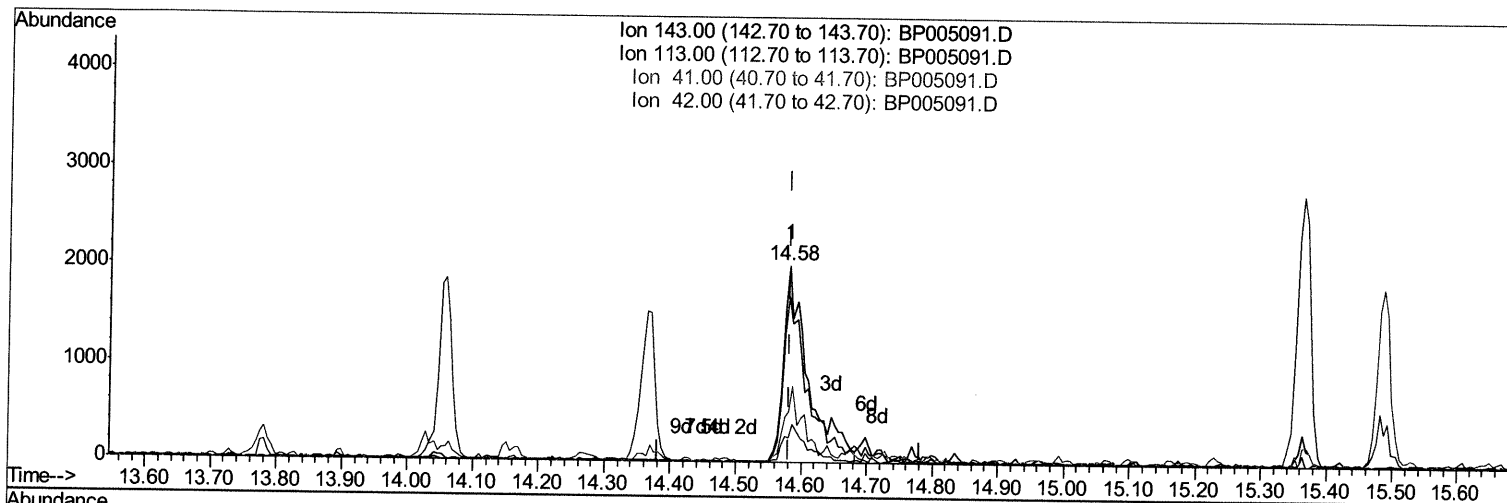

(52) 4-Nitrophenol-d4 (S)

14.581min (+0.000) 6.08ng/ul m 04/01/21 JU

response 5326

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	84.16
41.00	27.10	25.87
42.00	18.80	12.66#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032921\
 Data File : BP005091.D
 Acq On : 30 Mar 2021 00:44
 Operator : CG/JU
 Sample : M1818-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:37 PM

Quant Time: Mar 30 02:53:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	26974	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	112338	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	73920	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	163382	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	173870	20.00	ng/ul	-0.01
86) Perylene-d12	23.50	264	175690	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3650	5.11	ng/uL	0.00
5) Phenol-d5	6.89	99	15566	6.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	40857	33.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	43629	26.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	29019	16.36	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	27937	33.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	30937	33.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	50686	28.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	4592	2.33	ng/ul	0.01
44) Dimethylphthalate-d6	13.78	166	194591	36.25	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	230890	34.71	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	5326m >	6.08	ng/ul >	0.00 04/01/21
58) Fluorene-d10	15.36	176	170173	36.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	38108	35.32	ng/ul	0.00
71) Anthracene-d10	17.22	188	299586	40.73	ng/ul	0.00
79) Pyrene-d10	19.47	212	343937	41.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	381020	42.22	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.83	163	9469	1.725 ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed