


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005092.D
Acq On : 30 Mar 2021 01:18
Operator : CG/JU
Sample : M1818-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:10:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

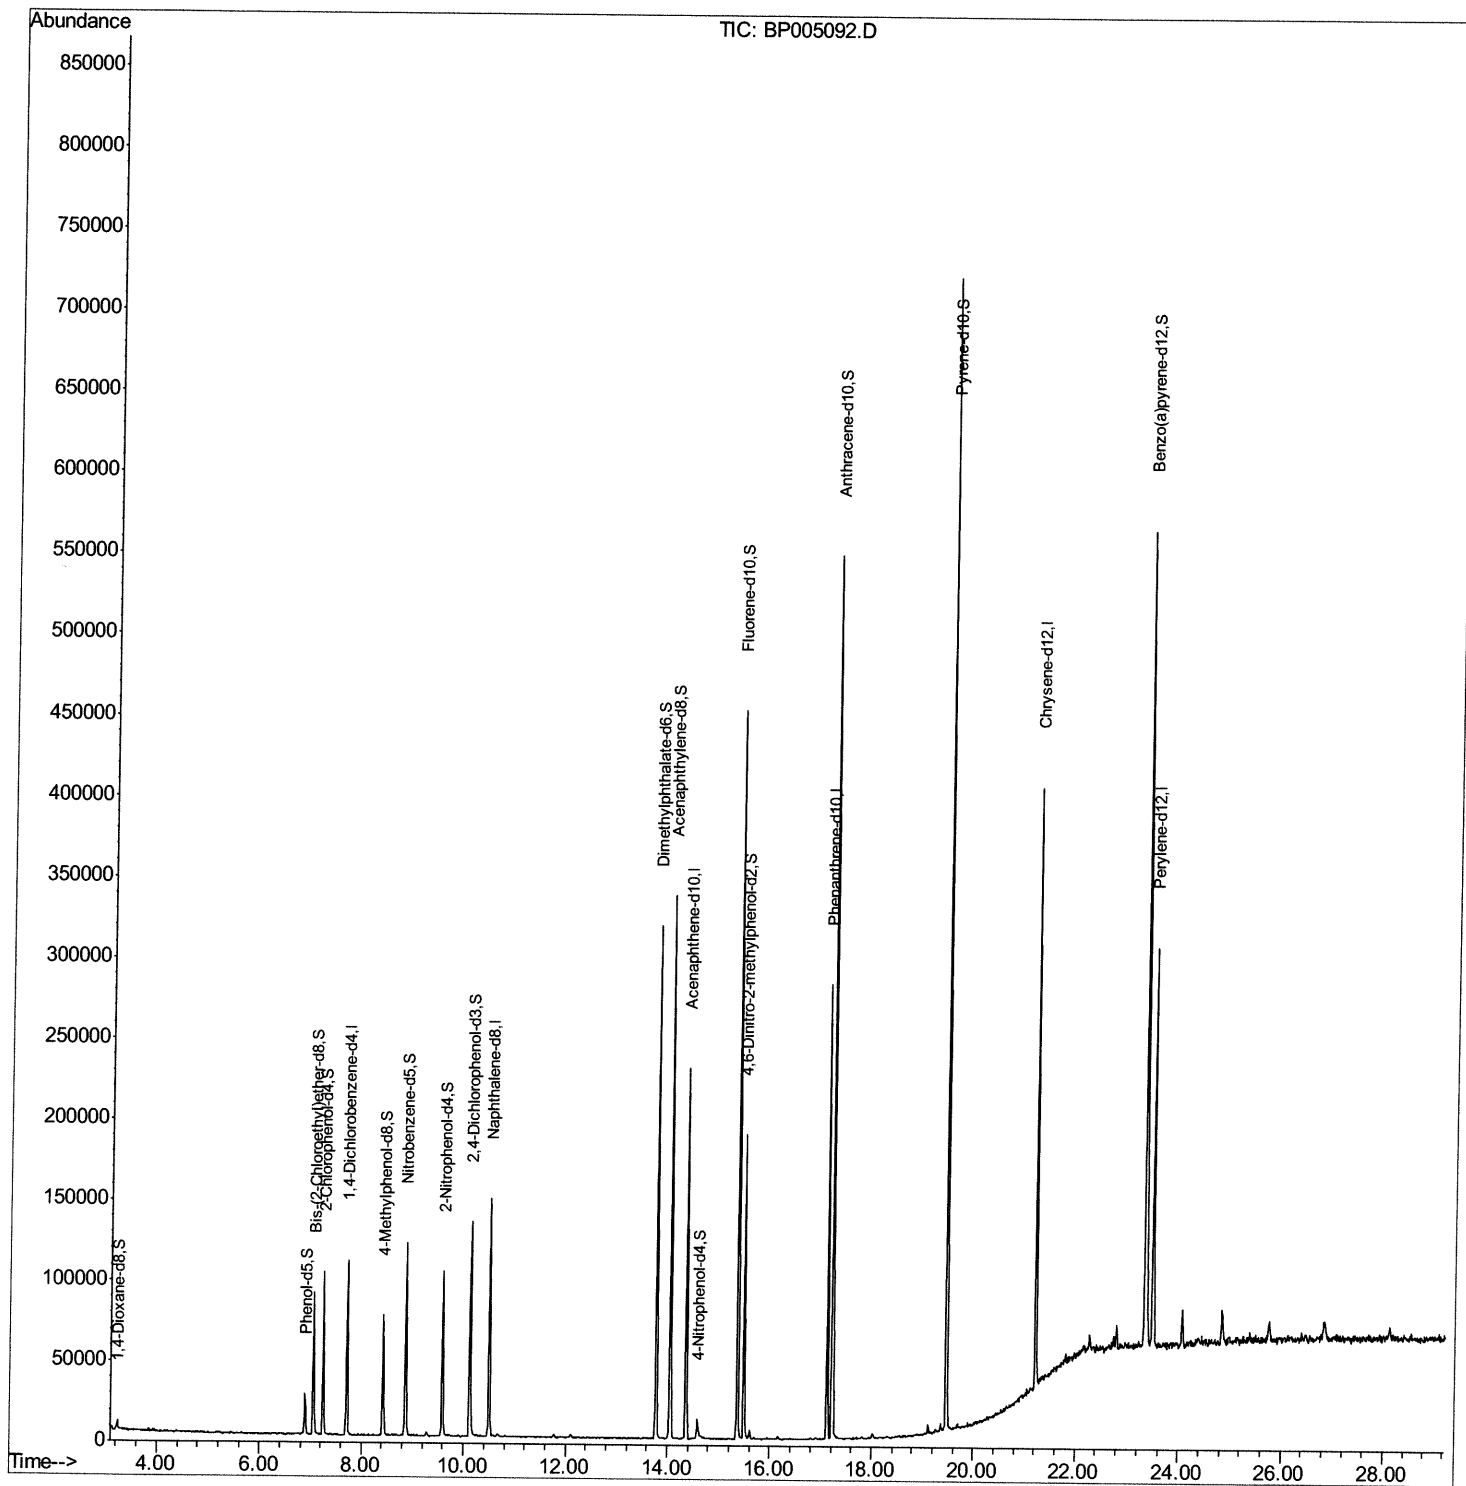

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005092.D
Acq On : 30 Mar 2021 01:18
Operator : CG/JU
Sample : M1818-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:07:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

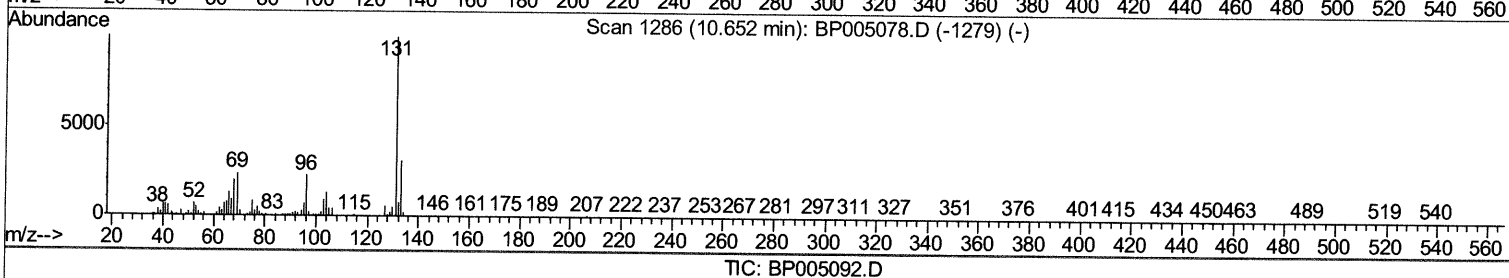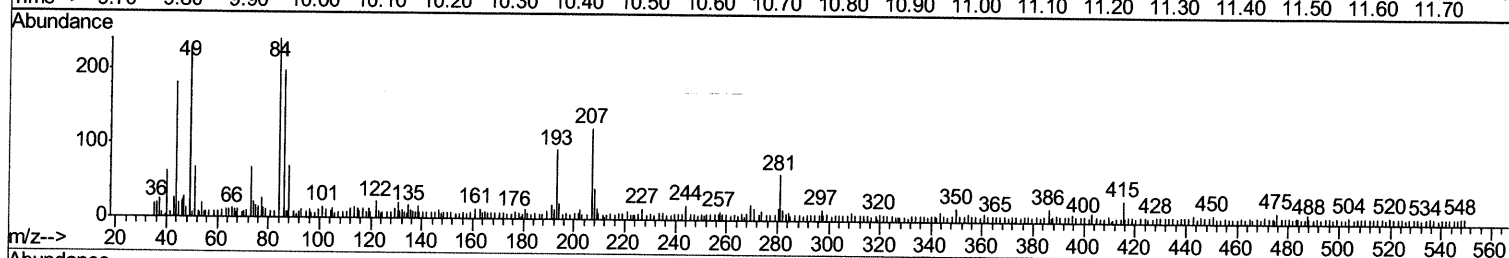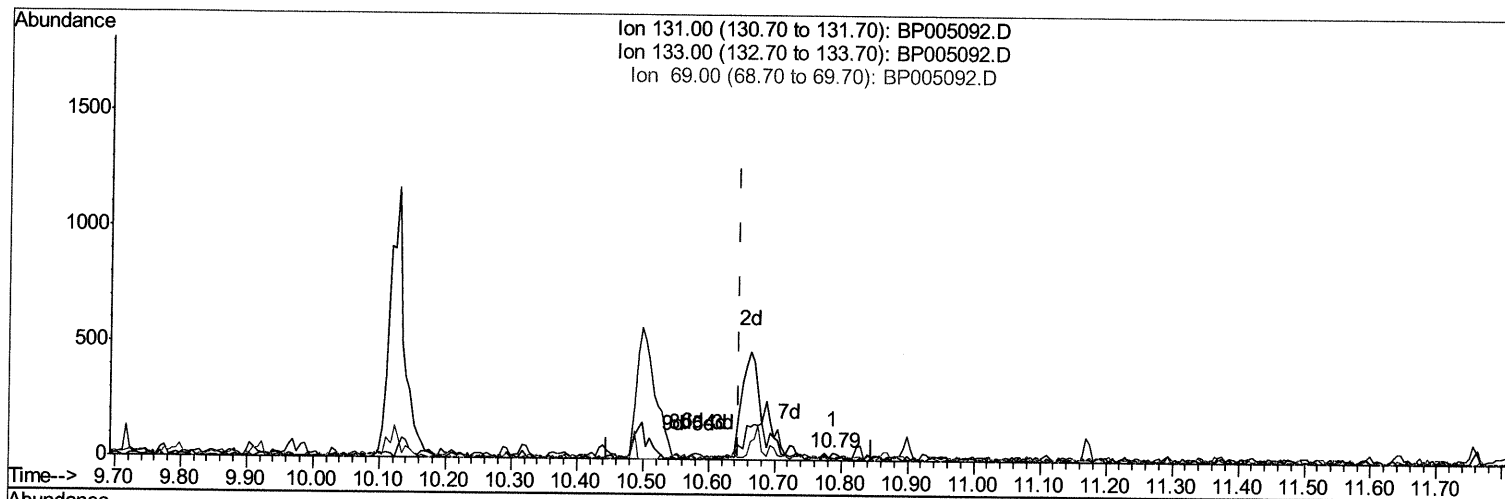

(29) 4-Chloroaniline-d4 (S)

10.787min (+0.141) 0.01ng/ul

response 29

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	28.13
69.00	21.50	21.88
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005092.D
 Acq On : 30 Mar 2021 01:18
 Operator : CG/JU
 Sample : M1818-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:07:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

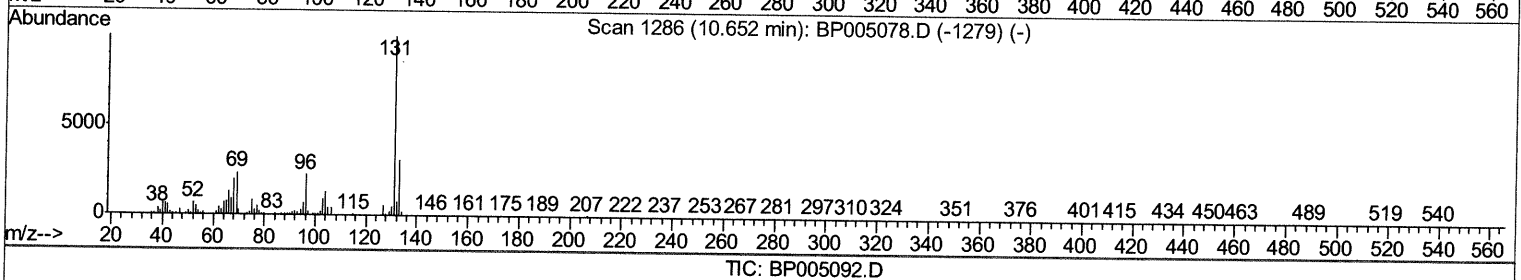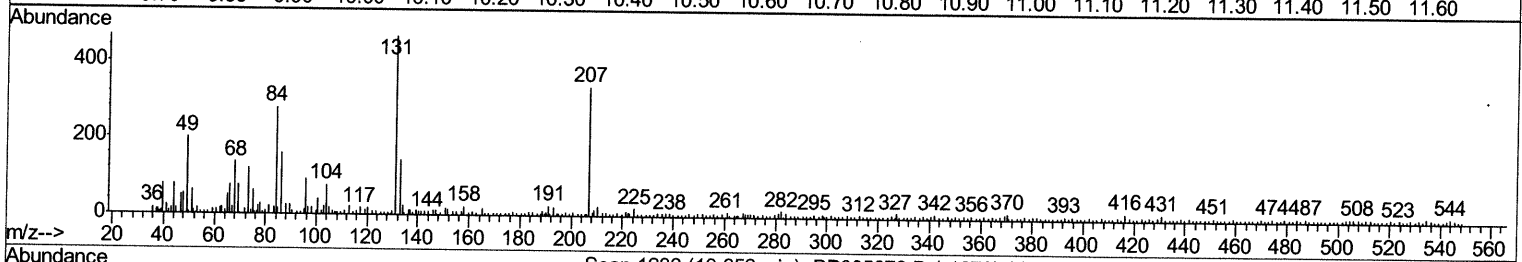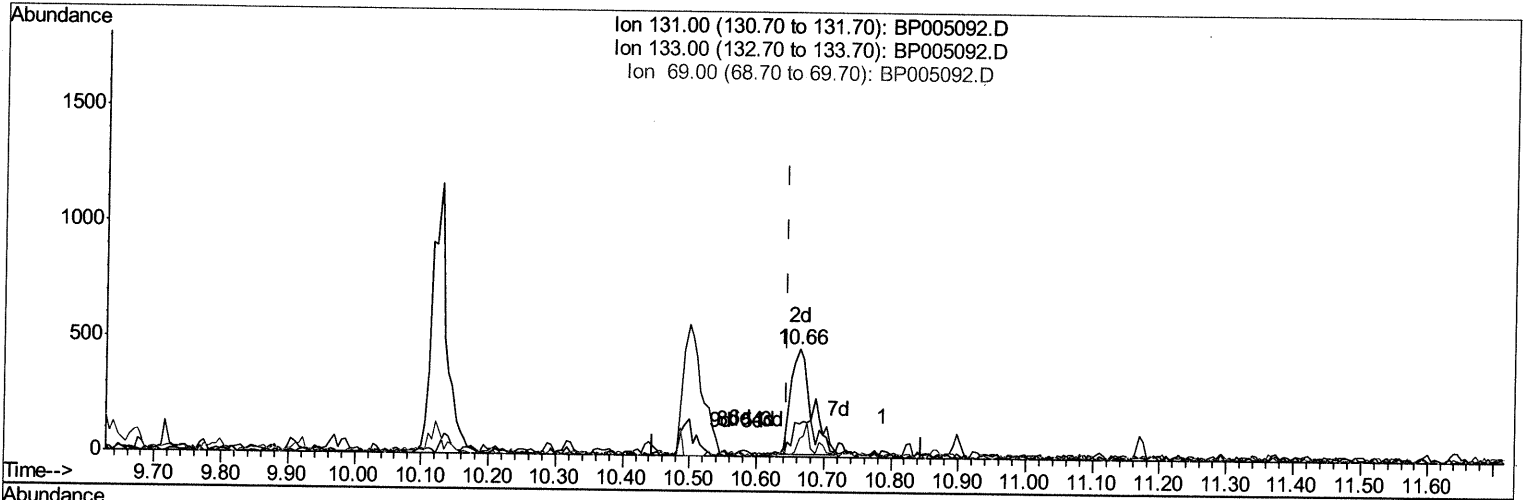

TIC: BP005092.D

(29) 4-Chloroaniline-d4 (S)

10.663min (+0.018) 0.50ng/ul m

04/01/2021

response 1004

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	31.12
69.00	21.50	16.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005092.D
Acq On : 30 Mar 2021 01:18
Operator : CG/JU
Sample : M1818-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
C0AA3

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:08:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

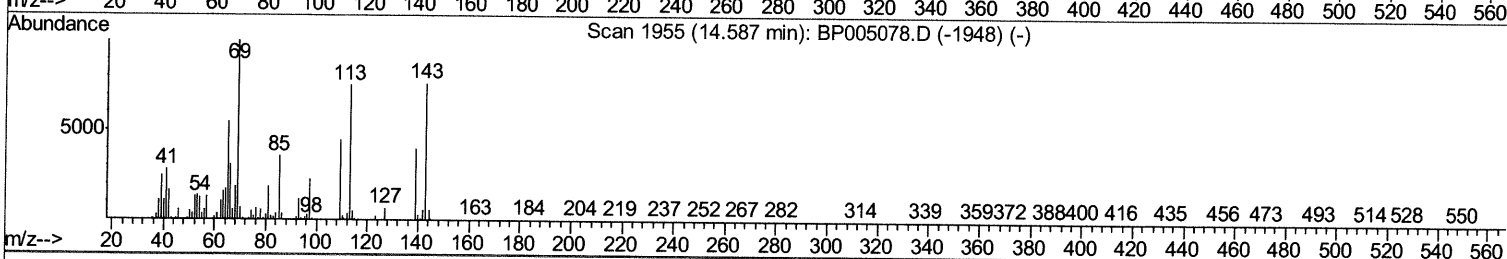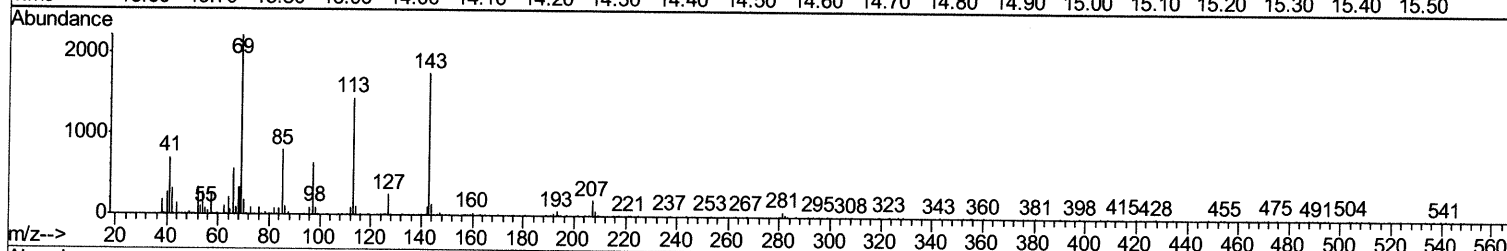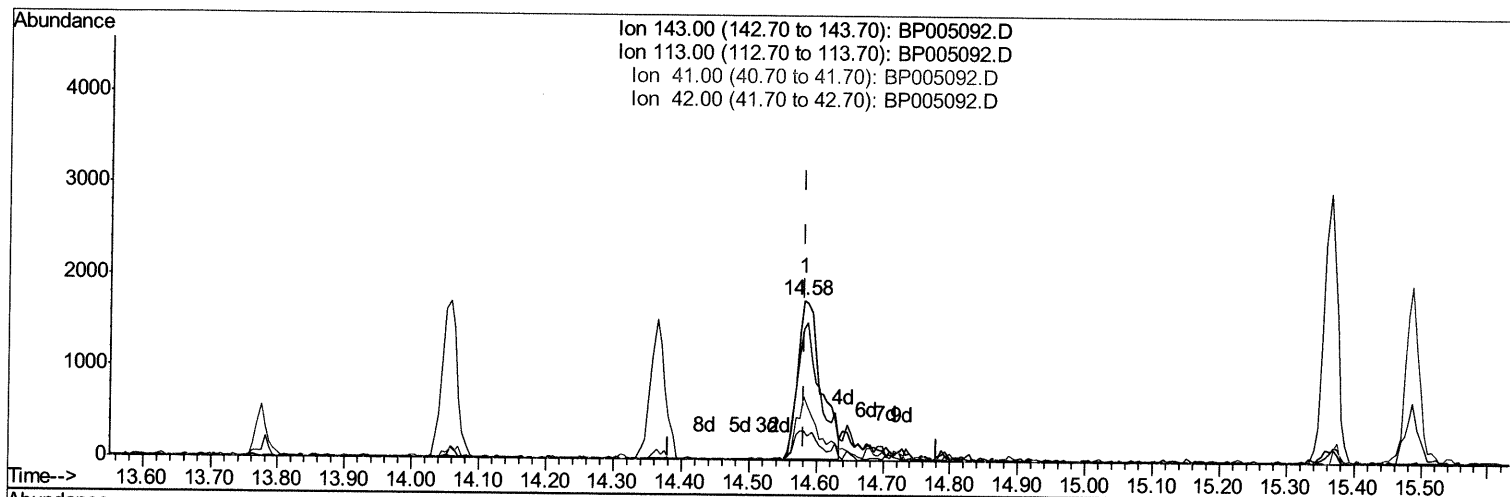

TIC: BP005092.D

(52) 4-Nitrophenol-d4 (S)

14.581min (+0.000) 4.73ng/ui

response 4256

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	82.34
41.00	27.10	40.00#
42.00	18.80	19.09

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005092.D
 Acq On : 30 Mar 2021 01:18
 Operator : CG/JU
 Sample : M1818-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:08:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

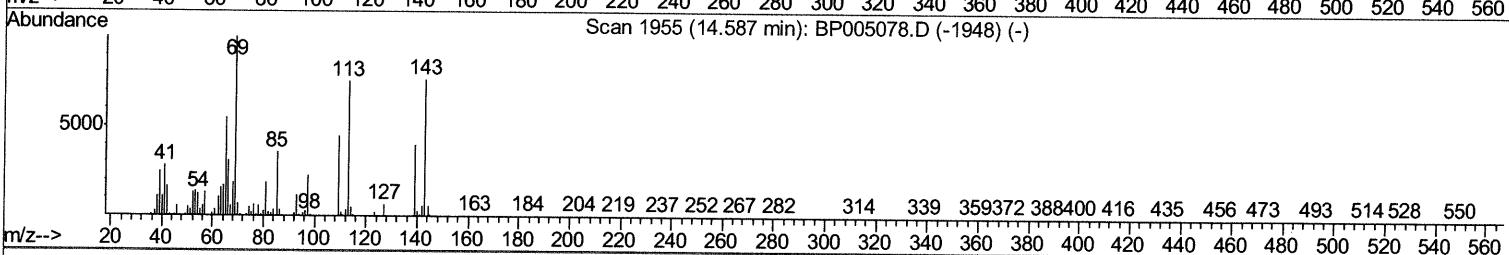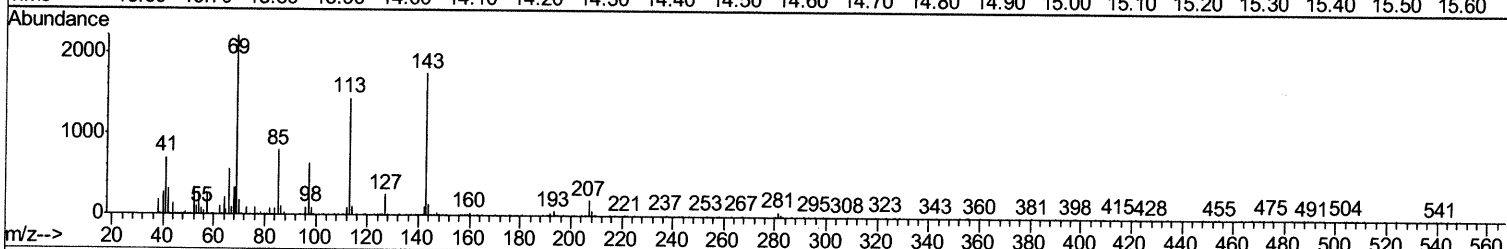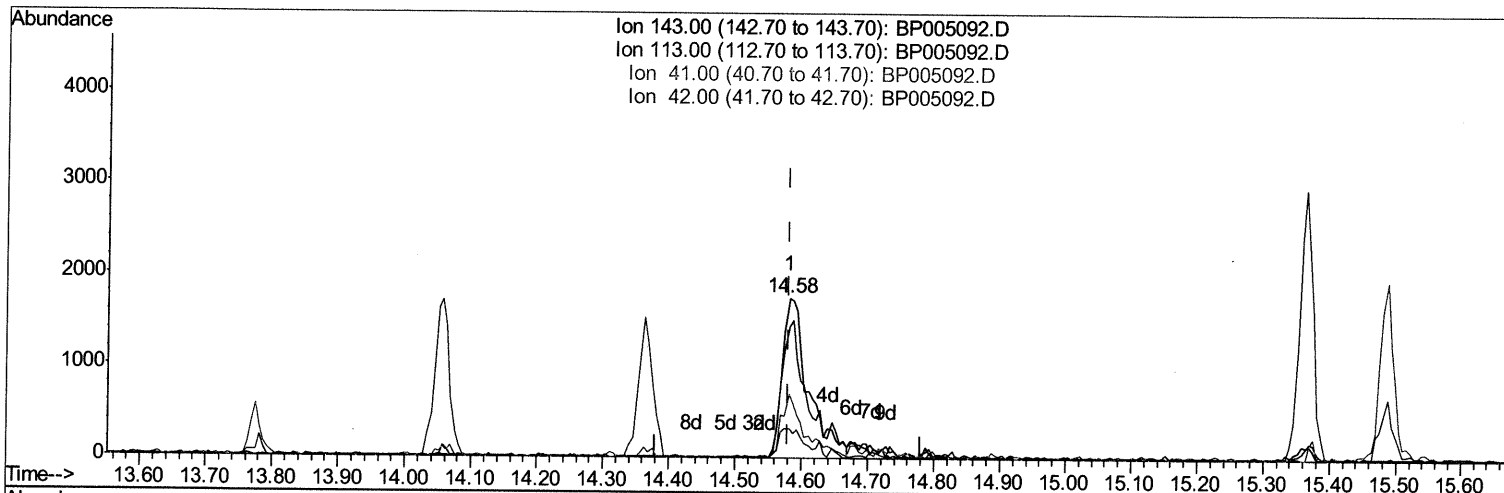

TIC: BP005092.D

(52) 4-Nitrophenol-d4 (S)

14.581min (+0.000) 5.25ng/ul m 04/01/21 JU

response 4722

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	82.34
41.00	27.10	40.00#
42.00	18.80	18.17

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032921\
 Data File : BP005092.D
 Acq On : 30 Mar 2021 01:18
 Operator : CG/JU
 Sample : M1818-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:46 PM

Quant Time: Mar 30 03:10:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	28153	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	115062	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	75915	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	164358	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	171602	20.00	ng/ul	-0.01
86) Perylene-d12	23.50	264	170253	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3230	4.33	ng/uL	0.00
5) Phenol-d5	6.89	99	14660	6.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	38607	30.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	40138	23.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	28041	15.14	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	25679	30.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	29095	30.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	47305	25.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	1004m >	0.50	ng/ul >	0.02 04/01/21 JU
44) Dimethylphthalate-d6	13.78	166	191572	34.75	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	218096	31.92	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	4722m >	5.25	ng/ul >	0.00 04/01/21 JU
58) Fluorene-d10	15.36	176	166764	34.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	37731	34.76	ng/ul	0.00
71) Anthracene-d10	17.22	188	296453	40.06	ng/ul	0.00
79) Pyrene-d10	19.47	212	339007	41.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	365557	41.80	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed