


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005093.D
Acq On : 30 Mar 2021 01:51
Operator : CG/JU
Sample : M1783-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0G07

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:39 PM

Quant Time: Mar 30 03:14:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

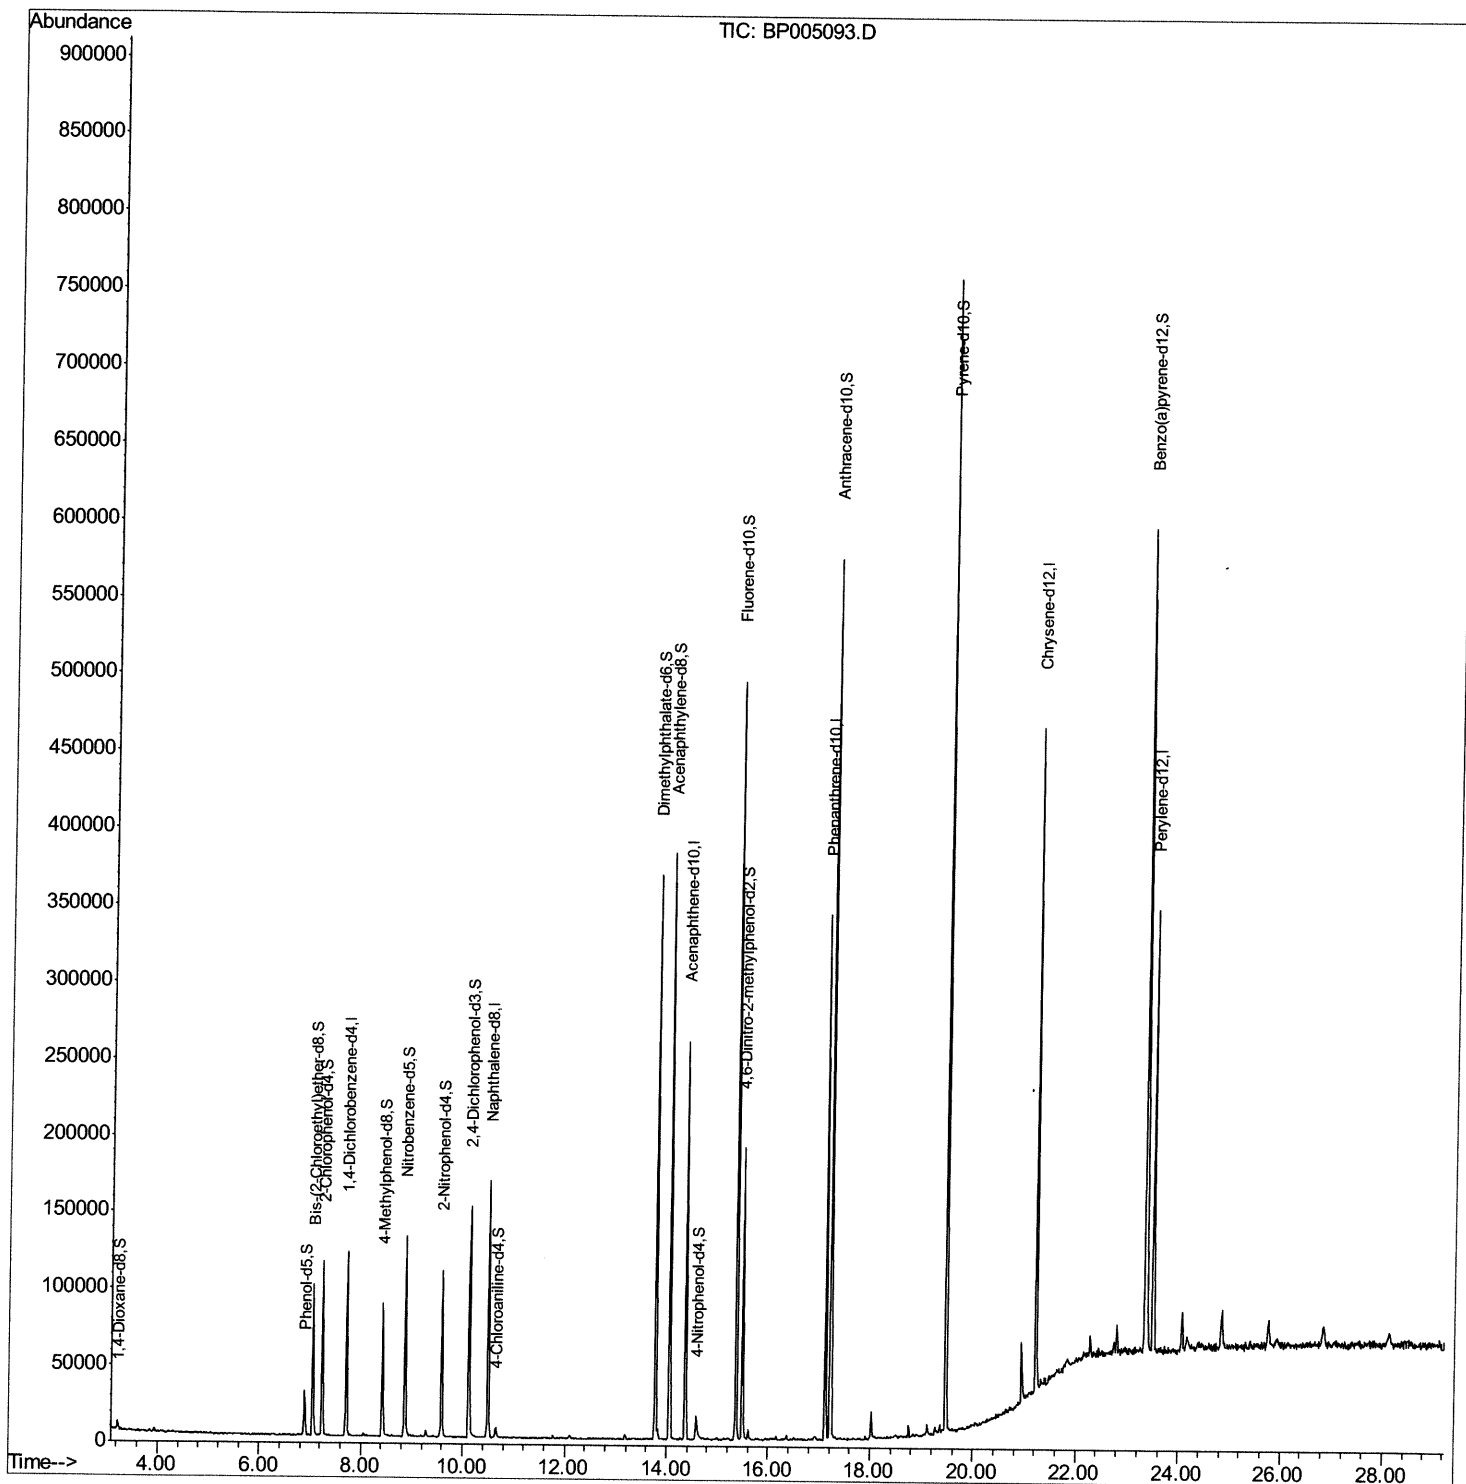

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
Data File : BP005093.D
Acq On : 30 Mar 2021 01:51
Operator : CG/JU
Sample : M1783-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0G07

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:39 PM

Quant Time: Mar 30 03:13:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

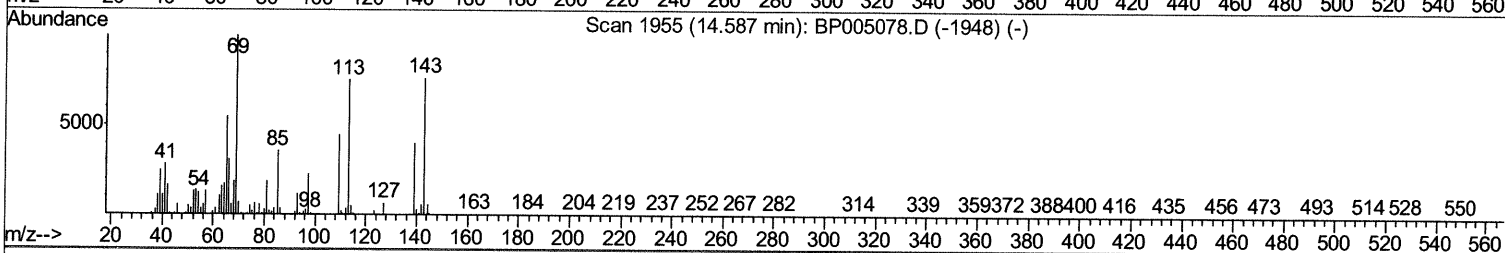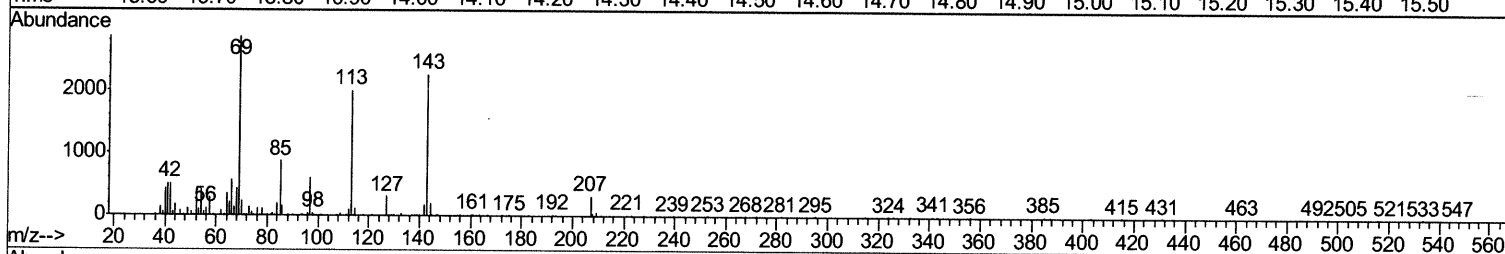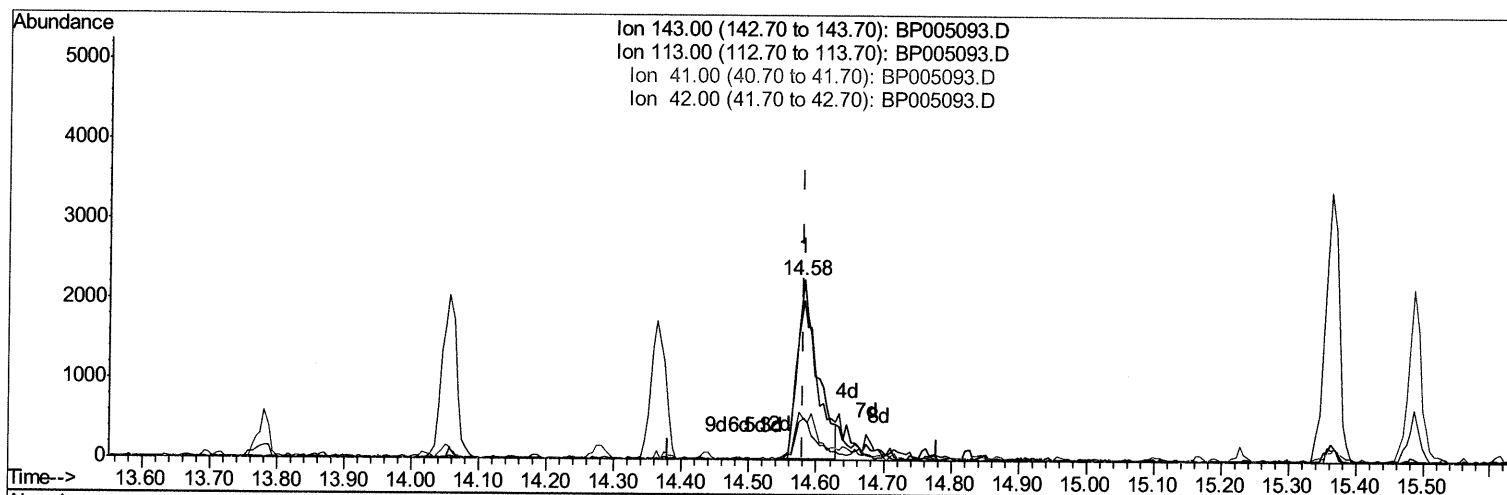

TIC: BP005093.D

(52) 4-Nitrophenol-d4 (S)

14.580min (-0.000) 4.55ng/ul

response 4590

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	88.73
41.00	27.10	22.73
42.00	18.80	23.04#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP032921\
 Data File : BP005093.D
 Acq On : 30 Mar 2021 01:51
 Operator : CG/JU
 Sample : M1783-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0G07

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:39 PM

Quant Time: Mar 30 03:13:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

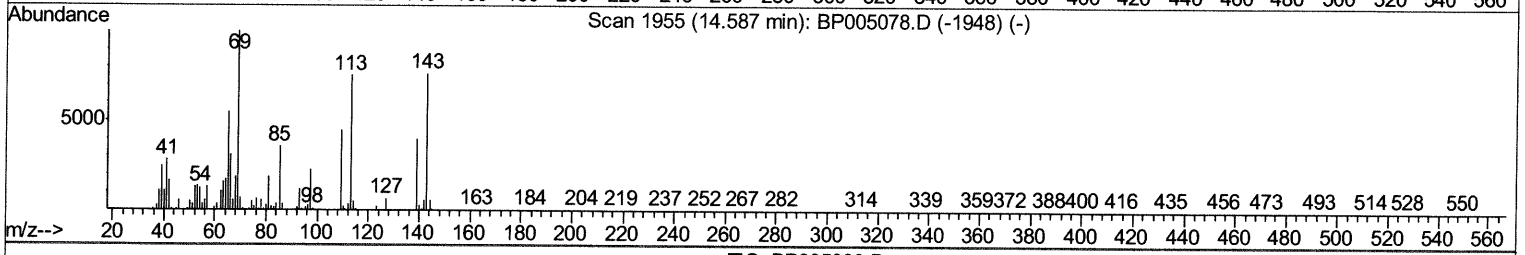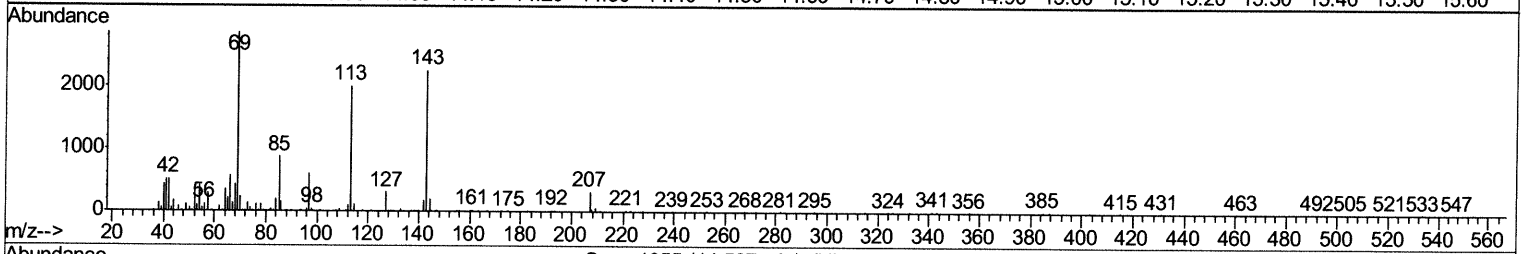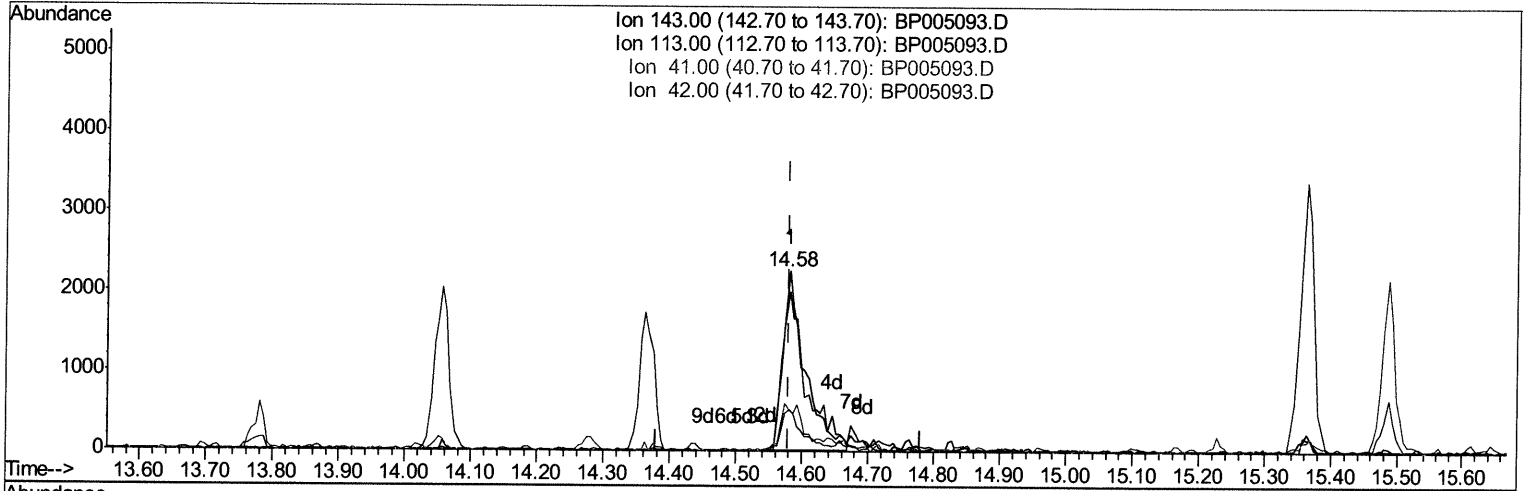

TIC: BP005093.D

(52) 4-Nitrophenol-d4 (S)

14.580min (-0.000) 5.19ng/ul m 04/01/20

response 5233

Ion	Exp%	Act%
143.00	100	100
113.00	81.90	88.73
41.00	27.10	22.73
42.00	18.80	23.04#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032921\
 Data File : BP005093.D
 Acq On : 30 Mar 2021 01:51
 Operator : CG/JU
 Sample : M1783-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0G07

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:39 PM

Quant Time: Mar 30 03:14:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	31074	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	127236	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	84990	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	189974	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	202223	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	201374	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3669	4.46	ng/uL	0.00
5) Phenol-d5	6.89	99	17037	6.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	42755	30.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	44956	23.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	29801	14.58	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	28216	30.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	31588	30.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	53641	26.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	3672	1.65	ng/ul	0.01
44) Dimethylphthalate-d6	13.78	166	216032	35.01	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	248434	32.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	5233m>	5.19	ng/ul >	0.00
58) Fluorene-d10	15.36	176	185306	34.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	38708	30.85	ng/ul	0.00
71) Anthracene-d10	17.23	188	319761	37.39	ng/ul	0.00
79) Pyrene-d10	19.47	212	361502	37.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	398983	38.57	ng/ul	0.00

04/01/2021

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed