

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP032921\
 Data File : BP005087.D
 Acq On : 29 Mar 2021 22:28
 Operator : CG/JU
 Sample : M1818-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:30 PM

Quant Time: Mar 30 02:10:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 30 00:27:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	30106	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	122081	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	82591	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	185101	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	194416	20.00	ng/ul	0.00
86) Perylene-d12	23.50	264	197928	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3650	4.58	ng/uL	0.00
5) Phenol-d5	6.89	99	16040	6.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	40114	29.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	43626	23.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	29333	14.81	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	27341	30.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	31915	32.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	50605	26.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	4184m	1.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	201344	33.57	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	236198	31.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	5303m	5.41	ng/ul	0.00
58) Fluorene-d10	15.36	176	177232	34.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	40471	33.10	ng/ul	0.00
71) Anthracene-d10	17.23	188	314461	37.74	ng/ul	0.00
79) Pyrene-d10	19.47	212	353941	38.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.36	264	392448	38.60	ng/ul	0.00

Target Compounds				Ovalue	
45) Dimethylphthalate	13.83	163	10248	1.671	ng/ul# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP032921\
Data File : BP005087.D
Acq On : 29 Mar 2021 22:28
Operator : CG/JU
Sample : M1818-02
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Time: Mar 30 02:10:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP032921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 30 00:27:26 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
3/30/2021 4:12:30 PM

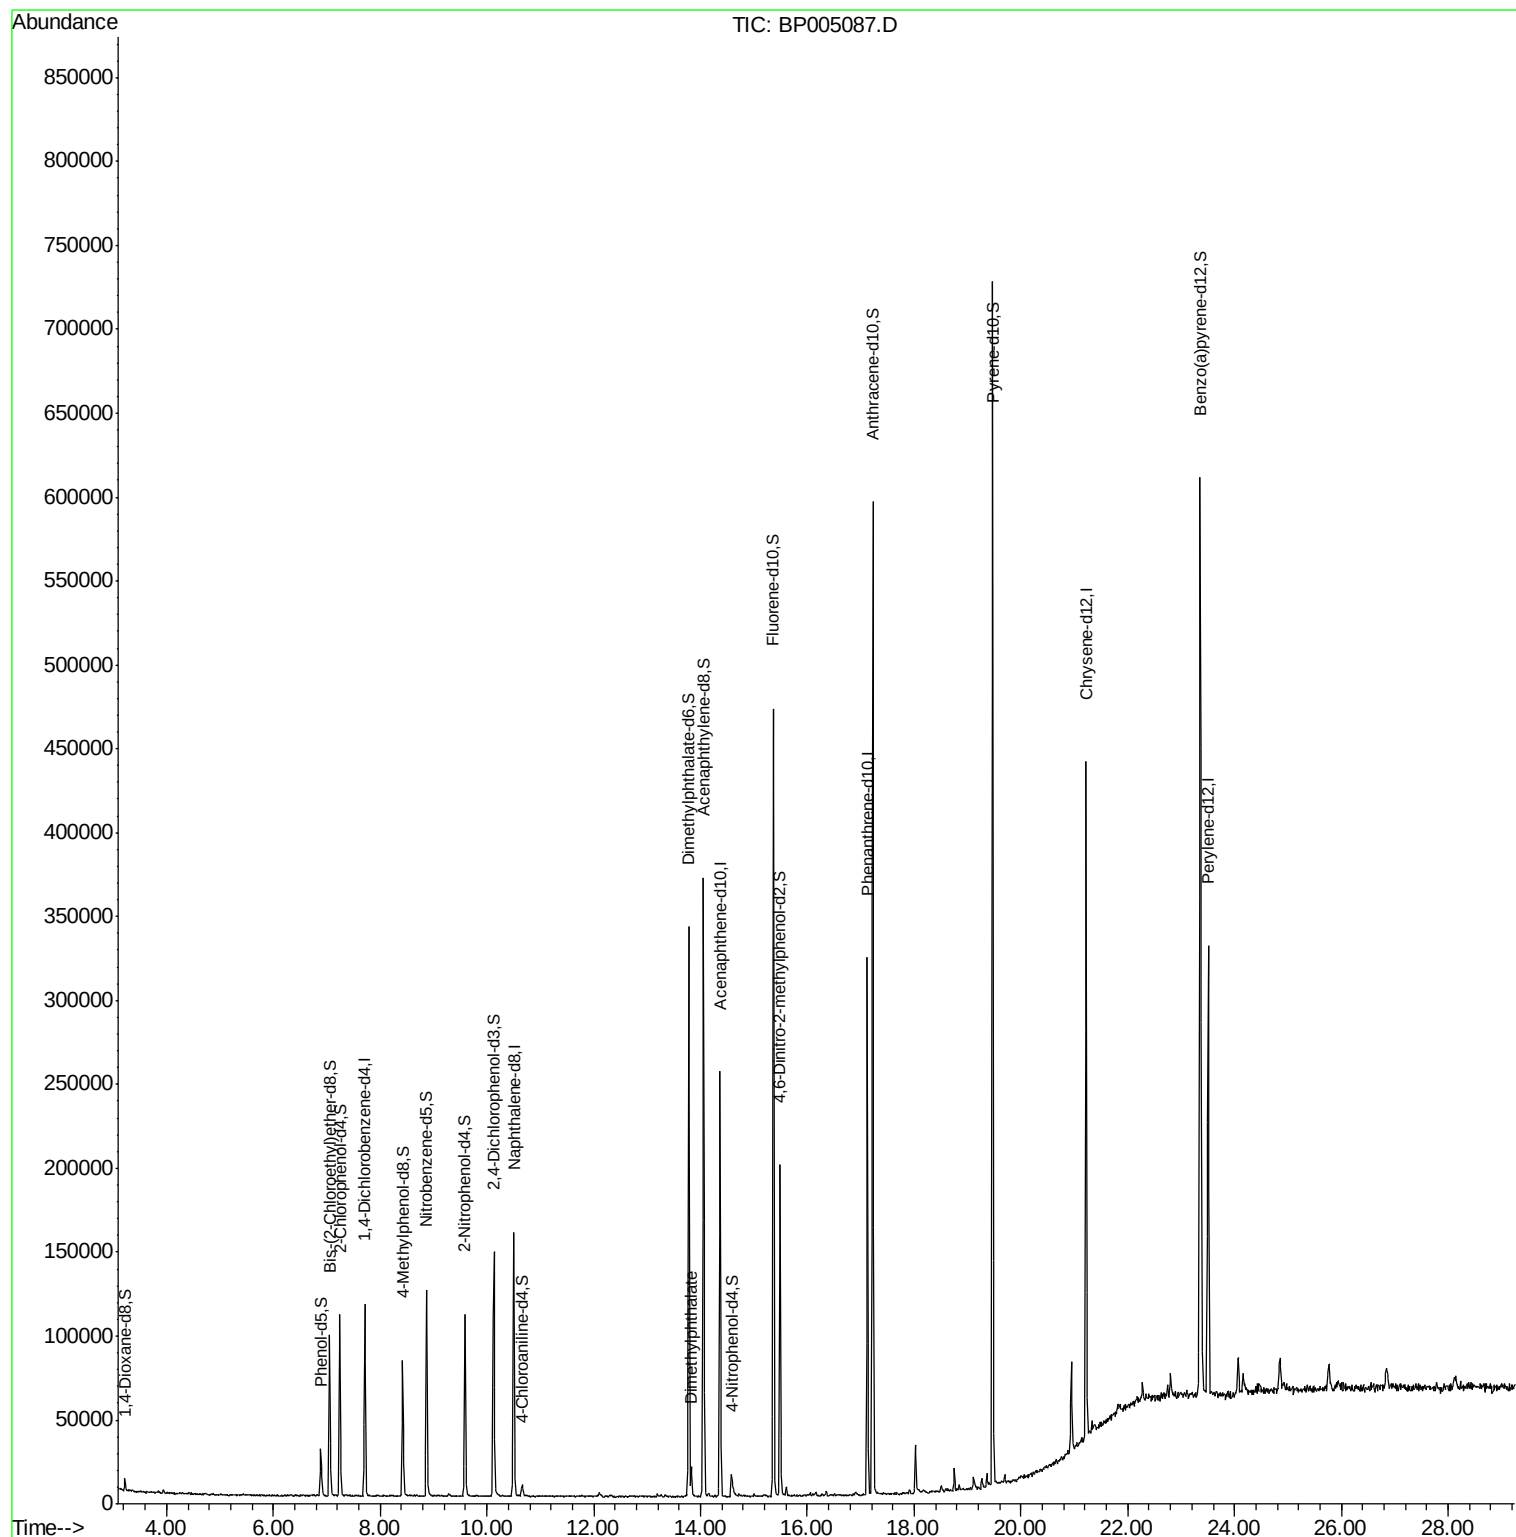

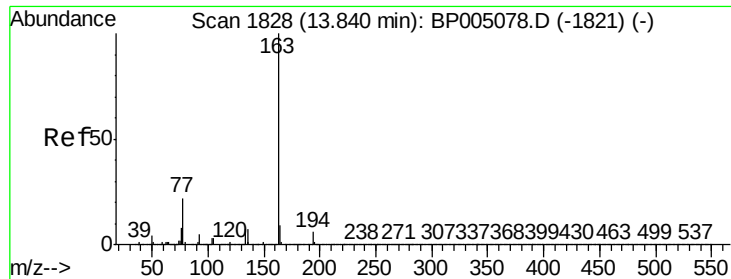

#45
 Dimethylphthalate
 Concen: 1.671 ng/ul
 RT: 13.83 min Scan# 1826
 Delta R.T. 0.00 min
 Lab File: BP005087.D
 Acq: 29 Mar 2021 22:28

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.0	3.4	5.2#
164	8.4	8.6	13.0#

Manual Integrations
 APPROVED

mohammad
 3/30/2021 4:12:30 PM

