
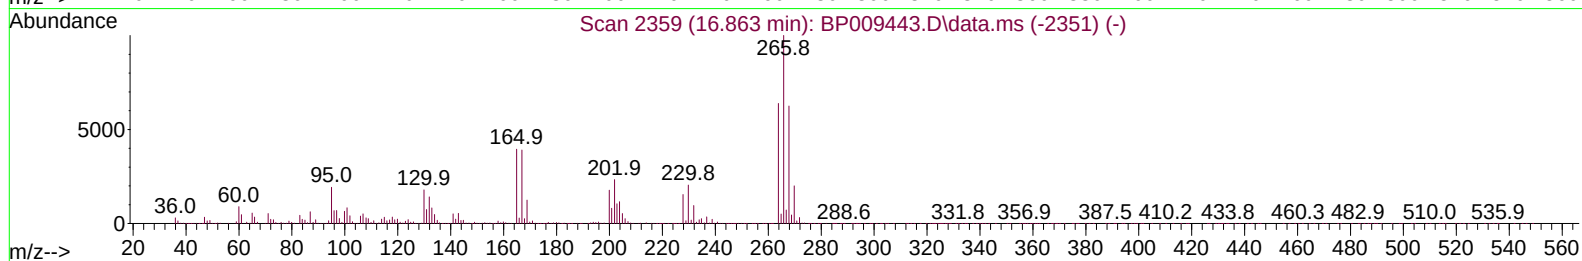
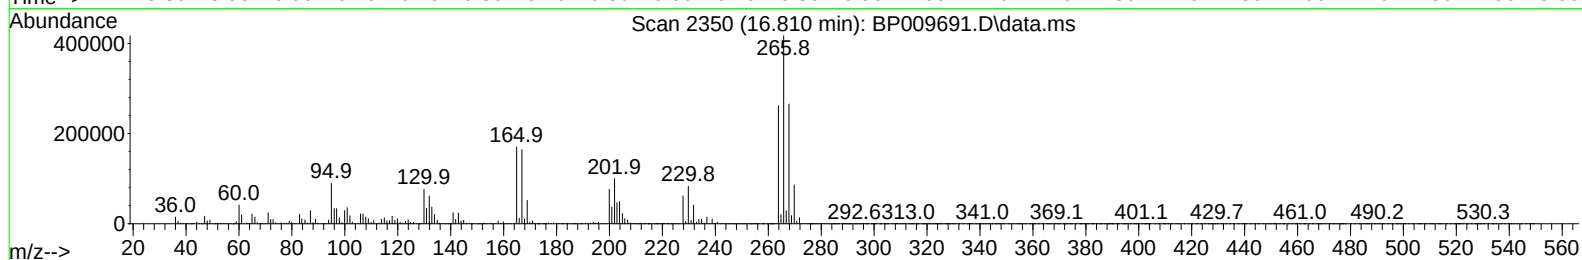


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040522\
Data File : BP009691.D
Acq On : 05 Apr 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 13:52:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 13:35:48 2022
Response via : Initial Calibration

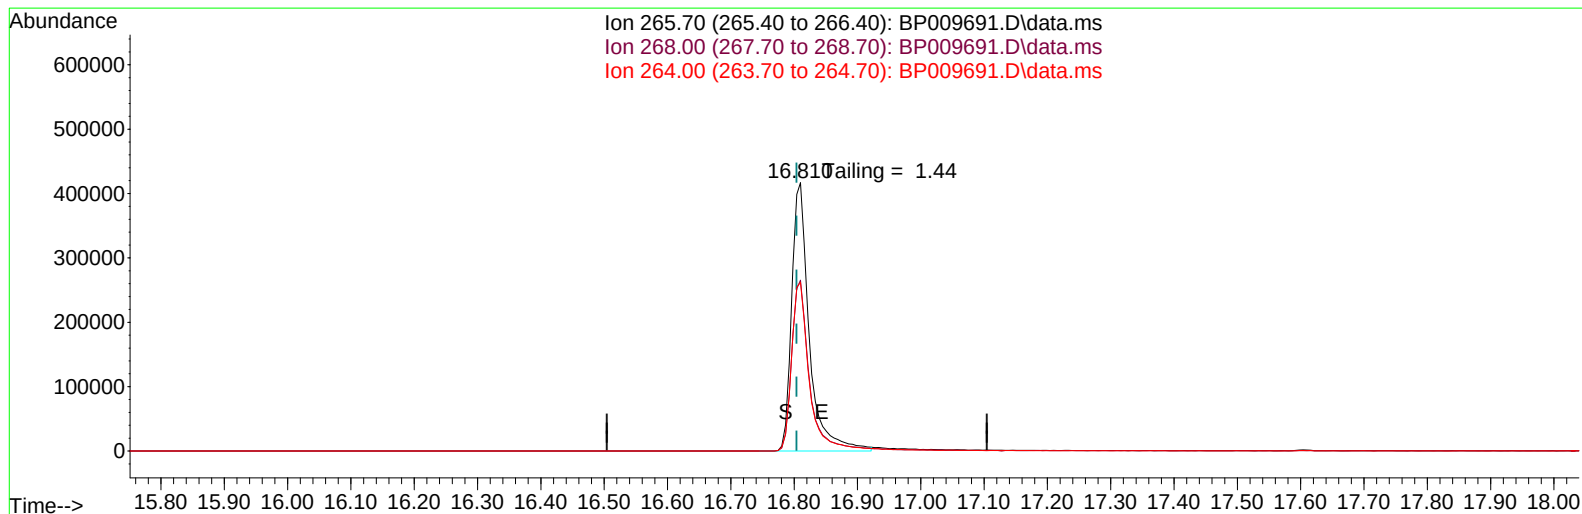

TIC: BP009691.D\data.ms

(70) Pentachlorophenol (C)




16.810min (+ 0.006) 3146179.02 ng

response 828980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.68
264.00	63.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040522\
 Data File : BP009691.D
 Acq On : 05 Apr 2022 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 13:52:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 13:35:48 2022
 Response via : Initial Calibration

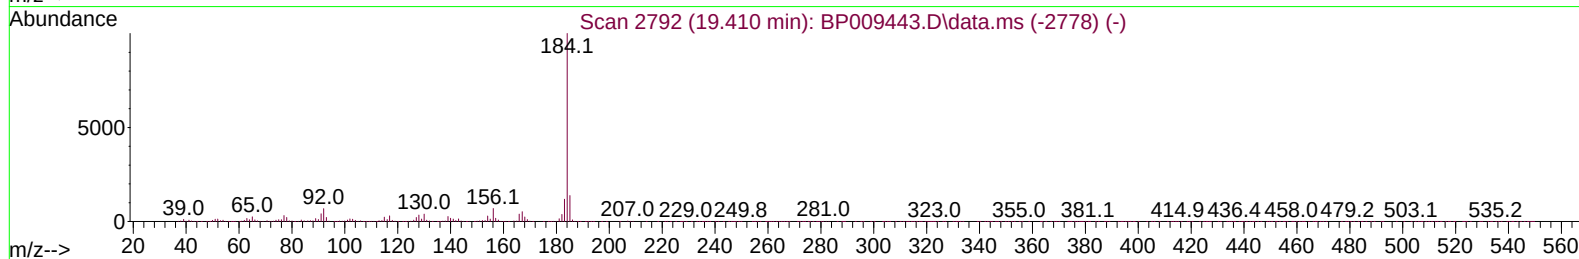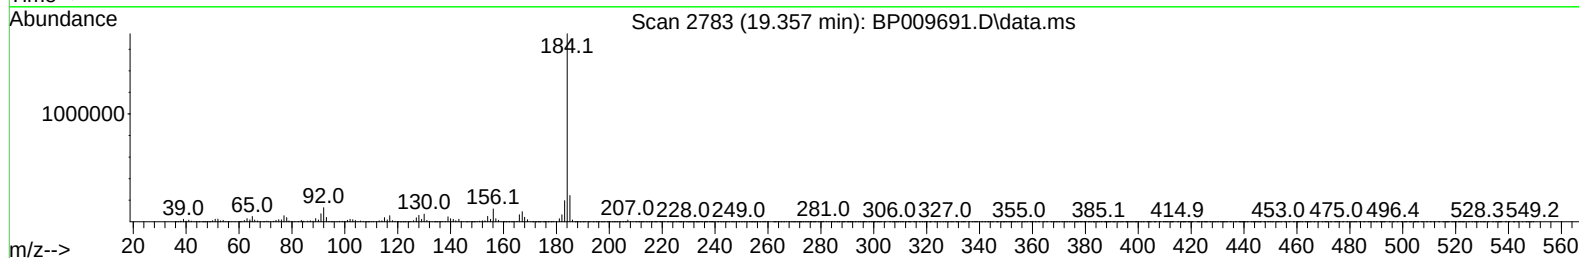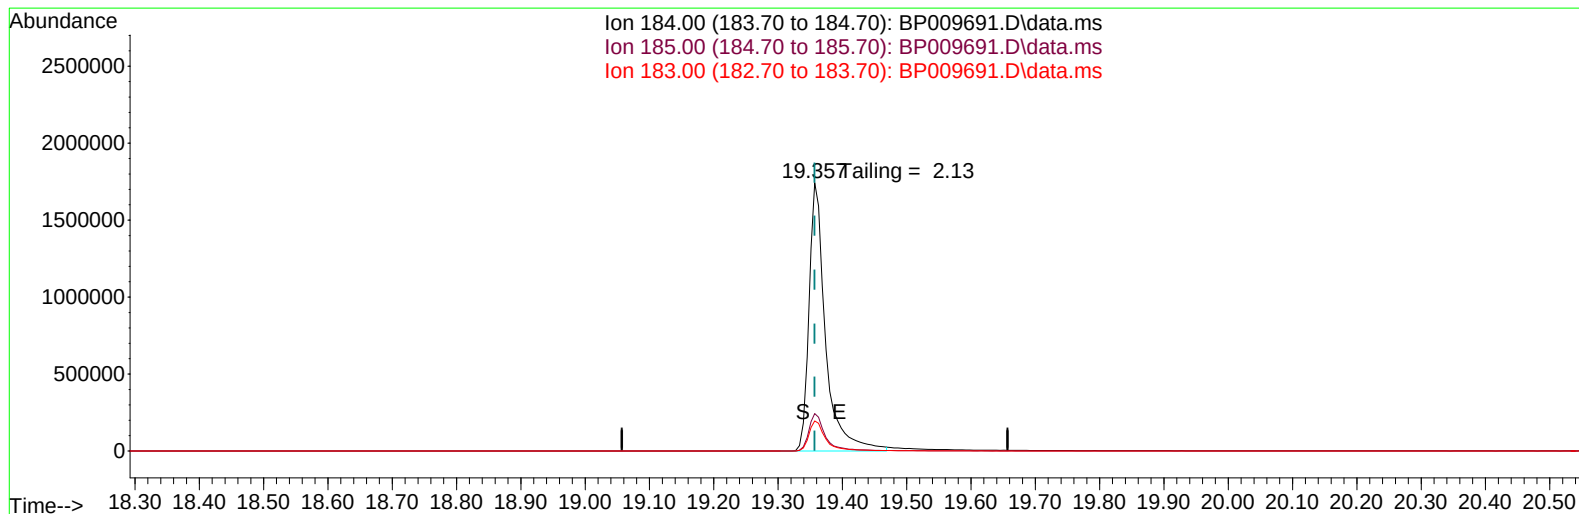

TIC: BP009691.D\data.ms

(77) Benzidine**19.357min (-0.000) 1177044.31 ng****response 3202451**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.95
183.00	11.70	11.25
0.00	0.00	0.00