
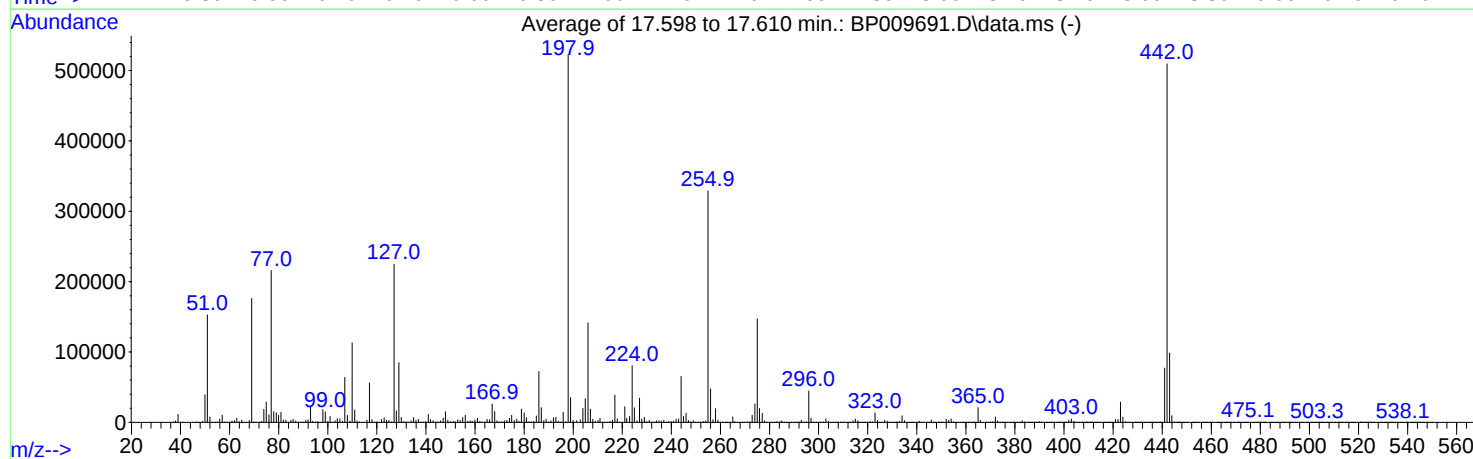


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040522\
 Data File : BP009691.D
 Acq On : 05 Apr 2022 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 05 13:35:48 2022

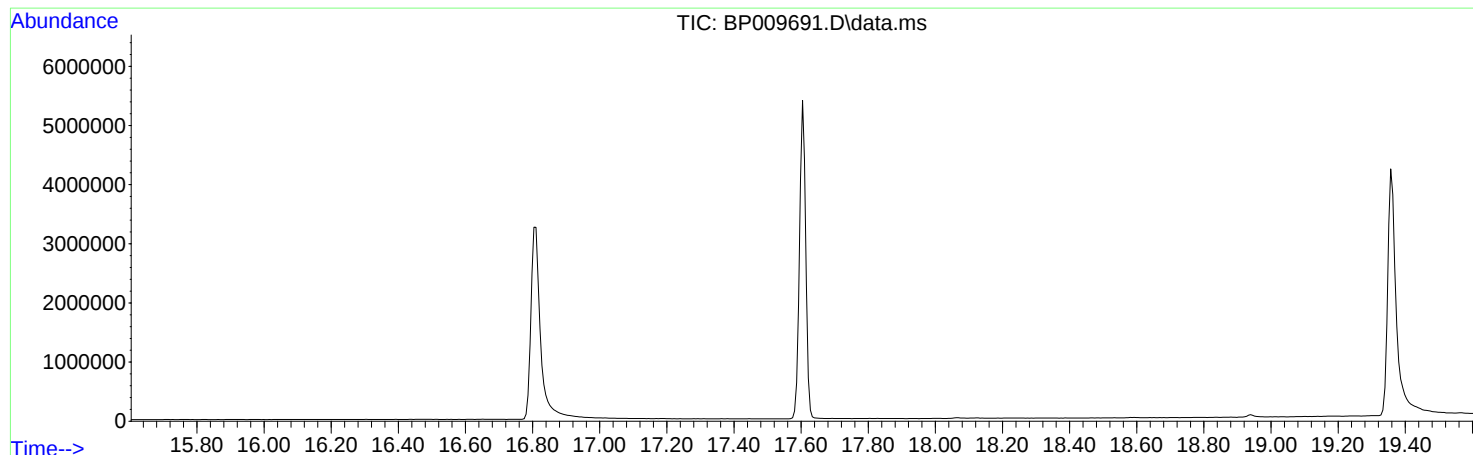




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	152833	PASS
68	69	0.00	2	1.6	2746	PASS
69	198	0.00	100	33.7	176327	PASS
70	69	0.00	2	0.6	976	PASS
127	198	10	80	43.0	225037	PASS
197	198	0.00	2	0.2	839	PASS
198	198	100	100	100.0	522859	PASS
199	198	5	9	6.7	35194	PASS
275	198	10	60	28.1	147041	PASS
365	198	1	100	4.0	21015	PASS
441	198	0.01	100	14.7	76995	PASS
442	442	100	100	100.0	509440	PASS
443	442	15	24	19.3	98423	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040522\
Data File : BP009691.D
Acq On : 05 Apr 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 05 13:52:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 13:35:48 2022
Response via : Initial Calibration

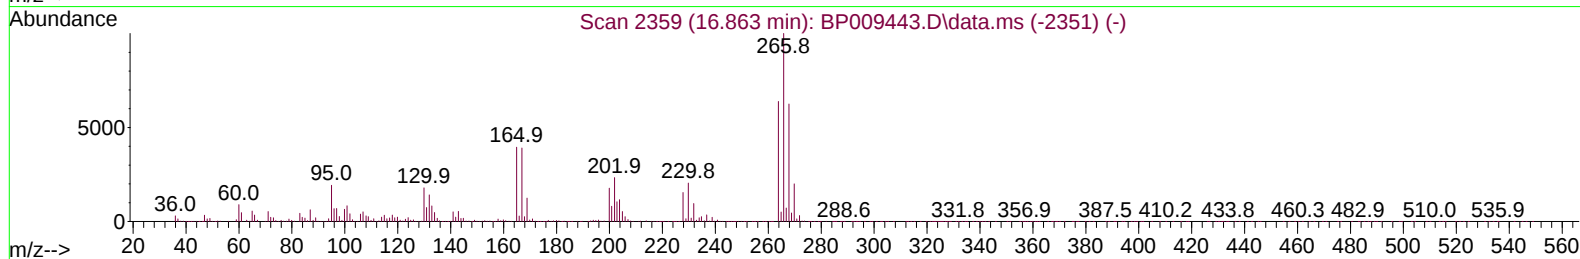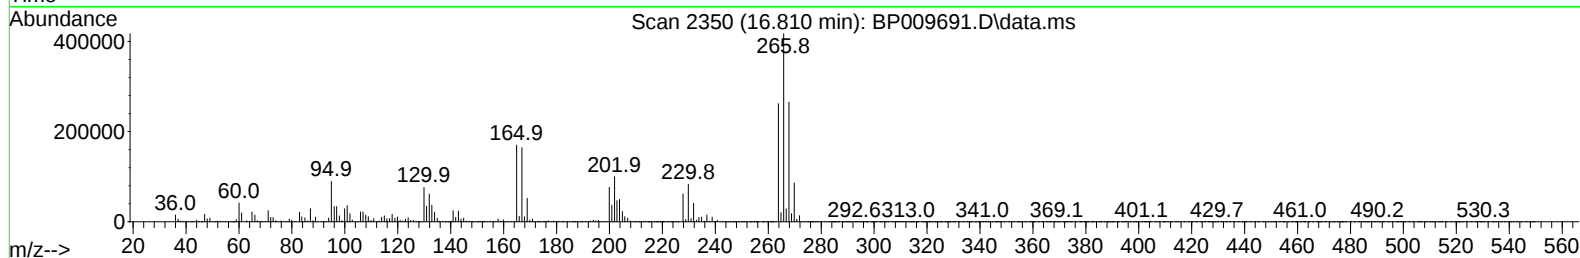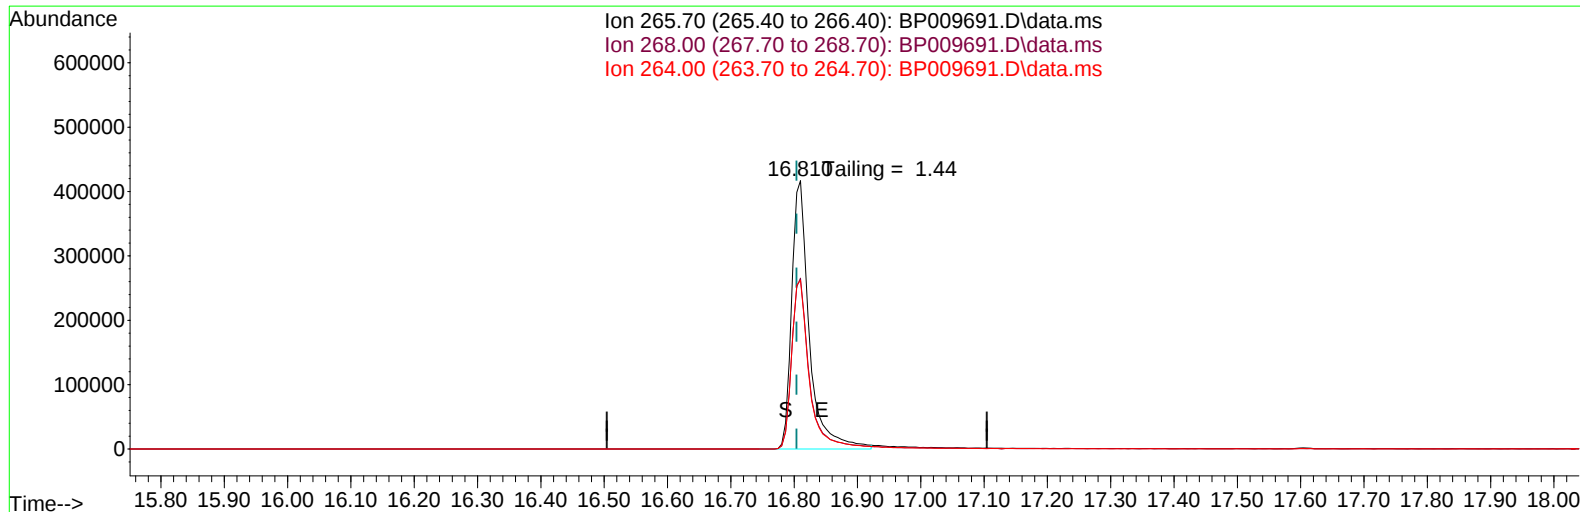

TIC: BP009691.D\data.ms

(70) Pentachlorophenol (C)

16.810min (+ 0.006) 3146179.02 ng




response 828980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.68
264.00	63.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040522\
 Data File : BP009691.D
 Acq On : 05 Apr 2022 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 13:52:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 13:35:48 2022
 Response via : Initial Calibration

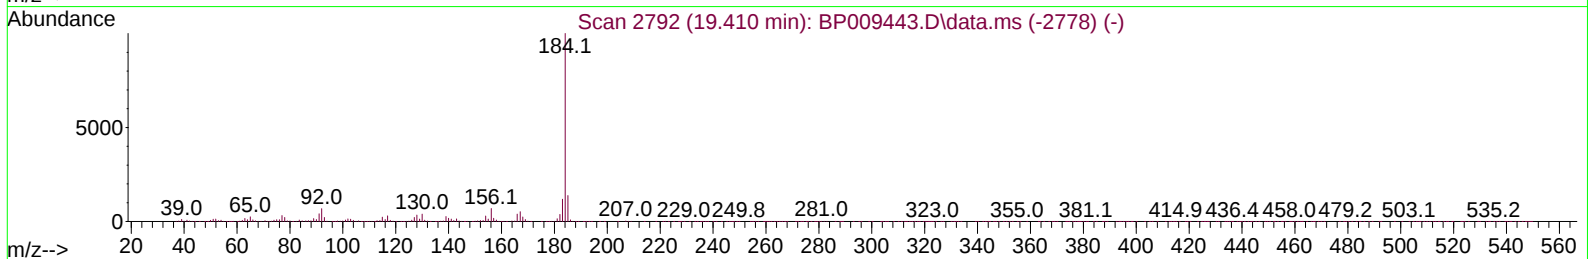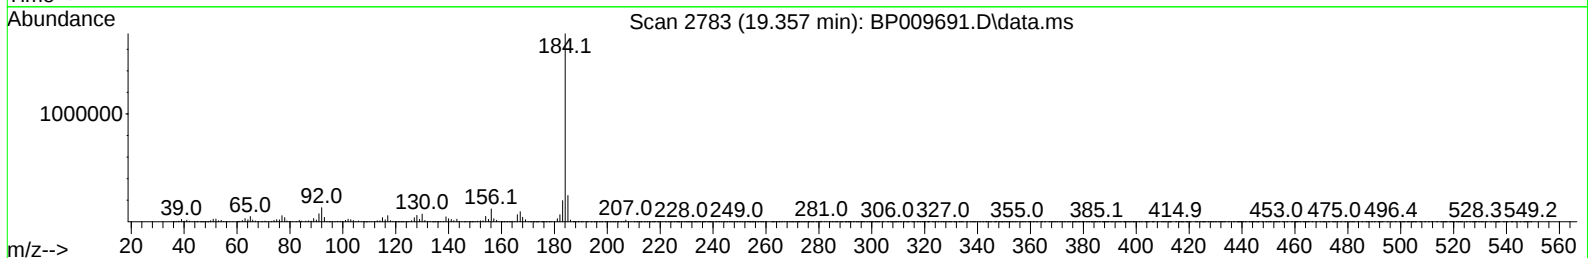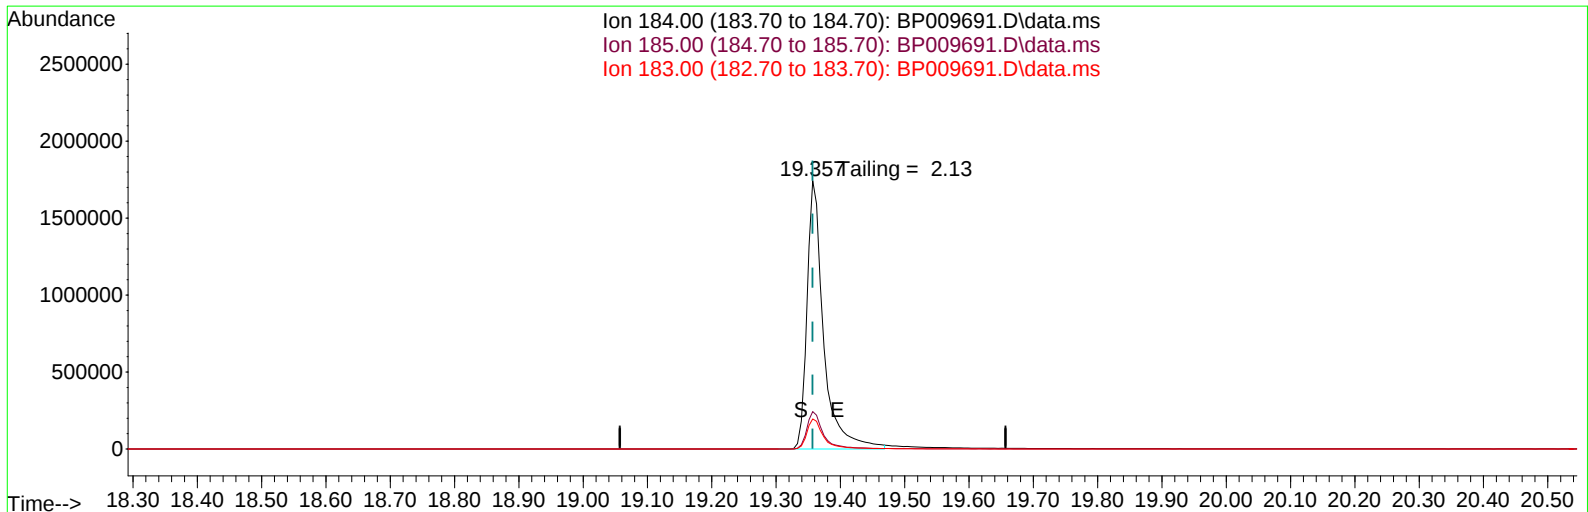

TIC: BP009691.D\data.ms

(77) Benzidine

19.357min (-0.000) 1177044.31 ng

response 3202451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.95
183.00	11.70	11.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2022	BNA_P	<u>BP009691.D</u>
Compound Name	Response	Retention Time
DDT	1573916	20.56
DDD	24628	20.13
DDE	3268	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27896	1601812	1.74

Instrument :
BNA_P
ClientSampleId :
DFTPP