




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014613.D
Acq On : 07 Apr 2023 20:06
Operator : CG/JU
Sample : 02225-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/10/2023
Supervised By :Jagrut Upadhyay 04/10/2023

Quant Time: Apr 08 01:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

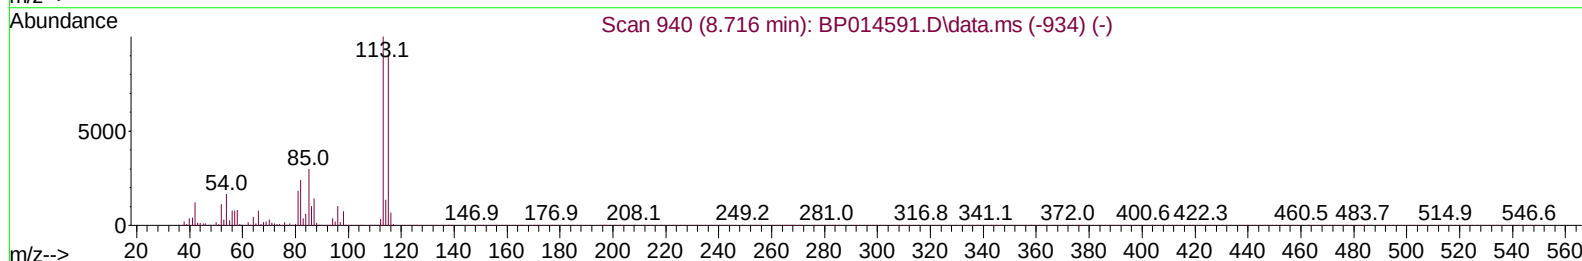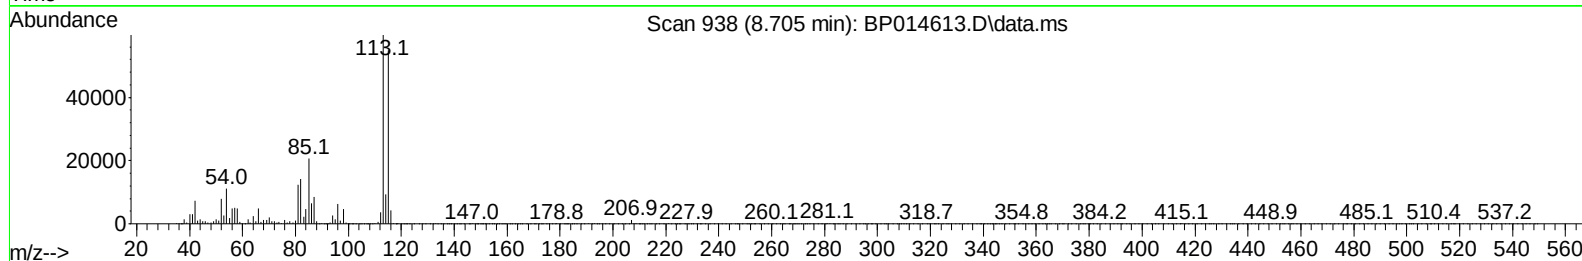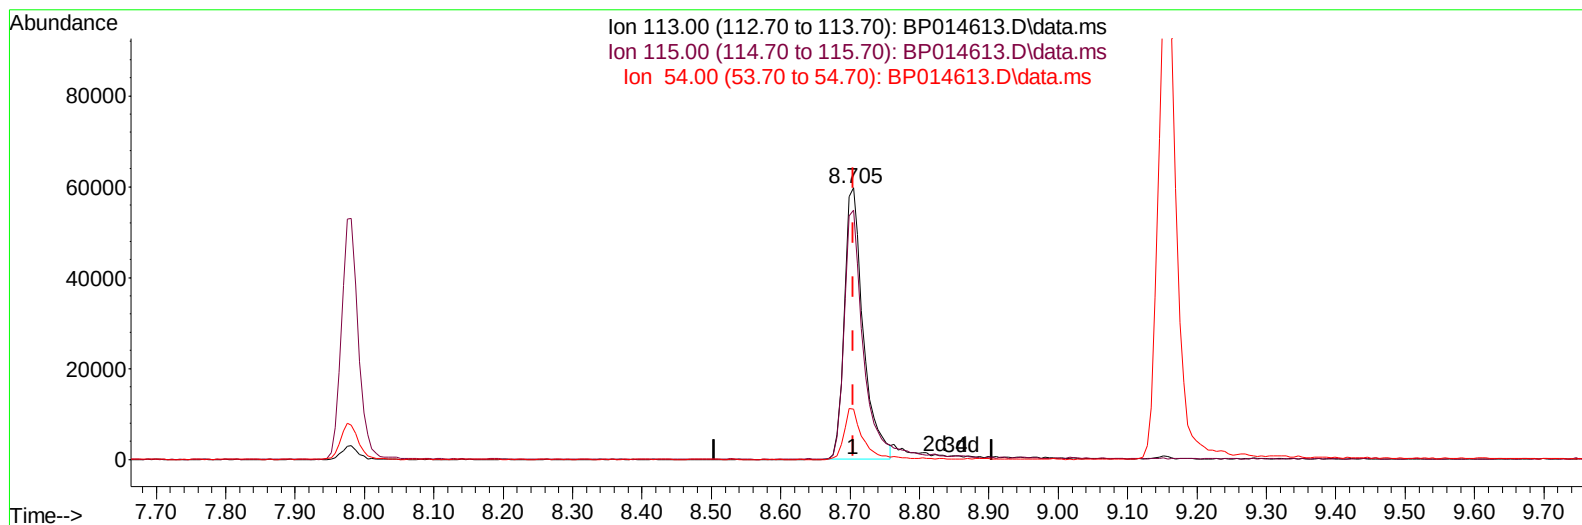

TIC: BP014613.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.705min (+ 0.000) 11.58 ng/u1

response 113355

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	91.90
54.00	15.10	18.58#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014613.D
 Acq On : 07 Apr 2023 20:06
 Operator : CG/JU
 Sample : 02225-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:50:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/10/2023
 Supervised By :Jagrut Upadhyay 04/10/2023

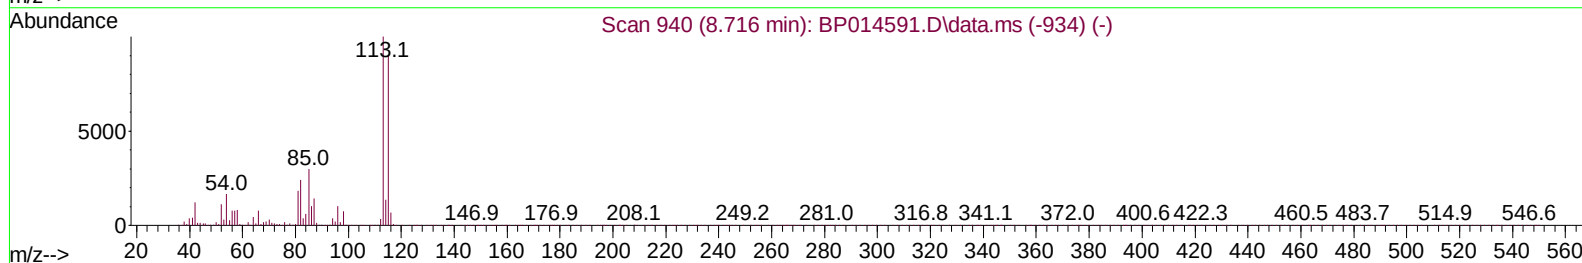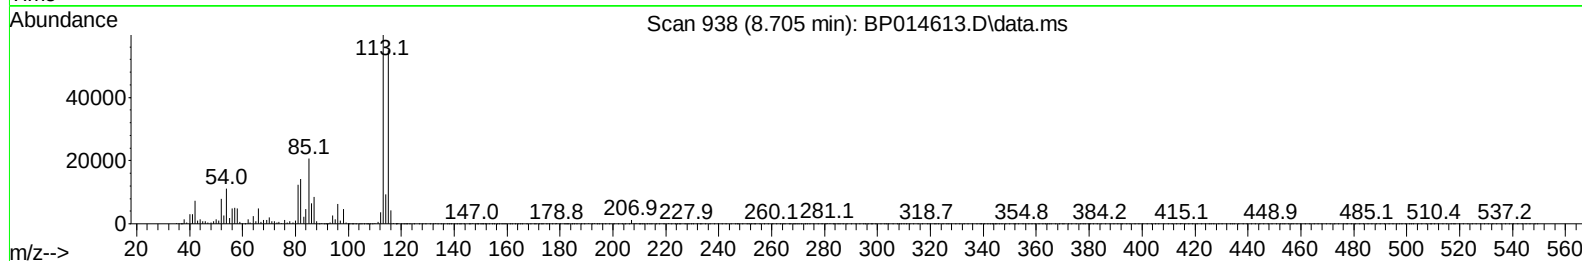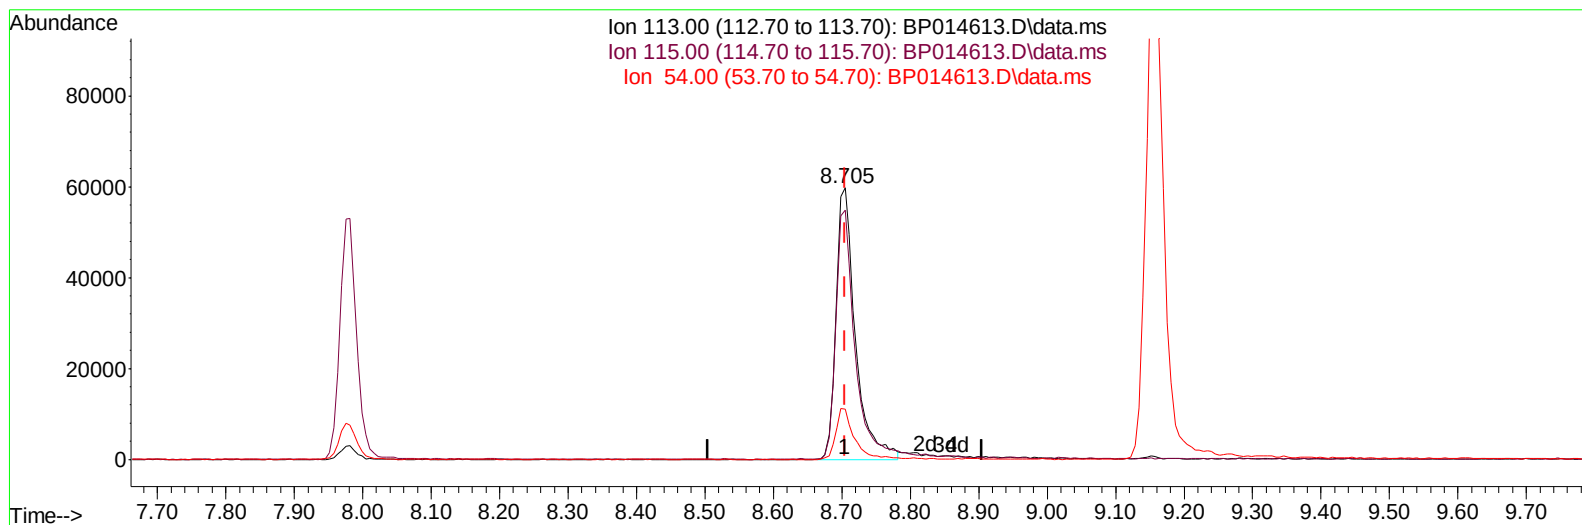

TIC: BP014613.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.705min (+ 0.000) 11.98 ng/ul m

response 117219

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	91.90
54.00	15.10	18.58#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014613.D
 Acq On : 07 Apr 2023 20:06
 Operator : CG/JU
 Sample : 02225-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:50:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/10/2023
 Supervised By :Jagrut Upadhyay 04/10/2023

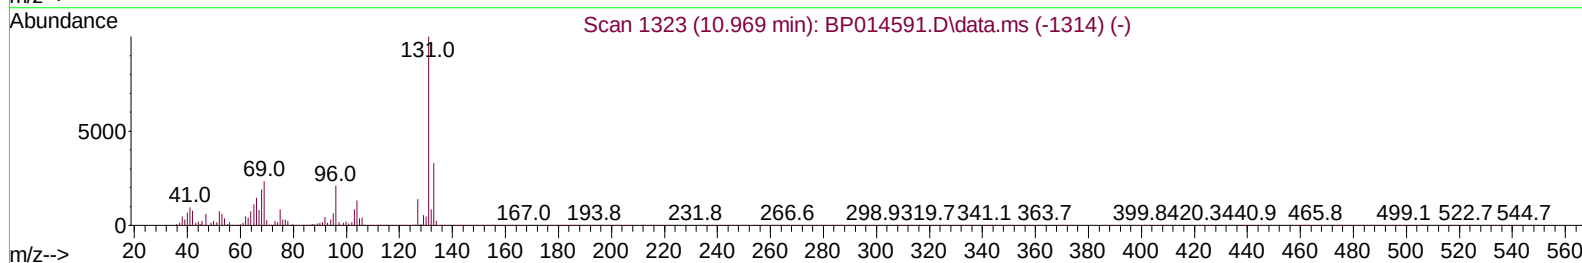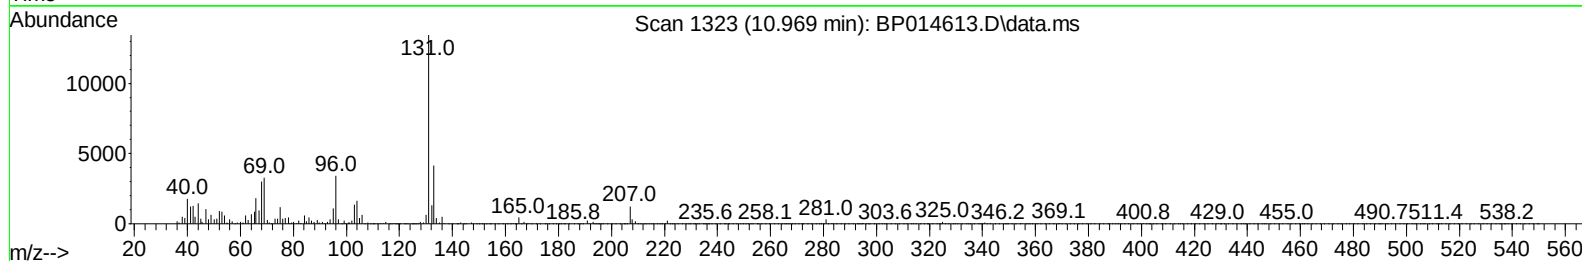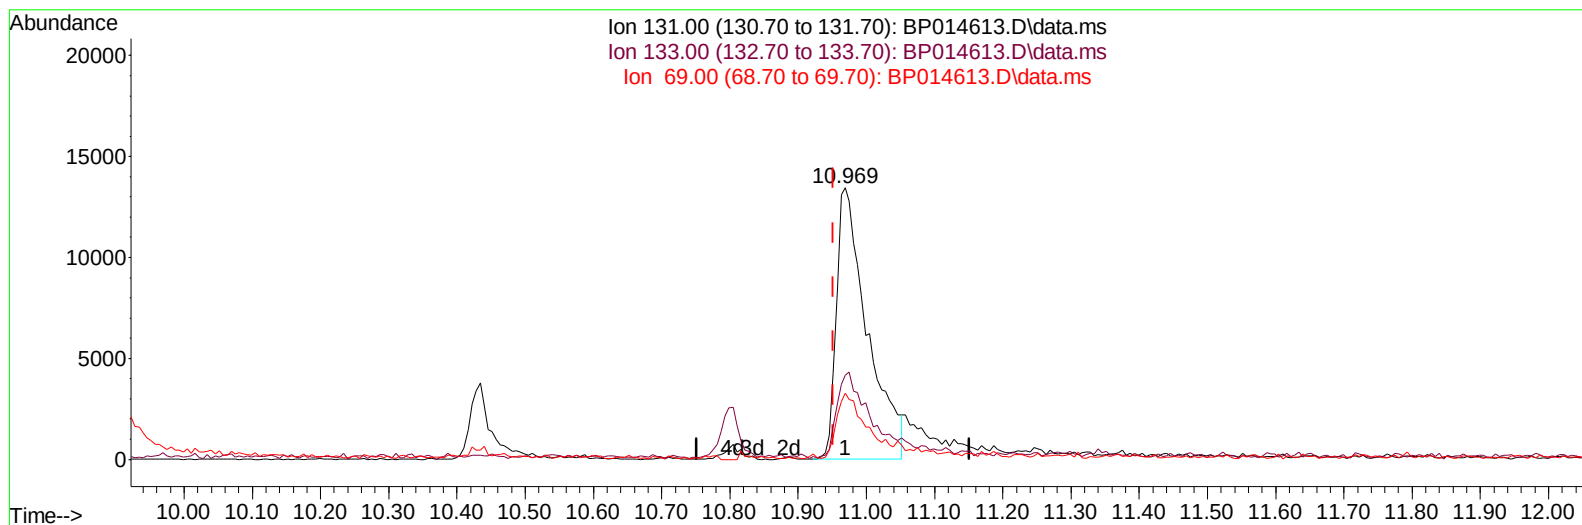

TIC: BP014613.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.018) 3.38 ng/ul

response 42370

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.91
69.00	21.30	24.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014613.D
 Acq On : 07 Apr 2023 20:06
 Operator : CG/JU
 Sample : 02225-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:50:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/10/2023
 Supervised By :Jagrut Upadhyay 04/10/2023

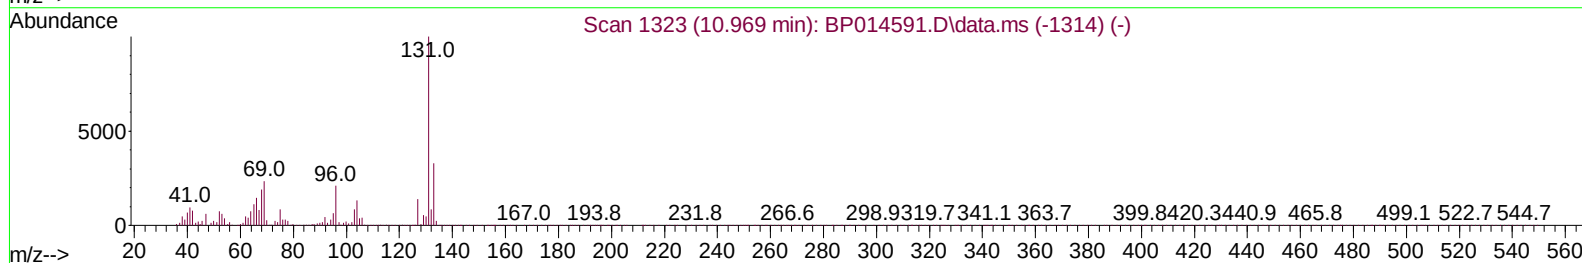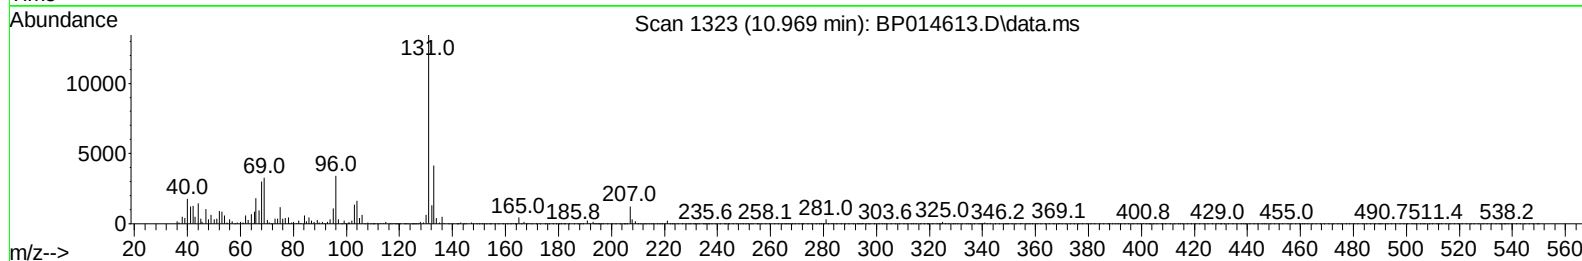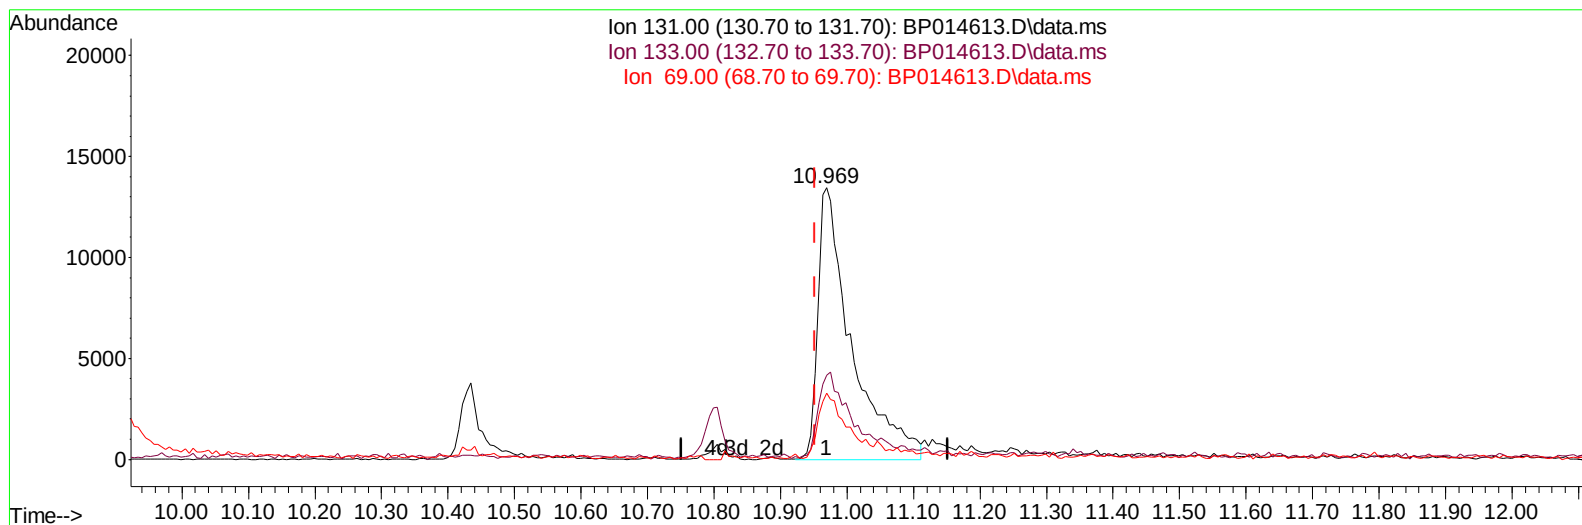

TIC: BP014613.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.018) 3.78 ng/ul m

response 47346

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.91
69.00	21.30	24.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014613.D
Acq On : 07 Apr 2023 20:06
Operator : CG/JU
Sample : 02225-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/10/2023
Supervised By :Jagrut Upadhyay 04/10/2023

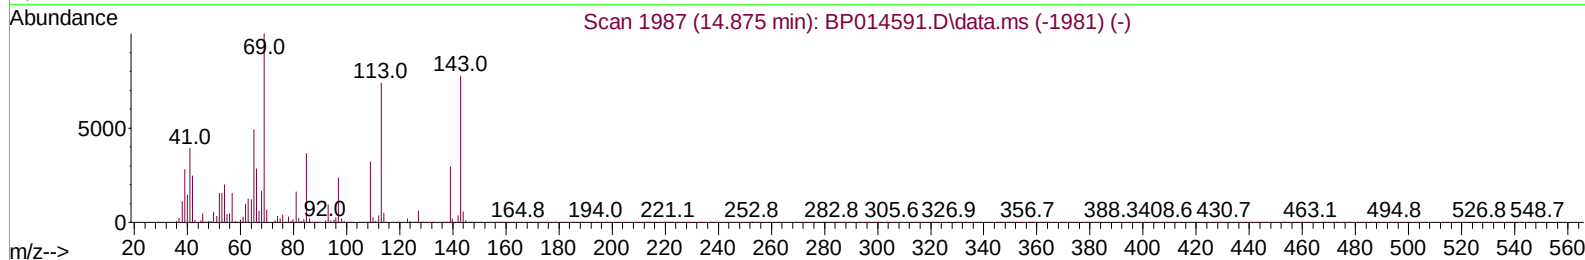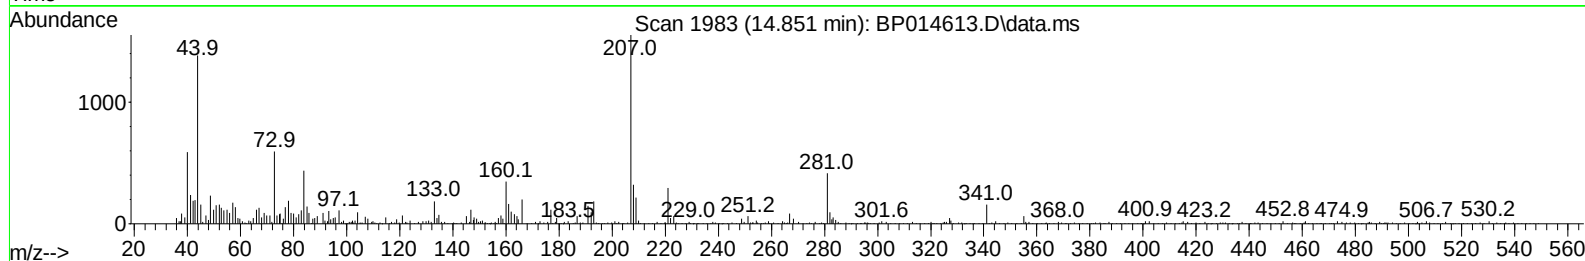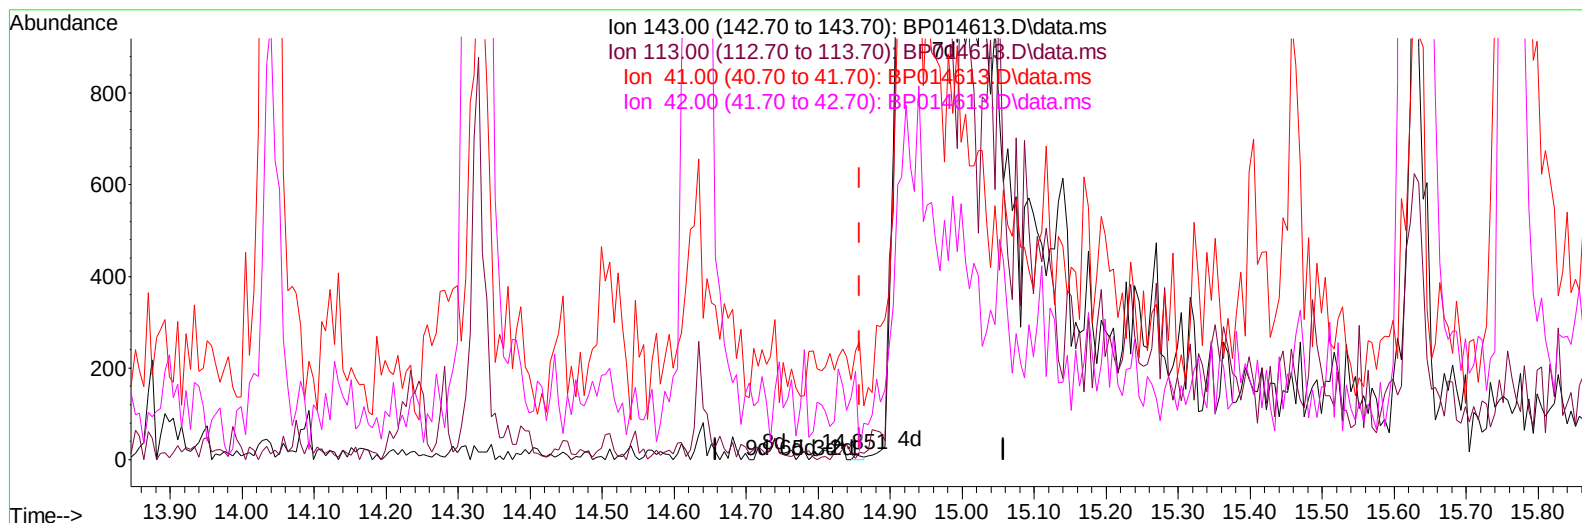

TIC: BP014613.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.851min (-0.006) 0.00 ng/u1

response 8

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	18.18#
41.00	44.20	2154.55#
42.00	31.50	1745.45#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014613.D
Acq On : 07 Apr 2023 20:06
Operator : CG/JU
Sample : 02225-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Quant Time: Apr 08 01:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/10/2023
Supervised By :Jagrut Upadhyay 04/10/2023

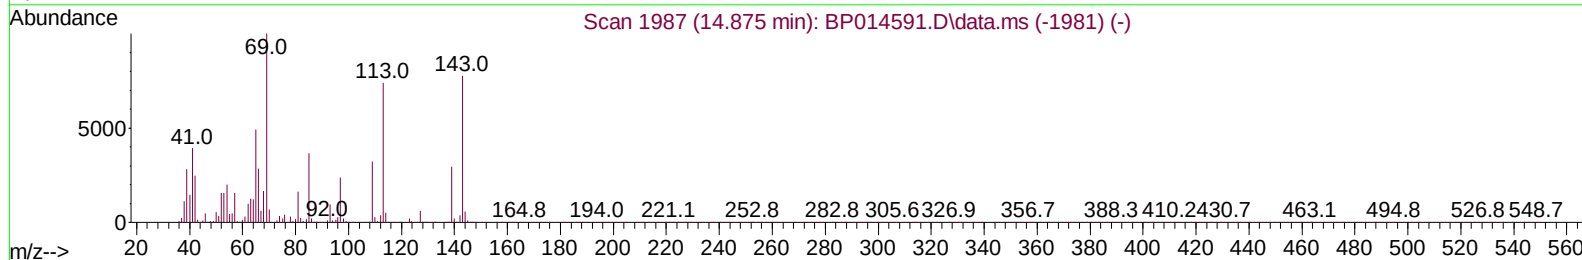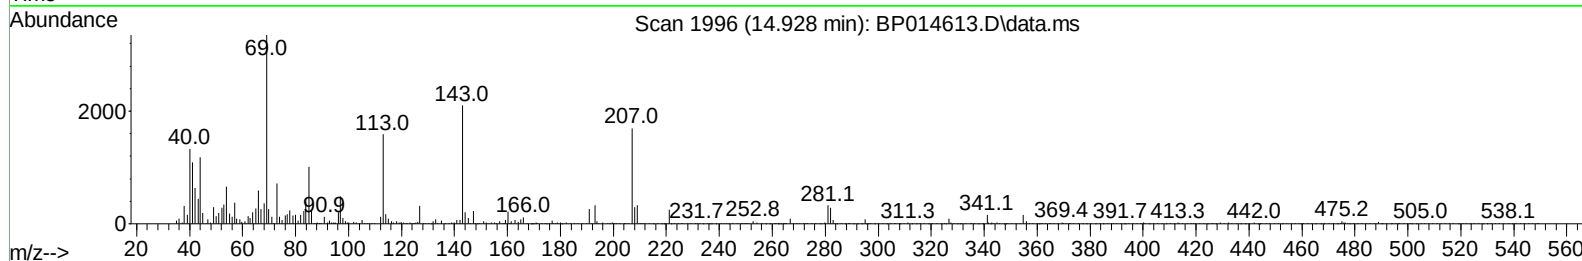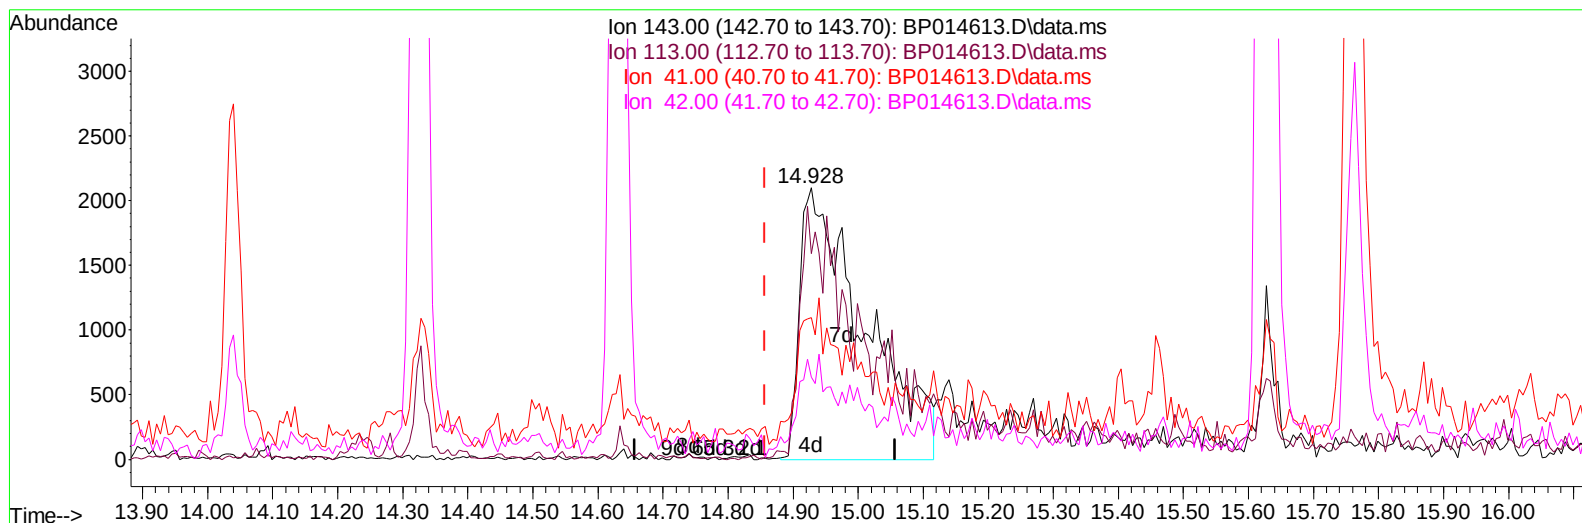

TIC: BP014613.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.928min (+ 0.071) 3.33 ng/ul m

response 14447

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	75.79#
41.00	44.20	52.24
42.00	31.50	30.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
 Data File : BP014613.D
 Acq On : 07 Apr 2023 20:06
 Operator : CG/JU
 Sample : 02225-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/10/2023
 Supervised By :Jagrut Upadhyay 04/10/2023

Quant Time: Apr 08 01:50:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	131562	20.000	ng/ul	0.00
20) Naphthalene-d8	10.799	136	565374	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	354145	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	748340	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	659535	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	775010	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	16972	5.003	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.152	99	56747	4.677	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	248794	31.959	ng/ul	0.00
11) 2-Chlorophenol-d4	7.511	132	197146	22.481	ng/ul	0.00
15) 4-Methylphenol-d8	8.705	113	117219m	11.977	ng/ul	0.00
21) Nitrobenzene-d5	9.158	128	130567	28.607	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	140130	26.812	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	219538	23.065	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	47346m	3.776	ng/ul	0.02
46) Dimethylphthalate-d6	14.040	166	925830	32.242	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	962491	30.208	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	14447m	3.330	ng/ul	0.07
60) Fluorene-d10	15.628	176	776118	32.411	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	142917	25.955	ng/ul	0.00
73) Anthracene-d10	17.492	188	1294622	35.747	ng/ul	0.00
81) Pyrene-d10	19.728	212	1515413	34.207	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.822	264	1484828	36.061	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040723\
Data File : BP014613.D
Acq On : 07 Apr 2023 20:06
Operator : CG/JU
Sample : 02225-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/10/2023
Supervised By :Jagrut Upadhyay 04/10/2023

Quant Time: Apr 08 01:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

